

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033034.D
 Acq On : 20 Nov 2023 20:08
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 20 23:44:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 20 23:40:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	289904	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	291686	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	149029	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	54376	35.874	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	71.740%
7) Chloroethane-d5	1.532	69	46663	40.028	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.060%
11) 1,1-Dichloroethene-d2	2.059	65	20998	33.856	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.720%
21) 2-Butanone-d5	3.780	46	97143	100.730	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.730%
24) Chloroform-d	4.249	84	165115	44.201	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.400%
26) 1,2-Dichloroethane-d4	4.940	65	111838	47.995	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.000%
32) Benzene-d6	4.960	84	289019	42.549	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.100%
36) 1,2-Dichloropropane-d6	5.989	67	89133	46.275	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.540%
41) Toluene-d8	7.246	98	244949	37.776	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	75.560%#
43) trans-1,3-Dichloroprop...	7.554	79	48179	42.845	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.680%
47) 2-Hexanone-d5	8.024	63	80470	100.957	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.960%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	135637	46.261	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.520%
66) 1,2-Dichlorobenzene-d4	11.561	152	128716	48.434	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.860%
Target Compounds						
61) 1,2,3-Trichloropropane	11.188	75	14194	6.602	ug/L	Qvalue # 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033034.D
Acq On : 20 Nov 2023 20:08
Operator : SY/MD
Sample : VIBLK
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 20 23:44:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 20 23:40:05 2023
Response via : Initial Calibration

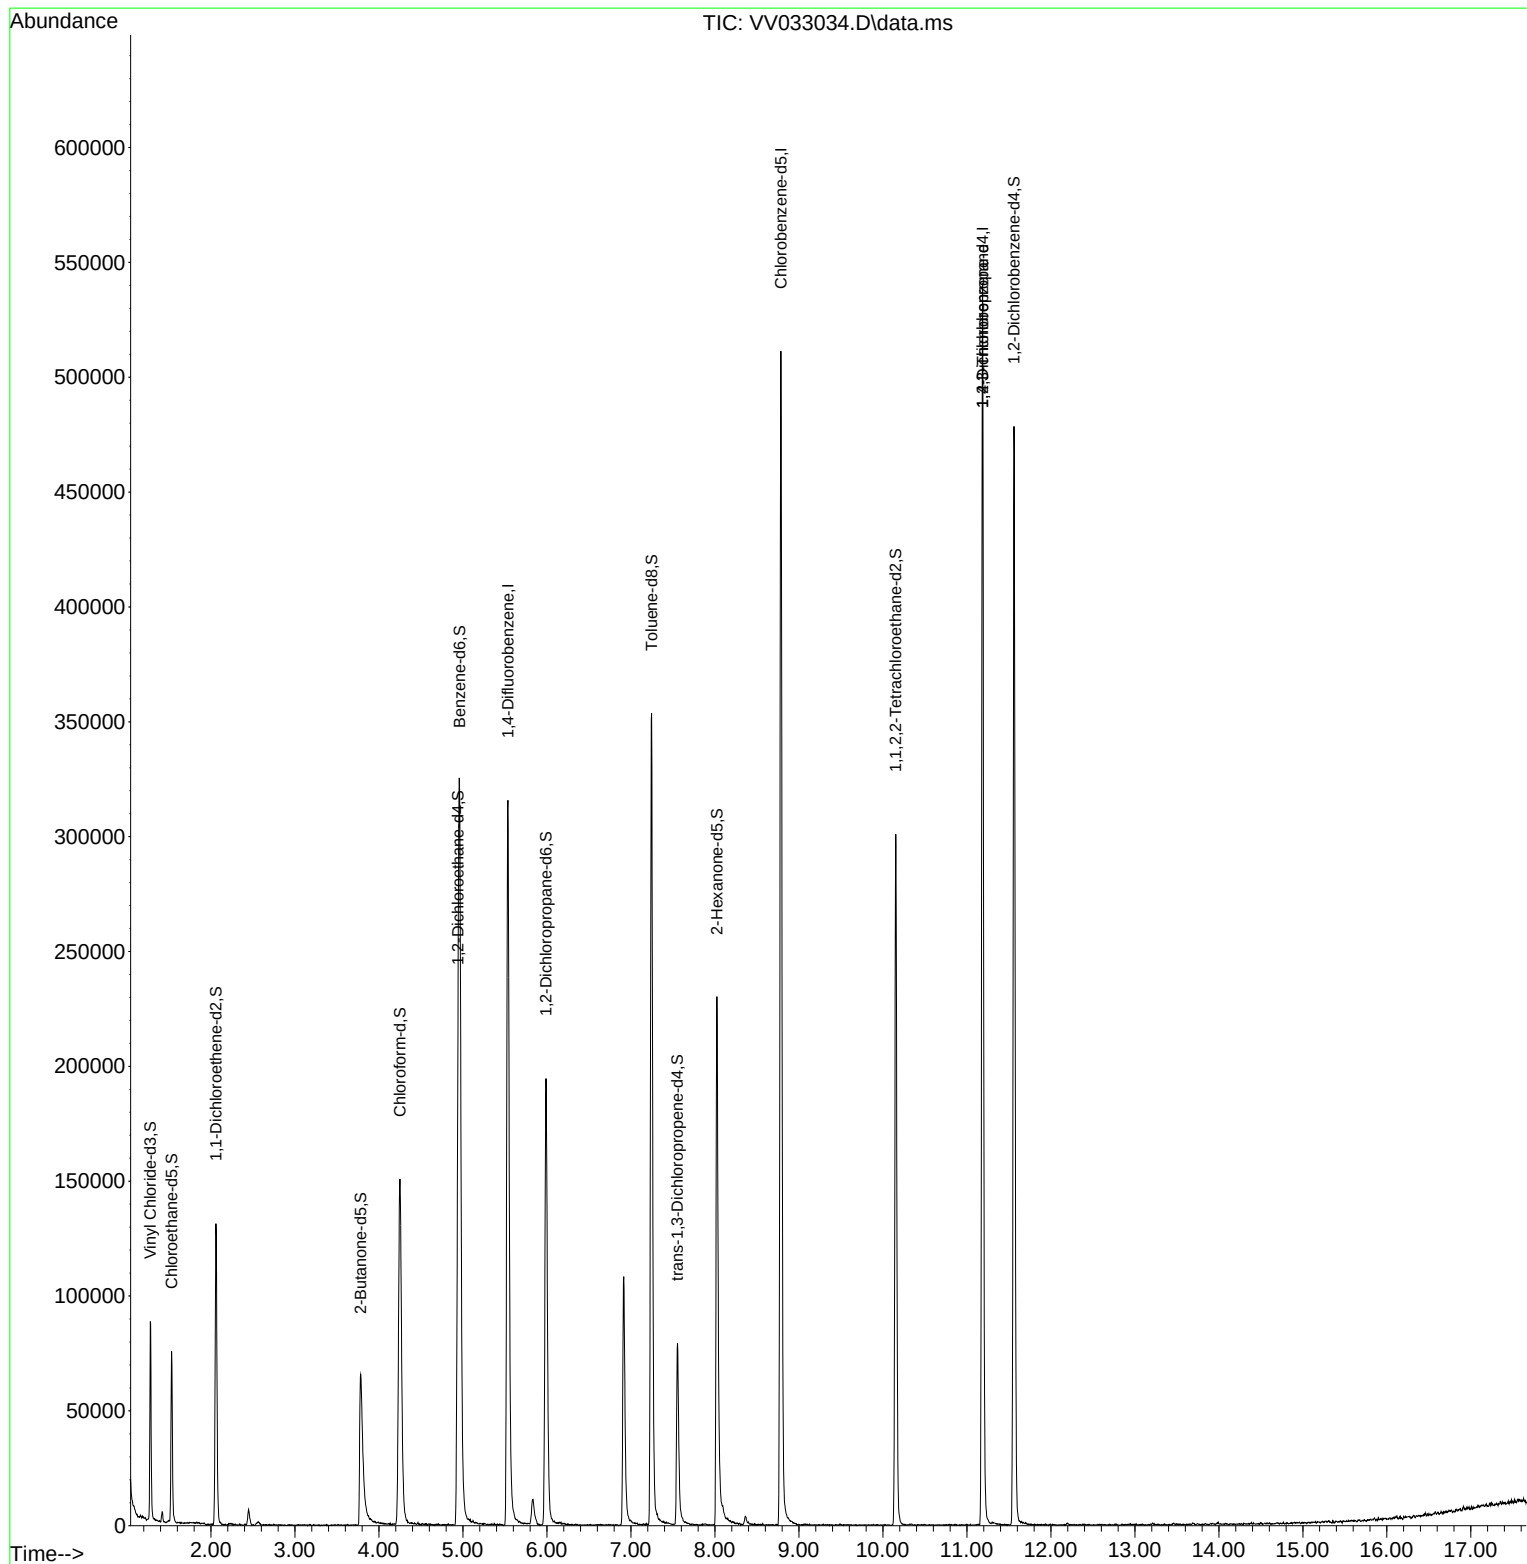

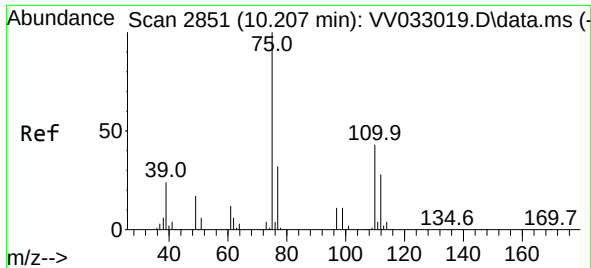

#61
 1,2,3-Trichloropropane
 Concen: 6.602 ug/L
 RT: 11.188 min Scan# 31
 Delta R.T. 0.980 min
 Lab File: VV033034.D
 Acq: 20 Nov 2023 20:08

Instrument :
 MSVOA_V
 ClientSampleId :

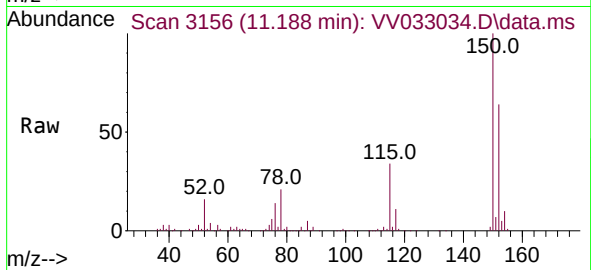

Tgt Ion: 75	Resp:	14194
Ion Ratio	Lower	Upper
75	100	
77	37.3	26.2 39.2
110	3.4	36.2 54.4#

