




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033017.D
Acq On : 20 Nov 2023 11:27
Operator : SY/MD
Sample : VIBLK249
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK249

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/21/2023
Supervised By :Semsettin Yesilyurt 11/21/2023

Quant Time: Nov 20 23:33:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 20 23:27:49 2023
Response via : Initial Calibration

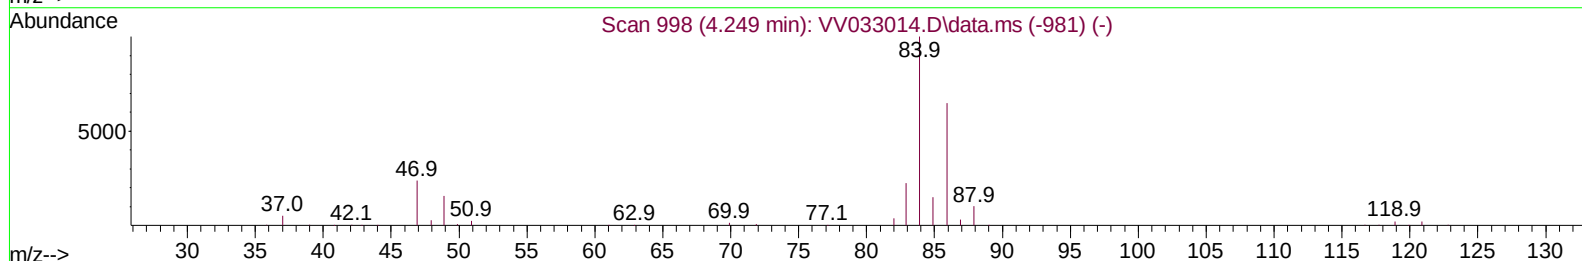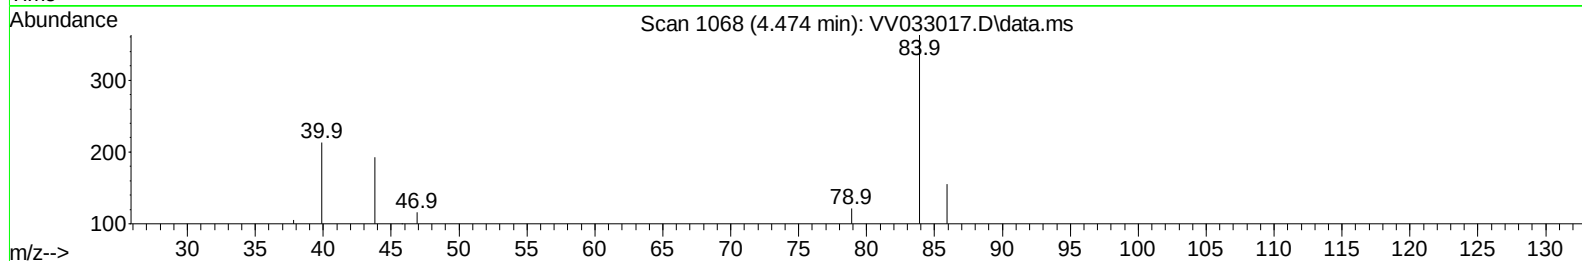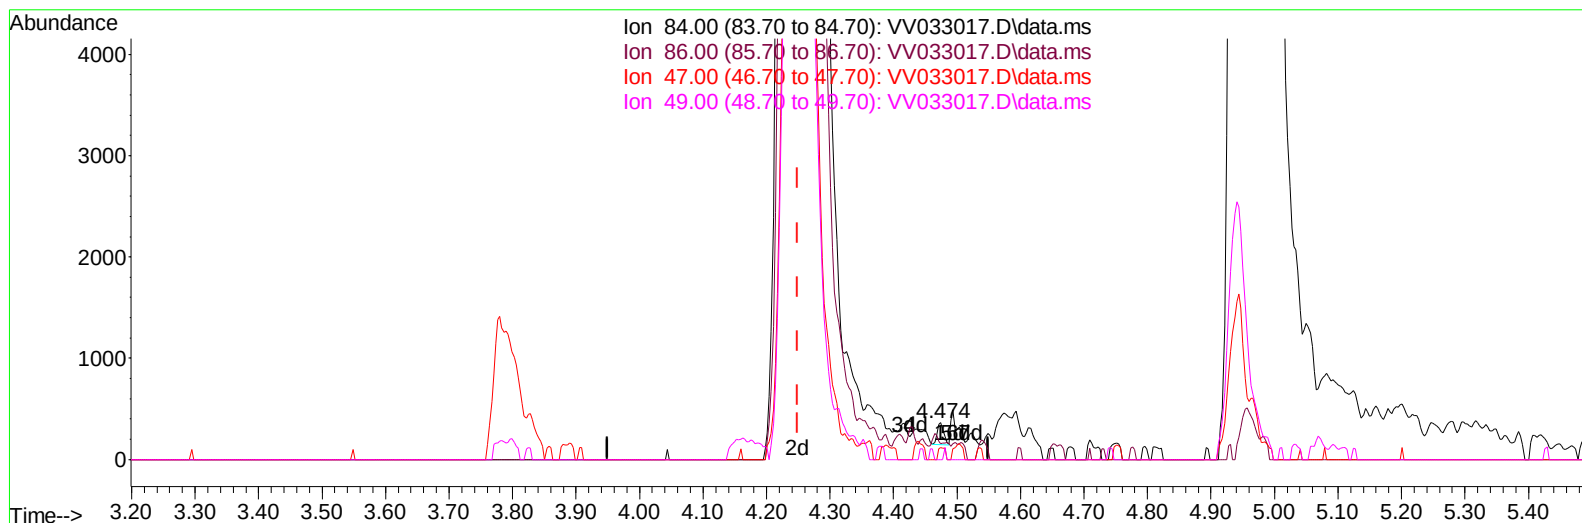

TIC: VV033017.D\data.ms

(24) Chloroform-d (S)

4.474min (+ 0.225) 0.03 ug/L

response 150

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.90	48.67
47.00	40.80	43.33
49.00	24.40	26.67




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033017.D
 Acq On : 20 Nov 2023 11:27
 Operator : SY/MD
 Sample : VIBLK249
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK249

Manual IntegrationsAPPROVED

Quant Time: Nov 20 23:33:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 20 23:27:49 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/21/2023
 Supervised By :Semsettin Yesilyurt 11/21/2023

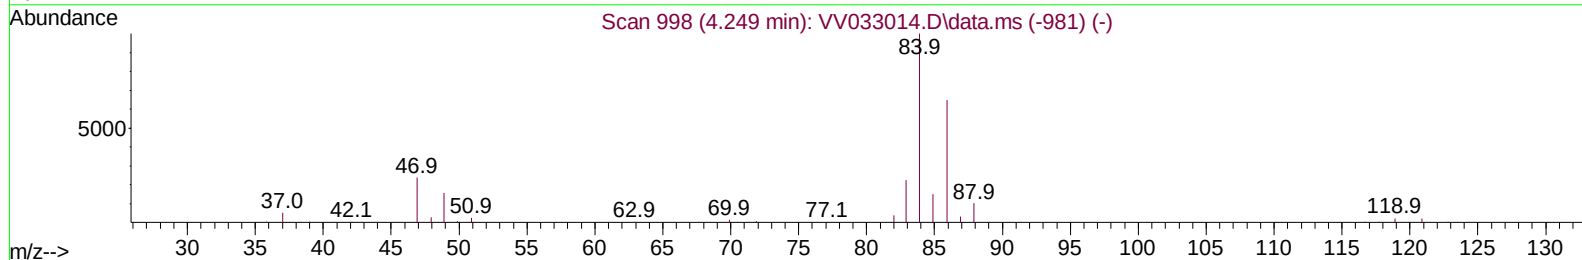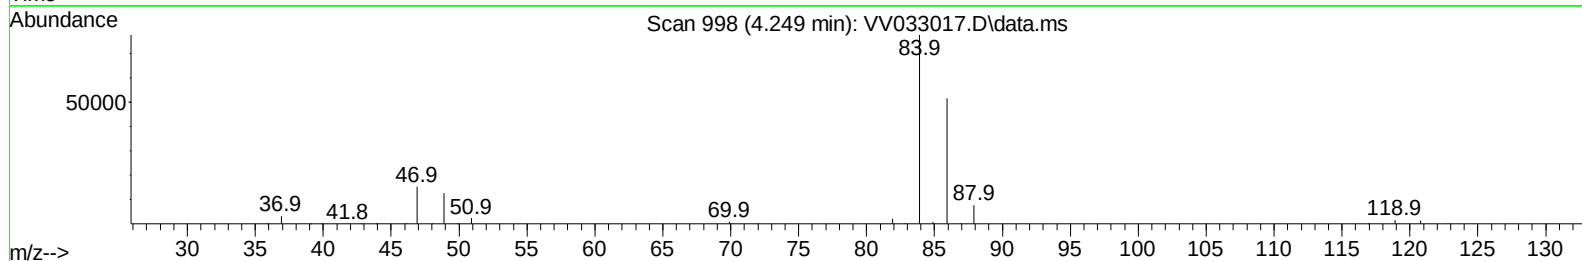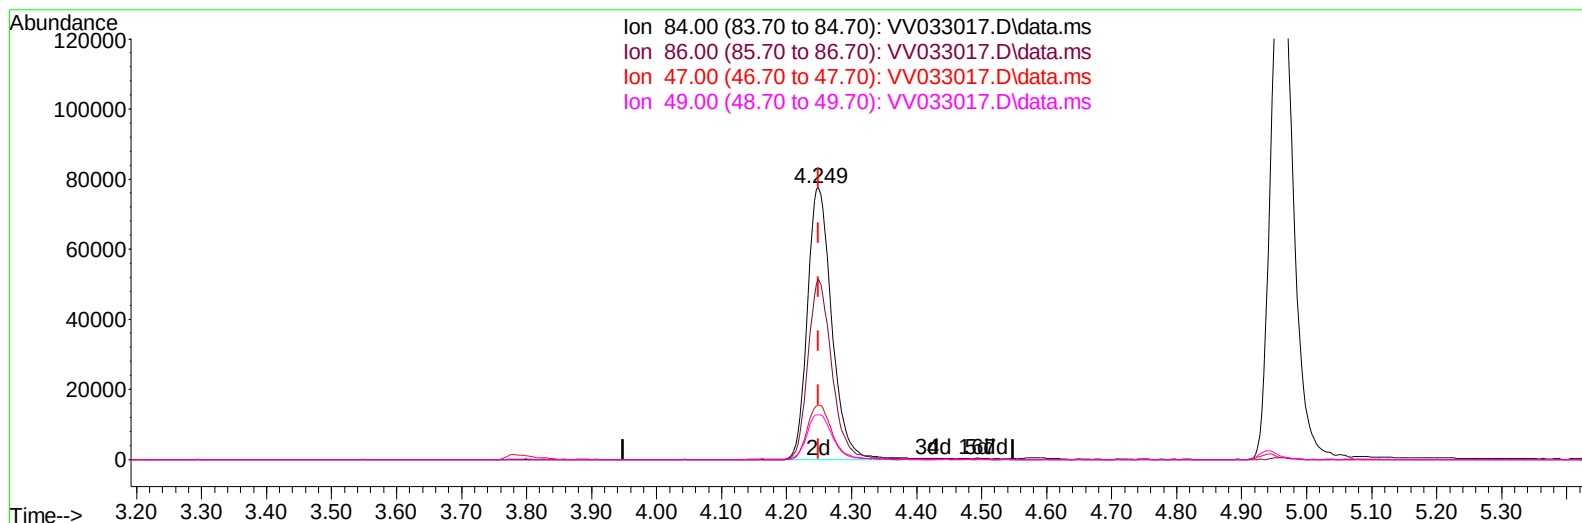

TIC: VV033017.D\data.ms

(24) Chloroform-d (S)

4.249min (+ 0.000) 39.18 ug/L m

response 202274

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.90	0.04#
47.00	40.80	0.03#
49.00	24.40	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033017.D
 Acq On : 20 Nov 2023 11:27
 Operator : SY/MD
 Sample : VIBLK249
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK249

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/21/2023
 Supervised By :Semsettin Yesilyurt 11/21/2023

Quant Time: Nov 20 23:33:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 20 23:27:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	400633	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	396210	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	207893	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	86214	41.158	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	82.320%	
7) Chloroethane-d5	1.532	69	68178	42.320	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	84.640%	
11) 1,1-Dichloroethene-d2	2.060	65	32441	37.849	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	75.700%	
21) 2-Butanone-d5	3.780	46	118570	88.967	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	88.970%	
24) Chloroform-d	4.249	84	202274m	39.183	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	78.360%	
26) 1,2-Dichloroethane-d4	4.941	65	129816	40.313	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	80.620%	
32) Benzene-d6	4.960	84	366143	39.683	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	79.360%	
36) 1,2-Dichloropropane-d6	5.989	67	113039	43.204	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	86.400%	
41) Toluene-d8	7.243	98	316677	35.954	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	71.900%#	
43) trans-1,3-Dichloroprop...	7.555	79	61034	39.958	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	79.920%	
47) 2-Hexanone-d5	8.021	63	94867	87.621	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	87.620%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	159193	39.971	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	79.940%	
66) 1,2-Dichlorobenzene-d4	11.561	152	162295	43.778	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	87.560%	
Target Compounds						
14) Carbon disulfide	2.240	76	11311	1.540	ug/L	98
17) trans-1,2-Dichloroethene	2.700	96	1592	0.563	ug/L	93
64) 1,3-Dichlorobenzene	11.124	146	6787	1.005	ug/L	98
65) 1,4-Dichlorobenzene	11.210	146	8467	1.180	ug/L	93
67) 1,2-Dichlorobenzene	11.580	146	8098	1.195	ug/L #	83
70) 1,2,4-trichlorobenzene	13.201	180	17106	3.556	ug/L	99
72) 1,2,3-Trichlorobenzene	13.683	180	24592	5.272	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033017.D
Acq On : 20 Nov 2023 11:27
Operator : SY/MD
Sample : VIBLK249
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK249

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/21/2023
Supervised By :Semsettin Yesilyurt 11/21/2023

Quant Time: Nov 20 23:33:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 20 23:27:49 2023
Response via : Initial Calibration

