

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033020.D
 Acq On : 20 Nov 2023 14:14
 Operator : SY/MD
 Sample : VV1120MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	151344	157900	12.88%	1.593%
2	1.532	146	153	165	rVB	108763	130046	10.60%	1.312%
3	2.018	301	304	306	rBV3	576	383	0.03%	0.004%
4	2.060	306	317	340	rVV	232615	345342	28.16%	3.484%
5	2.179	351	354	356	rVB2	661	403	0.03%	0.004%
6	2.317	395	397	399	rVB	581	238	0.02%	0.002%
7	2.445	428	437	450	rVB2	7510	13088	1.07%	0.132%
8	2.539	463	466	467	rBV	573	307	0.03%	0.003%
9	2.587	479	481	483	rBV2	478	212	0.02%	0.002%
10	2.696	508	515	523	rVB5	1543	2436	0.20%	0.025%
11	2.876	568	571	574	rVB3	479	279	0.02%	0.003%
12	2.947	590	593	596	rVB2	403	274	0.02%	0.003%
13	2.992	604	607	609	rBV2	355	231	0.02%	0.002%
14	3.076	629	633	634	rBV	359	233	0.02%	0.002%
15	3.121	643	647	650	rVB2	508	394	0.03%	0.004%
16	3.140	650	653	656	rVV2	453	249	0.02%	0.003%
17	3.182	661	666	670	rBV3	402	328	0.03%	0.003%
18	3.214	674	676	680	rBV	358	206	0.02%	0.002%
19	3.236	681	683	687	rVB3	550	317	0.03%	0.003%
20	3.259	687	690	693	rBV3	439	369	0.03%	0.004%
21	3.304	700	704	705	rBV2	385	201	0.02%	0.002%
22	3.346	715	717	720	rVV	321	216	0.02%	0.002%
23	3.545	777	779	784	rVB2	322	195	0.02%	0.002%
24	3.664	811	816	818	rBV3	486	434	0.04%	0.004%
25	3.777	841	851	877	rBV	74295	200488	16.35%	2.023%
26	4.246	982	997	1025	rBV2	194725	502199	40.95%	5.066%
27	4.699	1136	1138	1141	rVV3	366	246	0.02%	0.002%
28	4.719	1141	1144	1146	rVV4	723	408	0.03%	0.004%
29	4.741	1149	1151	1158	rVB3	641	663	0.05%	0.007%
30	4.777	1158	1162	1164	rBV2	478	347	0.03%	0.004%
31	4.850	1182	1185	1188	rBV3	644	357	0.03%	0.004%
32	4.870	1189	1191	1196	rBV4	365	208	0.02%	0.002%
33	4.953	1199	1217	1243	rBV2	461640	1226397	100.00%	12.372%
34	5.432	1363	1366	1370	rBV4	461	403	0.03%	0.004%
35	5.529	1385	1396	1424	rBV	416680	852151	69.48%	8.597%
36	5.825	1478	1488	1501	rBV4	11197	24801	2.02%	0.250%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033020.D
 Acq On : 20 Nov 2023 14:14
 Operator : SY/MD
 Sample : VV1120MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	5.985	1524	1538	1565	rBV	260079	543544	44.32%	5.483%
38	6.291	1631	1633	1635	rBV2	519	304	0.02%	0.003%
39	6.326	1641	1644	1646	rBV2	554	302	0.02%	0.003%
40	6.490	1693	1695	1697	rVB	546	236	0.02%	0.002%
41	6.567	1717	1719	1721	rBV	336	208	0.02%	0.002%
42	6.616	1732	1734	1739	rBV4	356	297	0.02%	0.003%
43	6.657	1745	1747	1750	rBV2	394	223	0.02%	0.002%
44	6.680	1753	1754	1757	rVB	492	217	0.02%	0.002%
45	6.911	1815	1826	1858	rBV	151689	290293	23.67%	2.929%
46	7.243	1917	1929	1949	rBV	570455	1004724	81.92%	10.136%
47	7.551	2016	2025	2047	rBV	108218	192947	15.73%	1.947%
48	7.786	2094	2098	2101	rBV4	488	377	0.03%	0.004%
49	7.863	2120	2122	2125	rBV2	323	233	0.02%	0.002%
50	8.021	2162	2171	2208	rBV	259121	477461	38.93%	4.817%
51	8.365	2268	2278	2286	rBV8	2720	4836	0.39%	0.049%
52	8.622	2355	2358	2360	rVB2	629	308	0.03%	0.003%
53	8.783	2397	2408	2447	rBV	642883	1061565	86.56%	10.710%
54	9.201	2536	2538	2541	rBV2	360	208	0.02%	0.002%
55	9.329	2575	2578	2581	rBV2	401	265	0.02%	0.003%
56	9.407	2600	2602	2606	rBV2	275	227	0.02%	0.002%
57	9.622	2667	2669	2673	rVB2	443	261	0.02%	0.003%
58	9.644	2673	2676	2678	rBV2	351	271	0.02%	0.003%
59	9.876	2742	2748	2755	rVB4	1474	1653	0.13%	0.017%
60	9.960	2771	2774	2775	rBV	534	206	0.02%	0.002%
61	10.005	2785	2788	2791	rVB2	420	212	0.02%	0.002%
62	10.091	2812	2815	2819	rVB2	452	303	0.02%	0.003%
63	10.153	2819	2834	2851	rBV	342920	549967	44.84%	5.548%
64	10.281	2869	2874	2875	rBV3	459	328	0.03%	0.003%
65	10.326	2881	2888	2893	rBV3	1224	1516	0.12%	0.015%
66	10.484	2929	2937	2939	rBV3	1428	1807	0.15%	0.018%
67	10.670	2991	2995	2999	rBV2	464	391	0.03%	0.004%
68	10.731	3012	3014	3015	rBV	441	235	0.02%	0.002%
69	10.783	3027	3030	3034	rVB3	810	505	0.04%	0.005%
70	10.860	3046	3054	3066	rVB3	2420	3516	0.29%	0.035%
71	11.053	3110	3114	3116	rBV2	315	238	0.02%	0.002%
72	11.127	3130	3137	3144	rBV3	4129	6245	0.51%	0.063%
73	11.185	3144	3155	3183	rVV	717407	1123057	91.57%	11.330%
74	11.406	3223	3224	3228	rBV3	545	307	0.03%	0.003%
75	11.452	3236	3238	3241	rVB	590	337	0.03%	0.003%
76	11.480	3244	3247	3251	rBV2	355	253	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033020.D
 Acq On : 20 Nov 2023 14:14
 Operator : SY/MD
 Sample : VV1120MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	11.519	3256	3259	3260	rBV2	489	197	0.02%	0.002%
78	11.561	3260	3272	3297	rBV	666835	1035384	84.42%	10.445%
79	11.792	3342	3344	3349	rVB2	555	470	0.04%	0.005%
80	11.898	3373	3377	3379	rBV	392	280	0.02%	0.003%
81	11.940	3389	3390	3392	rBV	462	237	0.02%	0.002%
82	11.995	3404	3407	3409	rBV2	402	285	0.02%	0.003%
83	12.021	3413	3415	3418	rBV2	277	197	0.02%	0.002%
84	12.062	3426	3428	3433	rBV2	267	234	0.02%	0.002%
85	12.185	3461	3466	3467	rBV2	1138	797	0.06%	0.008%
86	12.300	3500	3502	3508	rBV	315	347	0.03%	0.004%
87	12.371	3517	3524	3530	rBV3	1501	1815	0.15%	0.018%
88	12.477	3553	3557	3558	rBV2	469	351	0.03%	0.004%
89	12.554	3578	3581	3583	rBV	279	201	0.02%	0.002%
90	12.590	3583	3592	3601	rVV5	6936	11378	0.93%	0.115%
91	12.731	3633	3636	3641	rBV3	375	324	0.03%	0.003%
92	13.162	3766	3770	3774	rBV4	558	537	0.04%	0.005%
93	13.204	3774	3783	3793	rVV3	15895	24051	1.96%	0.243%
94	13.445	3848	3858	3872	rBV	43846	70603	5.76%	0.712%
95	13.683	3924	3932	3943	rBV3	19496	28857	2.35%	0.291%
96	13.895	3995	3998	4002	rVB3	624	500	0.04%	0.005%
97	13.924	4004	4007	4009	rBV2	825	506	0.04%	0.005%
98	14.066	4049	4051	4054	rBV2	575	282	0.02%	0.003%
99	14.287	4117	4120	4123	rBV4	815	690	0.06%	0.007%
100	14.519	4190	4192	4196	rBV3	825	502	0.04%	0.005%




Sum of corrected areas: 9912357

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033020.D
Acq On : 20 Nov 2023 14:14
Operator : SY/MD
Sample : VV1120MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

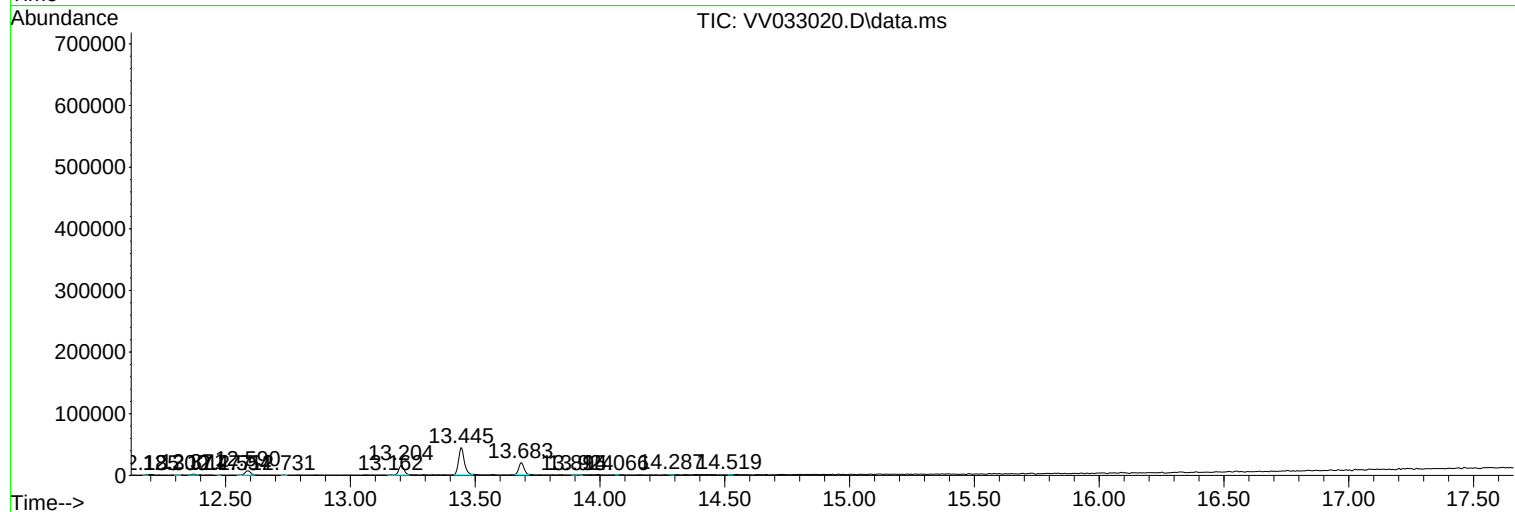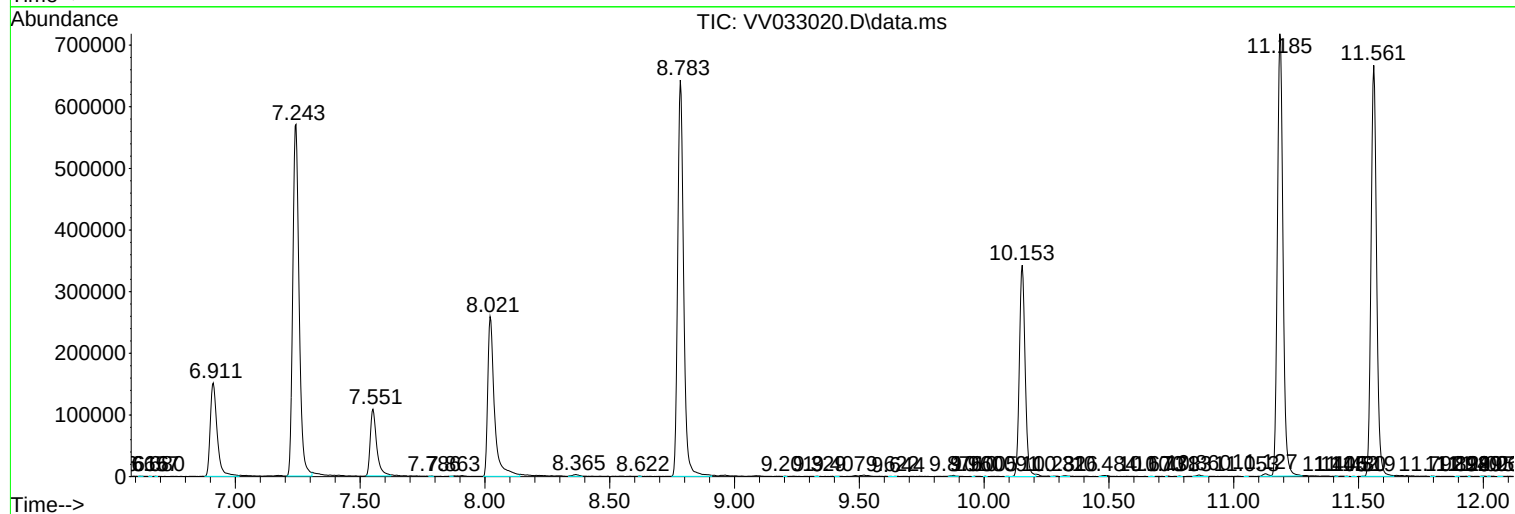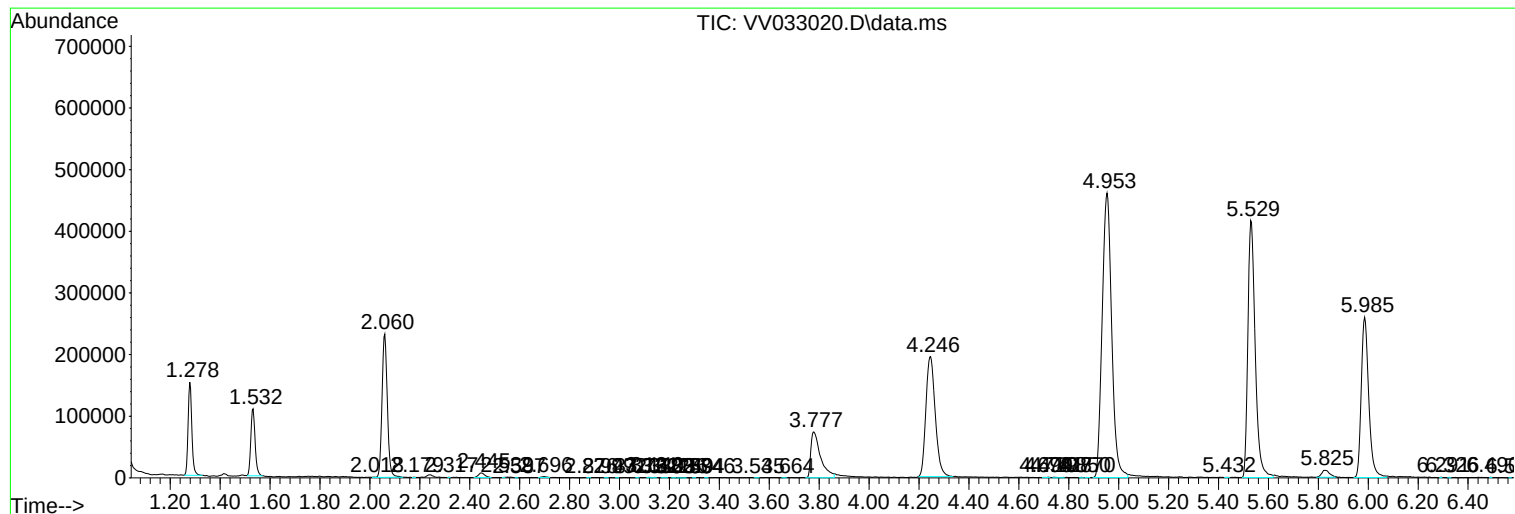

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033020.D
Acq On : 20 Nov 2023 14:14
Operator : SY/MD
Sample : VV1120MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033020.D
Acq On : 20 Nov 2023 14:14
Operator : SY/MD
Sample : VV1120MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc