

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033025.D
 Acq On : 20 Nov 2023 16:39
 Operator : SY/MD
 Sample : 05436-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1C2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033025.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	101203	109202	12.33%	1.395%
2	1.532	146	153	166	rVB	77486	90603	10.23%	1.157%
3	1.970	286	289	290	rBV2	307	133	0.02%	0.002%
4	2.002	297	299	300	rBV	390	152	0.02%	0.002%
5	2.060	307	317	332	rBV	153218	223005	25.18%	2.849%
6	2.207	361	363	364	rBV	370	186	0.02%	0.002%
7	2.497	451	453	455	rBV	317	157	0.02%	0.002%
8	2.535	463	465	468	rVB2	256	148	0.02%	0.002%
9	2.564	472	474	477	rVV	338	173	0.02%	0.002%
10	2.651	499	501	503	rVB2	346	151	0.02%	0.002%
11	2.661	503	504	505	rBV2	219	68	0.01%	0.001%
12	2.699	513	516	521	rBV2	502	370	0.04%	0.005%
13	2.722	521	523	529	rVB2	471	282	0.03%	0.004%
14	2.802	545	548	550	rBV2	197	139	0.02%	0.002%
15	2.870	566	569	571	rBV	230	127	0.01%	0.002%
16	2.928	585	587	589	rVB	251	95	0.01%	0.001%
17	2.947	589	593	597	rBV2	502	481	0.05%	0.006%
18	2.998	606	609	610	rBV	361	174	0.02%	0.002%
19	3.040	617	622	624	rBV	250	197	0.02%	0.003%
20	3.191	666	669	672	rBV3	333	244	0.03%	0.003%
21	3.223	677	679	680	rBV3	148	48	0.01%	0.001%
22	3.256	686	689	693	rBV2	315	248	0.03%	0.003%
23	3.362	719	722	724	rBV	373	267	0.03%	0.003%
24	3.407	734	736	738	rVB	279	78	0.01%	0.001%
25	3.458	750	752	755	rVB	227	75	0.01%	0.001%
26	3.474	755	757	760	rBV	250	178	0.02%	0.002%
27	3.622	800	803	808	rBV2	366	229	0.03%	0.003%
28	3.690	822	824	825	rBV2	287	102	0.01%	0.001%
29	3.783	845	853	880	rBV	57095	153781	17.36%	1.964%
30	4.249	983	998	1025	rBV	147499	381224	43.05%	4.870%
31	4.603	1106	1108	1111	rBV2	484	270	0.03%	0.003%
32	4.825	1175	1177	1179	rBV	242	60	0.01%	0.001%
33	4.841	1179	1182	1183	rBV2	433	211	0.02%	0.003%
34	4.892	1195	1198	1199	rBV	515	324	0.04%	0.004%
35	4.957	1202	1218	1250	rVV2	325188	877557	99.09%	11.210%
36	5.297	1322	1324	1327	rBV3	685	310	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033025.D
 Acq On : 20 Nov 2023 16:39
 Operator : SY/MD
 Sample : 05436-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1C2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	5.465	1374	1376	1377	rBV2	334	158	0.02%	0.002%
38	5.535	1387	1398	1427	rBV	273278	564448	63.74%	7.211%
39	5.831	1478	1490	1521	rBV	441361	885588	100.00%	11.313%
40	5.989	1528	1539	1568	rVB	191074	393491	44.43%	5.027%
41	6.233	1613	1615	1619	rBV3	679	310	0.04%	0.004%
42	6.587	1722	1725	1726	rBV	271	163	0.02%	0.002%
43	6.596	1726	1728	1730	rVV2	466	207	0.02%	0.003%
44	6.815	1794	1796	1804	rVB2	390	376	0.04%	0.005%
45	6.857	1804	1809	1813	rBV	394	382	0.04%	0.005%
46	6.915	1816	1827	1848	rBV	110590	205829	23.24%	2.629%
47	7.243	1918	1929	1953	rBV	372693	664722	75.06%	8.492%
48	7.554	2014	2026	2046	rBV	80563	143935	16.25%	1.839%
49	7.876	2114	2126	2139	rBV3	9096	17191	1.94%	0.220%
50	8.024	2162	2172	2197	rBV	205725	372487	42.06%	4.758%
51	8.548	2333	2335	2336	rBV	238	82	0.01%	0.001%
52	8.619	2354	2357	2363	rVB3	409	271	0.03%	0.003%
53	8.670	2368	2373	2376	rBV3	700	553	0.06%	0.007%
54	8.731	2390	2392	2397	rVB2	438	299	0.03%	0.004%
55	8.786	2397	2409	2435	rBV	436859	726515	82.04%	9.281%
56	9.053	2490	2492	2495	rBV	376	237	0.03%	0.003%
57	9.172	2527	2529	2531	rBV	464	177	0.02%	0.002%
58	9.265	2556	2558	2561	rVB2	424	220	0.02%	0.003%
59	9.294	2561	2567	2568	rBV	591	473	0.05%	0.006%
60	9.484	2620	2626	2627	rBV3	767	679	0.08%	0.009%
61	9.657	2677	2680	2681	rBV	274	147	0.02%	0.002%
62	9.725	2699	2701	2703	rVB	484	155	0.02%	0.002%
63	9.985	2777	2782	2784	rBV	377	284	0.03%	0.004%
64	10.098	2815	2817	2818	rBV	294	146	0.02%	0.002%
65	10.152	2823	2834	2852	rBV	289324	455582	51.44%	5.820%
66	10.329	2879	2889	2898	rVB3	9924	15475	1.75%	0.198%
67	10.423	2916	2918	2921	rBV2	435	245	0.03%	0.003%
68	10.455	2926	2928	2931	rBV	253	154	0.02%	0.002%
69	10.660	2990	2992	2995	rBV	308	161	0.02%	0.002%
70	10.722	3008	3011	3013	rBV	233	181	0.02%	0.002%
71	10.831	3044	3045	3049	rVB	466	168	0.02%	0.002%
72	10.860	3051	3054	3062	rVB3	1440	1686	0.19%	0.022%
73	11.021	3103	3104	3110	rBV2	499	341	0.04%	0.004%
74	11.107	3129	3131	3132	rBV2	463	163	0.02%	0.002%
75	11.188	3144	3156	3181	rBV	483381	752007	84.92%	9.607%
76	11.522	3254	3260	3261	rBV2	838	852	0.10%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033025.D
 Acq On : 20 Nov 2023 16:39
 Operator : SY/MD
 Sample : 05436-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1C2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	11.561	3261	3272	3293	rVV	495466	769417	86.88%	9.829%
78	11.760	3331	3334	3335	rBV	410	237	0.03%	0.003%
79	11.886	3370	3373	3375	rBV	614	342	0.04%	0.004%
80	11.918	3381	3383	3385	rBV	359	180	0.02%	0.002%
81	11.943	3389	3391	3395	rVV	374	240	0.03%	0.003%
82	11.992	3402	3406	3413	rBV2	547	700	0.08%	0.009%
83	12.040	3419	3421	3429	rVB2	367	352	0.04%	0.004%
84	12.152	3454	3456	3459	rVB	387	169	0.02%	0.002%
85	12.236	3480	3482	3483	rBV	315	136	0.02%	0.002%
86	12.384	3525	3528	3531	rVB2	549	334	0.04%	0.004%
87	12.448	3545	3548	3551	rBV2	353	164	0.02%	0.002%
88	12.786	3651	3653	3657	rBV2	307	272	0.03%	0.003%
89	13.017	3723	3725	3726	rBV	352	130	0.01%	0.002%
90	13.178	3771	3775	3777	rBV	460	376	0.04%	0.005%
91	13.210	3777	3785	3790	rVV5	1491	2095	0.24%	0.027%
92	13.258	3797	3800	3802	rBV2	427	210	0.02%	0.003%
93	13.451	3855	3860	3869	rVB3	2845	3692	0.42%	0.047%
94	13.580	3898	3900	3902	rBV2	416	266	0.03%	0.003%
95	13.619	3910	3912	3913	rBV	303	154	0.02%	0.002%
96	13.760	3954	3956	3957	rBV	479	129	0.01%	0.002%
97	13.905	3999	4001	4011	rVB4	531	727	0.08%	0.009%
98	14.049	4044	4046	4047	rBV	355	105	0.01%	0.001%




Sum of corrected areas: 7828016

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033025.D
Acq On : 20 Nov 2023 16:39
Operator : SY/MD
Sample : 05436-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1C2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

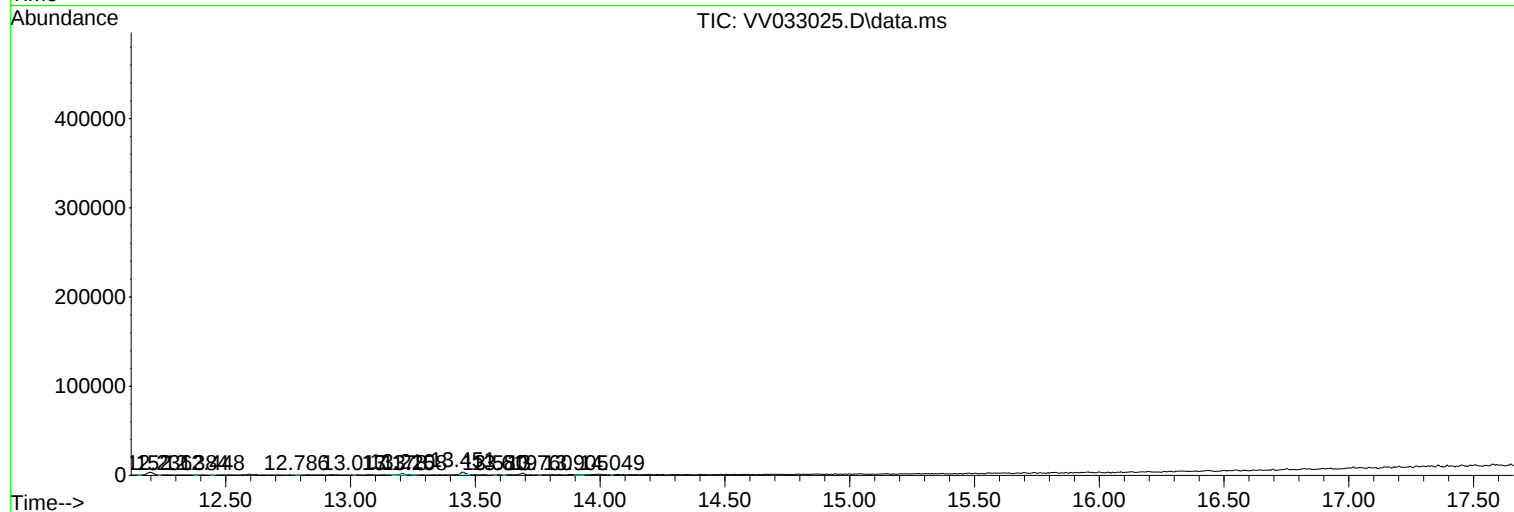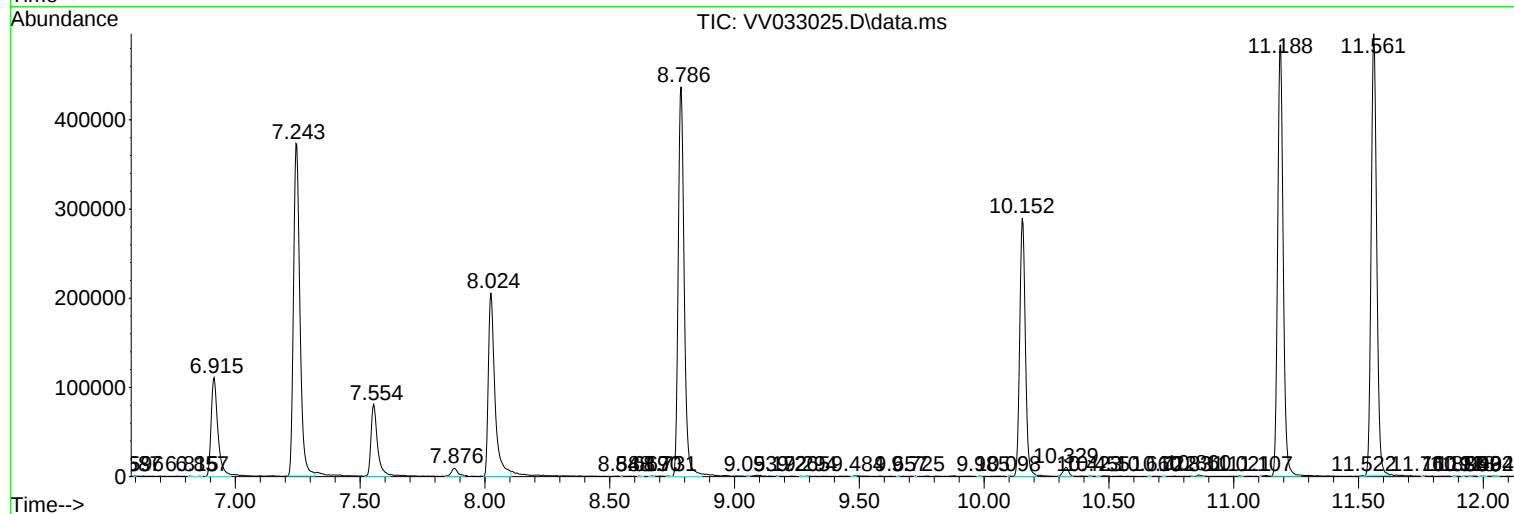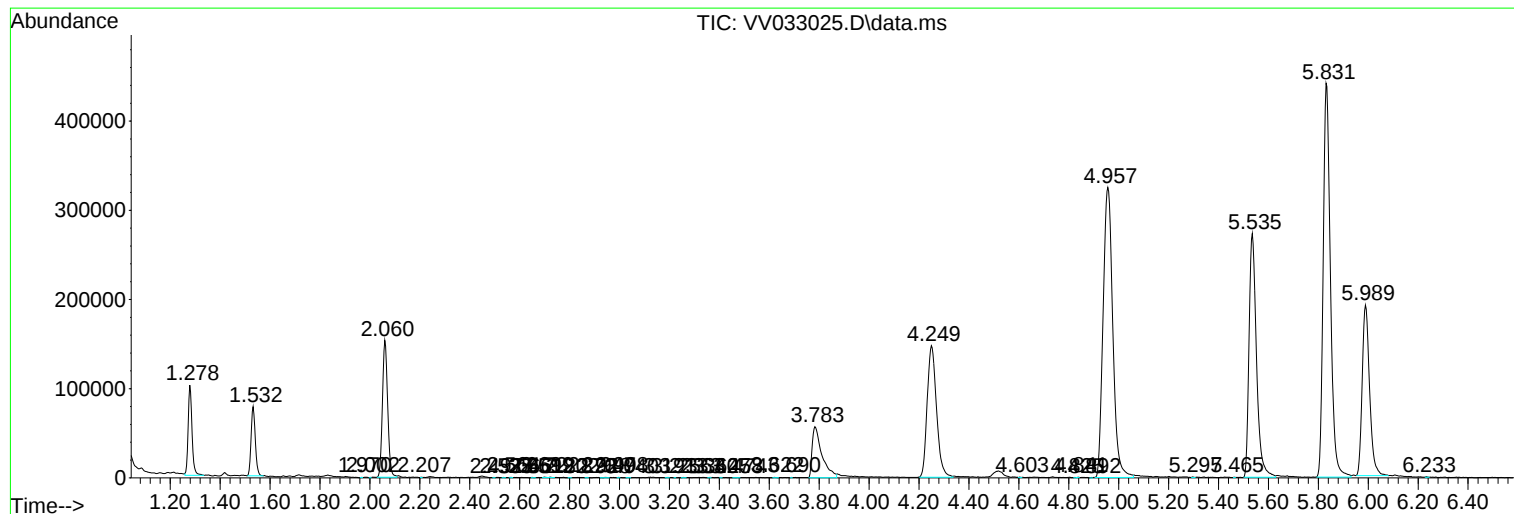

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033025.D
Acq On : 20 Nov 2023 16:39
Operator : SY/MD
Sample : 05436-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1C2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033025.D
Acq On : 20 Nov 2023 16:39
Operator : SY/MD
Sample : 05436-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1C2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc