

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033029.D
 Acq On : 20 Nov 2023 18:12
 Operator : SY/MD
 Sample : VIBLK252
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK252

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033029.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	99188	103075	12.26%	1.478%
2	1.532	146	153	174	rVB	76747	92902	11.05%	1.332%
3	2.060	307	317	340	rBV	146345	214933	25.56%	3.083%
4	2.191	355	358	361	rVB2	543	319	0.04%	0.005%
5	2.214	363	365	367	rBV3	370	197	0.02%	0.003%
6	2.449	431	438	448	rVB4	3418	6037	0.72%	0.087%
7	2.490	448	451	455	rVB2	322	212	0.03%	0.003%
8	2.526	460	462	463	rBV	427	182	0.02%	0.003%
9	2.536	463	465	467	rBV3	326	184	0.02%	0.003%
10	2.632	492	495	497	rBV2	380	191	0.02%	0.003%
11	2.687	509	512	515	rBV2	311	179	0.02%	0.003%
12	2.841	556	560	563	rBV2	342	267	0.03%	0.004%
13	2.870	568	569	573	rBV2	260	174	0.02%	0.002%
14	2.960	592	597	599	rBV2	228	203	0.02%	0.003%
15	2.982	600	604	607	rBV2	382	278	0.03%	0.004%
16	3.047	619	624	628	rVV2	306	397	0.05%	0.006%
17	3.105	638	642	643	rBV2	447	197	0.02%	0.003%
18	3.169	658	662	666	rBV2	348	259	0.03%	0.004%
19	3.188	666	668	672	rVB2	388	201	0.02%	0.003%
20	3.224	677	679	682	rBV2	308	199	0.02%	0.003%
21	3.307	703	705	709	rVB	321	210	0.02%	0.003%
22	3.352	717	719	723	rVB	339	223	0.03%	0.003%
23	3.429	741	743	745	rBV2	397	186	0.02%	0.003%
24	3.535	773	776	780	rVV2	284	231	0.03%	0.003%
25	3.600	790	796	798	rBV	375	295	0.04%	0.004%
26	3.619	798	802	803	rBV	285	167	0.02%	0.002%
27	3.674	814	819	821	rBV2	204	185	0.02%	0.003%
28	3.783	843	853	887	rBV	58554	163078	19.39%	2.339%
29	4.249	983	998	1030	rBV	138985	362571	43.11%	5.200%
30	4.433	1052	1055	1060	rBV2	952	725	0.09%	0.010%
31	4.593	1102	1105	1106	rBV	367	186	0.02%	0.003%
32	4.632	1113	1117	1118	rBV2	491	277	0.03%	0.004%
33	4.767	1155	1159	1163	rVV2	489	302	0.04%	0.004%
34	4.825	1172	1177	1182	rBV2	351	355	0.04%	0.005%
35	4.957	1199	1218	1251	rBV3	313540	840298	99.91%	12.052%
36	5.407	1356	1358	1363	rVB2	548	374	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033029.D
 Acq On : 20 Nov 2023 18:12
 Operator : SY/MD
 Sample : VIBLK252
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK252

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	5.535	1387	1398	1424	rBV	308090	629486	74.85%	9.029%
38	5.831	1479	1490	1504	rBV9	9176	19713	2.34%	0.283%
39	5.924	1516	1519	1522	rVB	410	208	0.02%	0.003%
40	5.989	1525	1539	1563	rBV	185625	382064	45.43%	5.480%
41	6.137	1581	1585	1591	rBV5	912	925	0.11%	0.013%
42	6.294	1632	1634	1636	rBV2	647	292	0.03%	0.004%
43	6.613	1728	1733	1734	rBV2	242	211	0.03%	0.003%
44	6.786	1785	1787	1794	rBV2	295	328	0.04%	0.005%
45	6.915	1816	1827	1852	rBV	104046	194106	23.08%	2.784%
46	7.246	1918	1930	1952	rBV	356737	630803	75.00%	9.048%
47	7.555	2017	2026	2046	rBV	74979	132045	15.70%	1.894%
48	7.709	2072	2074	2076	rVB2	534	247	0.03%	0.004%
49	7.754	2085	2088	2091	rBV3	406	294	0.03%	0.004%
50	7.812	2103	2106	2108	rBV2	346	226	0.03%	0.003%
51	7.870	2119	2124	2126	rBV2	433	416	0.05%	0.006%
52	7.931	2141	2143	2150	rVB3	589	517	0.06%	0.007%
53	7.963	2150	2153	2154	rBV	276	179	0.02%	0.003%
54	8.024	2163	2172	2197	rBV	200908	363720	43.25%	5.217%
55	8.577	2341	2344	2348	rBV2	239	253	0.03%	0.004%
56	8.619	2355	2357	2360	rVB	383	167	0.02%	0.002%
57	8.786	2398	2409	2428	rBV	489120	804410	95.64%	11.538%
58	9.172	2525	2529	2534	rBV2	332	369	0.04%	0.005%
59	9.493	2627	2629	2633	rVB	280	171	0.02%	0.002%
60	9.686	2684	2689	2691	rBV	328	284	0.03%	0.004%
61	9.728	2700	2702	2707	rVB2	289	211	0.03%	0.003%
62	9.802	2722	2725	2728	rBV3	231	181	0.02%	0.003%
63	9.841	2735	2737	2741	rBV2	214	182	0.02%	0.003%
64	9.963	2770	2775	2776	rVV2	363	269	0.03%	0.004%
65	9.989	2779	2783	2788	rBV2	347	338	0.04%	0.005%
66	10.153	2823	2834	2854	rVV	272063	430570	51.19%	6.176%
67	10.484	2935	2937	2939	rBV2	513	279	0.03%	0.004%
68	10.542	2952	2955	2959	rBV2	238	217	0.03%	0.003%
69	10.567	2961	2963	2966	rVB	353	191	0.02%	0.003%
70	10.648	2985	2988	2991	rBV2	286	199	0.02%	0.003%
71	10.792	3030	3033	3038	rBV2	194	191	0.02%	0.003%
72	11.185	3144	3155	3179	rBV	540776	841041	100.00%	12.063%
73	11.423	3226	3229	3230	rBV	372	187	0.02%	0.003%
74	11.452	3234	3238	3240	rBV	568	405	0.05%	0.006%
75	11.561	3260	3272	3293	rBV	472761	736583	87.58%	10.565%
76	11.863	3363	3366	3369	rBV2	381	231	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033029.D
 Acq On : 20 Nov 2023 18:12
 Operator : SY/MD
 Sample : VIBLK252
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK252

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	11.898	3375	3377	3380	rVB	381	185	0.02%	0.003%
78	12.008	3409	3411	3413	rBV	433	291	0.03%	0.004%
79	12.307	3498	3504	3505	rBV	348	297	0.04%	0.004%
80	12.384	3526	3528	3531	rVB2	584	298	0.04%	0.004%
81	12.429	3541	3542	3546	rVB	434	200	0.02%	0.003%
82	12.461	3550	3552	3555	rVB2	474	269	0.03%	0.004%
83	12.522	3569	3571	3575	rBV2	303	250	0.03%	0.004%
84	12.593	3589	3593	3594	rBV	573	444	0.05%	0.006%
85	12.619	3598	3601	3604	rBV2	446	404	0.05%	0.006%
86	12.722	3628	3633	3634	rBV	273	234	0.03%	0.003%
87	12.866	3676	3678	3684	rBV2	313	260	0.03%	0.004%
88	13.030	3728	3729	3734	rBV2	369	219	0.03%	0.003%
89	13.342	3823	3826	3830	rVB	472	233	0.03%	0.003%
90	13.394	3839	3842	3843	rBV2	375	174	0.02%	0.002%
91	13.455	3856	3861	3865	rBV5	1199	1162	0.14%	0.017%
92	13.535	3882	3886	3891	rBV4	405	528	0.06%	0.008%
93	13.574	3894	3898	3899	rBV2	271	178	0.02%	0.003%
94	13.654	3919	3923	3924	rBV2	469	388	0.05%	0.006%
95	13.686	3928	3933	3939	rBV3	1512	1729	0.21%	0.025%
96	13.731	3944	3947	3948	rBV2	360	216	0.03%	0.003%
97	13.760	3954	3956	3958	rBV	454	274	0.03%	0.004%
98	13.805	3968	3970	3973	rBV2	424	254	0.03%	0.004%
99	14.194	4088	4091	4093	rBV2	422	260	0.03%	0.004%
100	14.365	4141	4144	4148	rBV2	395	412	0.05%	0.006%




Sum of corrected areas: 6972117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033029.D
Acq On : 20 Nov 2023 18:12
Operator : SY/MD
Sample : VIBLK252
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK252

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

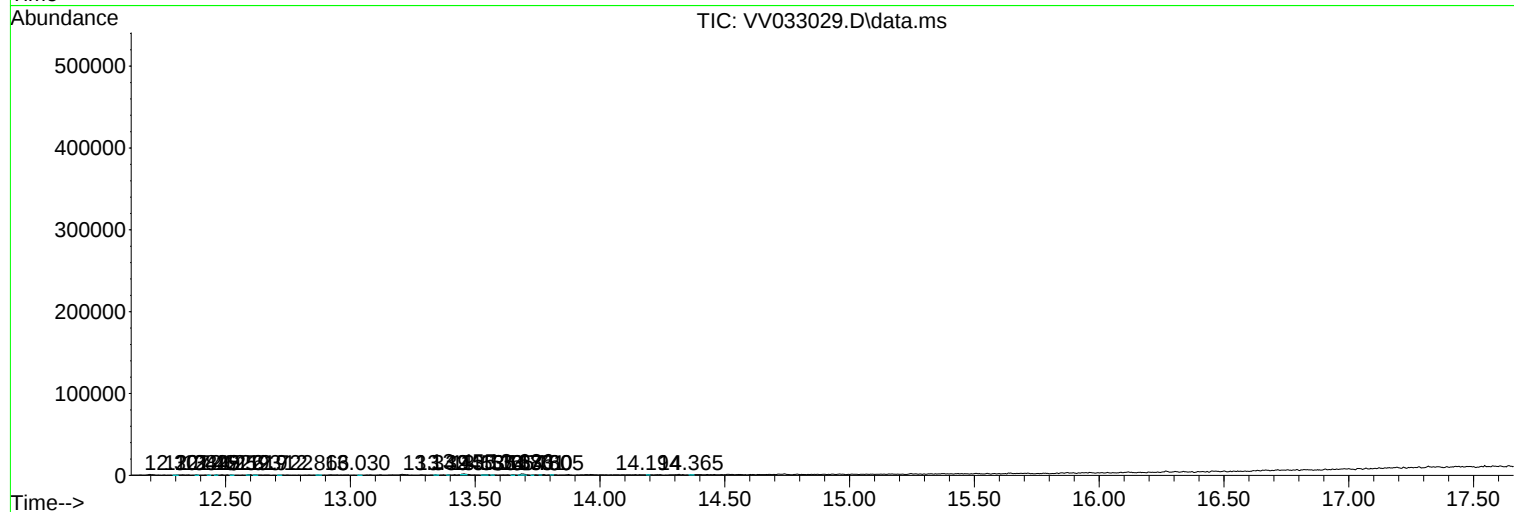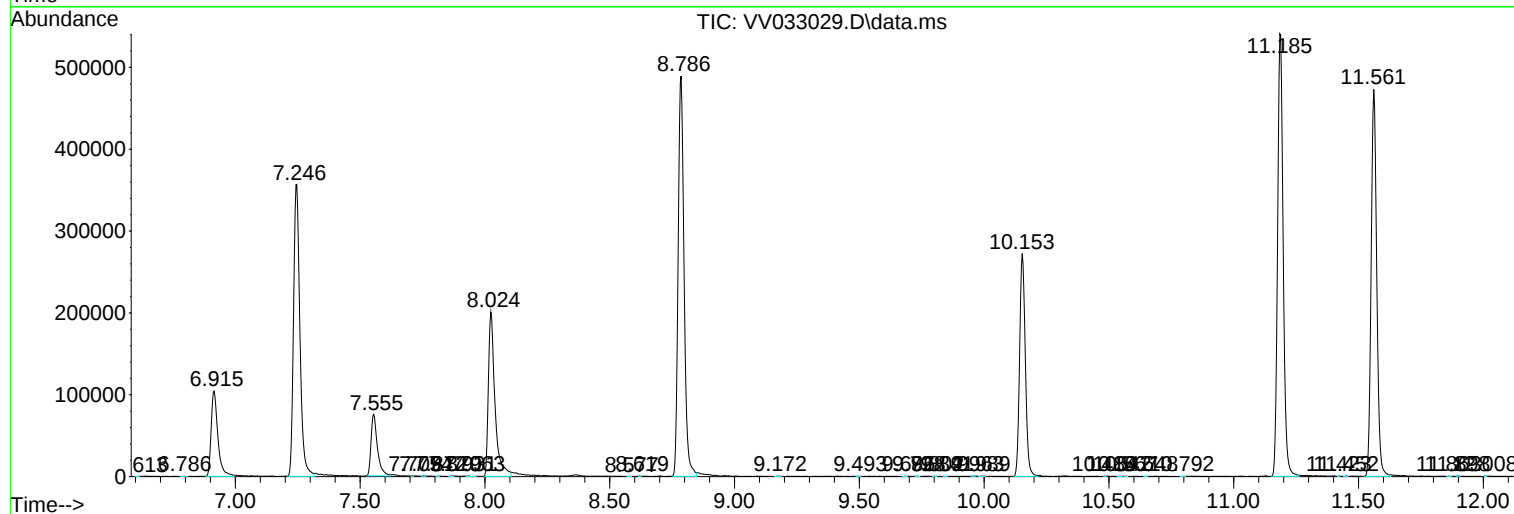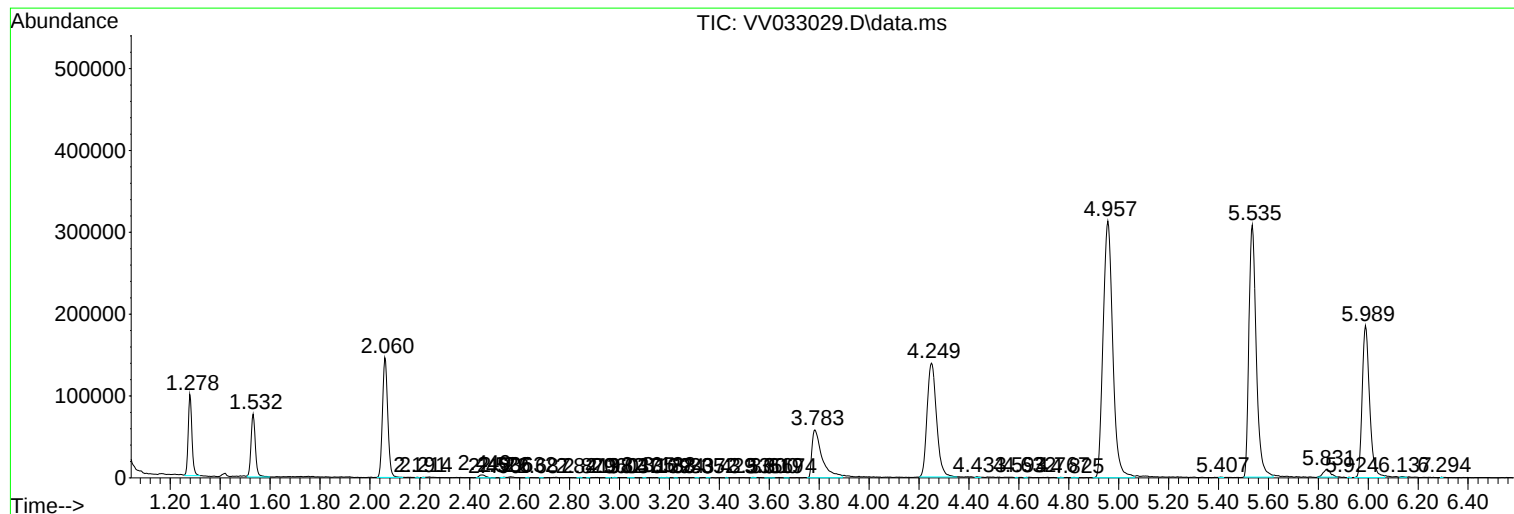

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033029.D
Acq On : 20 Nov 2023 18:12
Operator : SY/MD
Sample : VIBLK252
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK252

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033029.D
Acq On : 20 Nov 2023 18:12
Operator : SY/MD
Sample : VIBLK252
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK252

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc