

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033030.D
 Acq On : 20 Nov 2023 18:36
 Operator : SY/MD
 Sample : 05436-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1D0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	101837	107392	12.63%	1.576%
2	1.532	146	153	166	rVB	76776	90237	10.61%	1.324%
3	2.059	307	317	328	rBV	148871	220296	25.91%	3.233%
4	2.236	368	372	374	rBV2	698	578	0.07%	0.008%
5	2.297	387	391	393	rBV	371	230	0.03%	0.003%
6	2.307	393	394	396	rVV	454	169	0.02%	0.002%
7	2.333	400	402	406	rVB2	461	235	0.03%	0.003%
8	2.349	406	407	410	rVB2	526	179	0.02%	0.003%
9	2.368	411	413	416	rBV	256	156	0.02%	0.002%
10	2.423	427	430	431	rBV	223	124	0.01%	0.002%
11	2.449	431	438	447	rVV6	2357	4257	0.50%	0.062%
12	2.532	462	464	467	rBV2	509	241	0.03%	0.004%
13	2.629	492	494	497	rBV	496	155	0.02%	0.002%
14	2.683	508	511	513	rBV	412	230	0.03%	0.003%
15	2.764	534	536	541	rVB2	642	348	0.04%	0.005%
16	2.802	543	548	550	rBV3	303	277	0.03%	0.004%
17	2.931	587	588	591	rBV	452	232	0.03%	0.003%
18	2.998	605	609	612	rBV2	361	339	0.04%	0.005%
19	3.059	627	628	634	rVB	417	250	0.03%	0.004%
20	3.092	634	638	642	rBV	244	259	0.03%	0.004%
21	3.143	649	654	655	rBV	314	293	0.03%	0.004%
22	3.355	719	720	726	rVB	304	270	0.03%	0.004%
23	3.404	726	735	736	rBV	337	358	0.04%	0.005%
24	3.426	740	742	743	rBV	338	173	0.02%	0.003%
25	3.477	754	758	760	rVB	315	221	0.03%	0.003%
26	3.494	761	763	766	rVV2	239	118	0.01%	0.002%
27	3.561	782	784	789	rVB	301	150	0.02%	0.002%
28	3.625	801	804	805	rBV	267	165	0.02%	0.002%
29	3.658	810	814	815	rBV2	281	195	0.02%	0.003%
30	3.719	831	833	835	rBV	287	127	0.01%	0.002%
31	3.783	844	853	884	rBV2	54717	151975	17.87%	2.230%
32	4.146	963	966	969	rBV	711	527	0.06%	0.008%
33	4.249	984	998	1024	rBV2	144683	367451	43.21%	5.393%
34	4.625	1112	1115	1117	rBV	464	210	0.02%	0.003%
35	4.728	1145	1147	1148	rBV	325	122	0.01%	0.002%
36	4.956	1202	1218	1249	rBV3	317732	850350	100.00%	12.480%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033030.D
 Acq On : 20 Nov 2023 18:36
 Operator : SY/MD
 Sample : 05436-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1D0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	5.259	1310	1312	1315	rBV2	447	290	0.03%	0.004%
38	5.535	1386	1398	1424	rBV	281677	582145	68.46%	8.544%
39	5.831	1479	1490	1507	rBV3	13769	30611	3.60%	0.449%
40	5.989	1527	1539	1561	rBV	181742	372286	43.78%	5.464%
41	6.249	1618	1620	1624	rVB	310	202	0.02%	0.003%
42	6.313	1638	1640	1641	rBV	417	159	0.02%	0.002%
43	6.355	1650	1653	1657	rBV	342	288	0.03%	0.004%
44	6.481	1689	1692	1693	rBV	278	150	0.02%	0.002%
45	6.535	1705	1709	1712	rBV3	387	290	0.03%	0.004%
46	6.683	1752	1755	1757	rBV2	351	177	0.02%	0.003%
47	6.805	1791	1793	1796	rBV	361	230	0.03%	0.003%
48	6.876	1811	1815	1816	rBV2	254	151	0.02%	0.002%
49	6.915	1816	1827	1852	rBV	105323	197585	23.24%	2.900%
50	7.243	1918	1929	1951	rBV	358623	638582	75.10%	9.372%
51	7.554	2017	2026	2053	rBV	74702	136669	16.07%	2.006%
52	7.857	2117	2120	2121	rBV	586	386	0.05%	0.006%
53	7.870	2121	2124	2125	rBV	934	486	0.06%	0.007%
54	7.927	2140	2142	2143	rBV	366	122	0.01%	0.002%
55	8.024	2163	2172	2191	rBV	199966	359194	42.24%	5.272%
56	8.551	2332	2336	2339	rBV2	335	271	0.03%	0.004%
57	8.686	2376	2378	2379	rBV2	274	142	0.02%	0.002%
58	8.786	2397	2409	2437	rBV	448075	744704	87.58%	10.929%
59	9.017	2478	2481	2484	rVB2	487	358	0.04%	0.005%
60	9.143	2518	2520	2521	rBV	438	220	0.03%	0.003%
61	9.185	2529	2533	2537	rBV	342	416	0.05%	0.006%
62	9.214	2540	2542	2545	rVB	517	265	0.03%	0.004%
63	9.265	2555	2558	2561	rVB2	530	336	0.04%	0.005%
64	9.287	2561	2565	2567	rBV	339	293	0.03%	0.004%
65	9.352	2582	2585	2587	rBV3	352	208	0.02%	0.003%
66	9.387	2594	2596	2598	rBV2	193	133	0.02%	0.002%
67	9.439	2604	2612	2615	rBV2	377	537	0.06%	0.008%
68	9.570	2651	2653	2655	rBV	248	118	0.01%	0.002%
69	9.683	2685	2688	2690	rBV2	211	162	0.02%	0.002%
70	9.744	2705	2707	2712	rVB	482	290	0.03%	0.004%
71	9.773	2712	2716	2718	rBV	358	257	0.03%	0.004%
72	9.873	2743	2747	2748	rBV2	264	191	0.02%	0.003%
73	10.024	2792	2794	2798	rVV2	438	196	0.02%	0.003%
74	10.111	2819	2821	2823	rVV	583	222	0.03%	0.003%
75	10.152	2823	2834	2860	rVV	266319	424275	49.89%	6.227%
76	10.320	2882	2886	2887	rBV2	1275	857	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033030.D
 Acq On : 20 Nov 2023 18:36
 Operator : SY/MD
 Sample : 05436-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1D0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	10.423	2916	2918	2921	rVB2	433	130	0.02%	0.002%
78	10.667	2991	2994	2995	rBV	200	120	0.01%	0.002%
79	11.024	3098	3105	3107	rBV2	830	795	0.09%	0.012%
80	11.078	3118	3122	3126	rBV2	352	324	0.04%	0.005%
81	11.185	3144	3155	3182	rBV	493103	766106	90.09%	11.244%
82	11.561	3261	3272	3297	rVB	473047	747014	87.85%	10.963%
83	11.744	3327	3329	3331	rBV	548	282	0.03%	0.004%
84	11.757	3331	3333	3337	rVB2	667	361	0.04%	0.005%
85	11.824	3351	3354	3358	rVB3	546	319	0.04%	0.005%
86	12.008	3404	3411	3414	rBV2	551	579	0.07%	0.008%
87	12.046	3420	3423	3425	rVB2	302	138	0.02%	0.002%
88	12.149	3453	3455	3457	rBV2	334	139	0.02%	0.002%
89	12.268	3487	3492	3493	rBV2	502	322	0.04%	0.005%
90	12.541	3575	3577	3579	rBV2	491	264	0.03%	0.004%
91	12.660	3612	3614	3620	rBV2	421	383	0.05%	0.006%
92	12.911	3686	3692	3694	rBV2	512	468	0.06%	0.007%
93	13.062	3734	3739	3743	rBV2	473	523	0.06%	0.008%
94	13.300	3811	3813	3816	rVB	521	245	0.03%	0.004%
95	13.725	3943	3945	3947	rBV3	402	205	0.02%	0.003%
96	13.763	3954	3957	3962	rVB3	548	463	0.05%	0.007%
97	13.802	3967	3969	3971	rBV	639	265	0.03%	0.004%
98	13.850	3982	3984	3987	rBV3	577	423	0.05%	0.006%
99	13.905	3998	4001	4002	rBV2	553	297	0.03%	0.004%
100	14.088	4056	4058	4060	rBV2	553	239	0.03%	0.004%




Sum of corrected areas: 6813747

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033030.D
Acq On : 20 Nov 2023 18:36
Operator : SY/MD
Sample : 05436-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1D0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

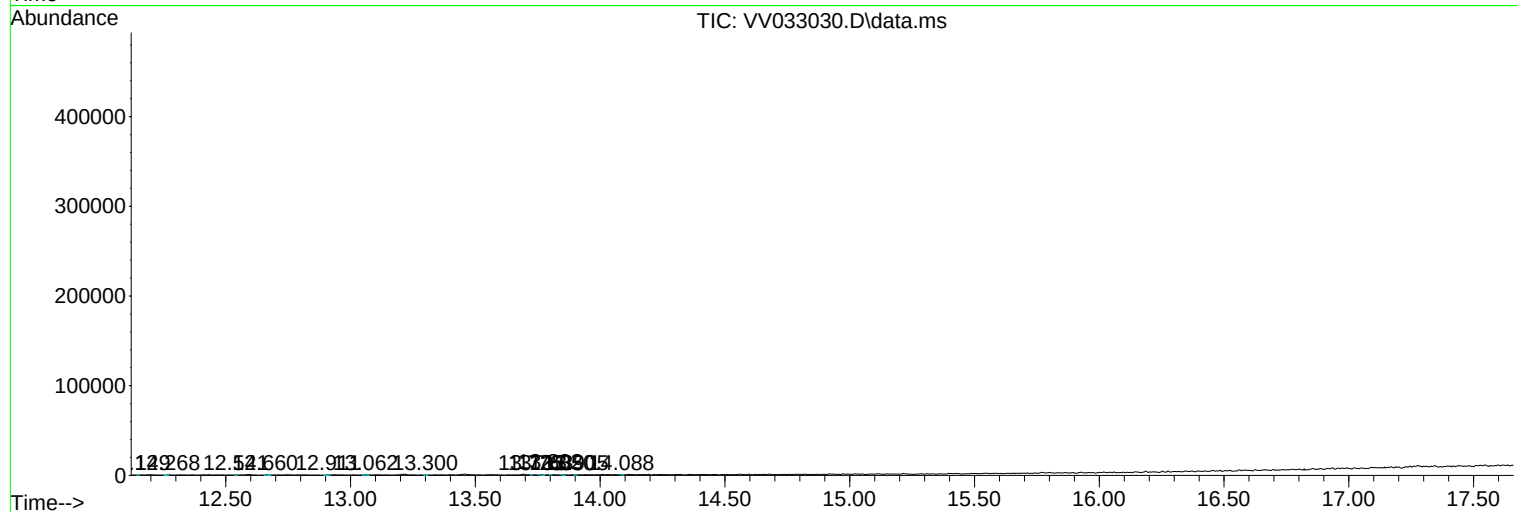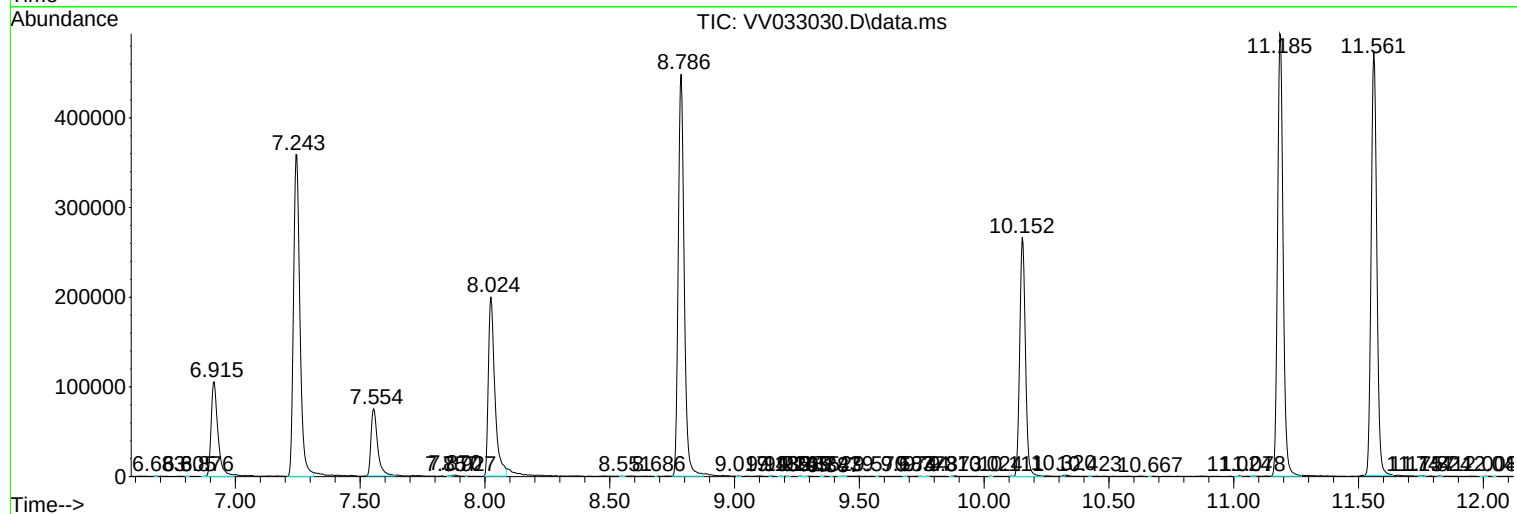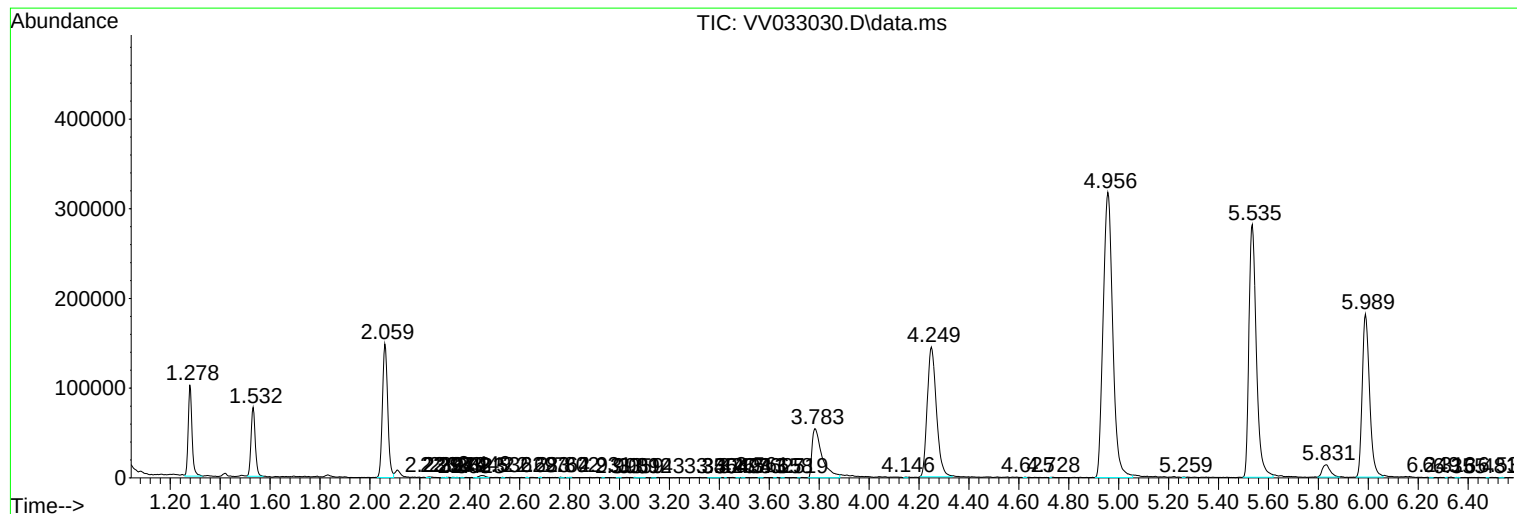

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033030.D
Acq On : 20 Nov 2023 18:36
Operator : SY/MD
Sample : 05436-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1D0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033030.D
Acq On : 20 Nov 2023 18:36
Operator : SY/MD
Sample : 05436-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1D0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------