

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033031.D
 Acq On : 20 Nov 2023 18:59
 Operator : SY/MD
 Sample : 05497-06
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	104677	110672	11.22%	1.383%
2	1.532	145	153	166	rVB	82972	99576	10.09%	1.245%
3	2.059	306	317	332	rBV	166758	244002	24.73%	3.050%
4	2.207	360	363	366	rBV2	818	741	0.08%	0.009%
5	2.449	432	438	445	rBV4	1389	1948	0.20%	0.024%
6	2.539	464	466	471	rVB2	614	496	0.05%	0.006%
7	2.561	471	473	475	rBV2	713	390	0.04%	0.005%
8	2.632	491	495	497	rBV2	421	320	0.03%	0.004%
9	2.725	520	524	528	rBV2	357	241	0.02%	0.003%
10	2.776	532	540	542	rBV	366	347	0.04%	0.004%
11	2.815	550	552	555	rVB2	393	220	0.02%	0.003%
12	2.838	556	559	562	rVV3	398	267	0.03%	0.003%
13	2.892	574	576	577	rBV3	268	145	0.01%	0.002%
14	2.915	581	583	588	rBV2	378	331	0.03%	0.004%
15	3.037	615	621	624	rBV	431	430	0.04%	0.005%
16	3.085	634	636	639	rVB2	267	135	0.01%	0.002%
17	3.278	694	696	700	rBV2	318	160	0.02%	0.002%
18	3.294	700	701	705	rVB	291	110	0.01%	0.001%
19	3.362	718	722	723	rBV	271	157	0.02%	0.002%
20	3.394	730	732	734	rBV	183	101	0.01%	0.001%
21	3.407	734	736	739	rBV2	284	189	0.02%	0.002%
22	3.510	766	768	770	rBV2	442	204	0.02%	0.003%
23	3.542	776	778	781	rVB2	356	185	0.02%	0.002%
24	3.564	782	785	787	rBV	354	214	0.02%	0.003%
25	3.590	790	793	796	rVB2	168	122	0.01%	0.002%
26	3.612	796	800	801	rBV2	260	213	0.02%	0.003%
27	3.657	811	814	816	rBV	162	119	0.01%	0.001%
28	3.670	816	818	822	rVB	487	265	0.03%	0.003%
29	3.741	838	840	843	rVB	281	146	0.01%	0.002%
30	3.780	844	852	879	rBV2	63412	167721	17.00%	2.096%
31	4.249	984	998	1035	rVB	161638	412854	41.84%	5.160%
32	4.696	1135	1137	1140	rVB	307	135	0.01%	0.002%
33	4.789	1164	1166	1167	rBV	264	92	0.01%	0.001%
34	4.899	1197	1200	1202	rBV	381	191	0.02%	0.002%
35	4.956	1202	1218	1244	rBV2	352253	936856	94.95%	11.710%
36	5.410	1357	1359	1362	rBV2	480	356	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033031.D
 Acq On : 20 Nov 2023 18:59
 Operator : SY/MD
 Sample : 05497-06
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	5.535	1386	1398	1427	rBV	361681	752024	76.22%	9.400%
38	5.738	1459	1461	1463	rBV	528	251	0.03%	0.003%
39	5.789	1474	1477	1478	rBV	499	348	0.04%	0.004%
40	5.825	1479	1488	1511	rVB3	17360	40151	4.07%	0.502%
41	5.989	1526	1539	1563	rBV	209629	431026	43.68%	5.387%
42	6.326	1643	1644	1646	rVB	448	148	0.01%	0.002%
43	6.394	1662	1665	1667	rBV2	311	210	0.02%	0.003%
44	6.407	1667	1669	1672	rVV2	316	137	0.01%	0.002%
45	6.452	1681	1683	1686	rBV2	218	100	0.01%	0.001%
46	6.464	1686	1687	1689	rBV2	421	109	0.01%	0.001%
47	6.516	1701	1703	1706	rBV2	298	116	0.01%	0.001%
48	6.590	1724	1726	1728	rBV2	345	241	0.02%	0.003%
49	6.735	1769	1771	1774	rVB2	437	217	0.02%	0.003%
50	6.754	1774	1777	1782	rBV2	380	493	0.05%	0.006%
51	6.915	1817	1827	1853	rBV2	118638	220691	22.37%	2.758%
52	7.127	1890	1893	1899	rBV5	516	524	0.05%	0.007%
53	7.204	1915	1917	1918	rBV	336	139	0.01%	0.002%
54	7.243	1918	1929	1952	rBV	402874	716676	72.63%	8.958%
55	7.554	2016	2026	2048	rBV2	86537	154793	15.69%	1.935%
56	7.789	2097	2099	2103	rVB2	318	196	0.02%	0.002%
57	7.985	2154	2160	2162	rBV2	452	444	0.04%	0.006%
58	8.024	2162	2172	2199	rBV	233757	431046	43.69%	5.388%
59	8.490	2315	2317	2319	rBV	279	114	0.01%	0.001%
60	8.564	2338	2340	2347	rVB4	529	401	0.04%	0.005%
61	8.786	2397	2409	2439	rBV	582646	957763	97.07%	11.971%
62	8.995	2472	2474	2477	rBV3	363	275	0.03%	0.003%
63	9.053	2490	2492	2493	rVB	357	102	0.01%	0.001%
64	9.069	2493	2497	2499	rBV2	565	482	0.05%	0.006%
65	9.123	2511	2514	2517	rBV	250	205	0.02%	0.003%
66	9.223	2543	2545	2549	rVB2	487	241	0.02%	0.003%
67	9.310	2569	2572	2578	rVB4	455	427	0.04%	0.005%
68	9.406	2598	2602	2606	rBV2	297	368	0.04%	0.005%
69	9.812	2726	2728	2732	rVB	359	176	0.02%	0.002%
70	9.956	2770	2773	2775	rBV2	240	191	0.02%	0.002%
71	10.043	2798	2800	2802	rBV2	351	187	0.02%	0.002%
72	10.152	2822	2834	2853	rBV	296750	471996	47.84%	5.899%
73	10.329	2877	2889	2898	rBV4	2634	4588	0.46%	0.057%
74	10.390	2906	2908	2910	rVB2	508	187	0.02%	0.002%
75	10.657	2989	2991	2994	rVB2	477	227	0.02%	0.003%
76	10.673	2994	2996	2997	rBV2	267	109	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112023\
 Data File : VW033031.D
 Acq On : 20 Nov 2023 18:59
 Operator : SY/MD
 Sample : 05497-06
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	10.860	3052	3054	3064	rVB3	743	937	0.09%	0.012%
78	10.966	3084	3087	3090	rBV	295	172	0.02%	0.002%
79	11.030	3105	3107	3108	rBV	303	95	0.01%	0.001%
80	11.185	3144	3155	3182	rBV	646057	986707	100.00%	12.333%
81	11.403	3221	3223	3225	rBV	238	106	0.01%	0.001%
82	11.442	3234	3235	3237	rBV	302	95	0.01%	0.001%
83	11.490	3246	3250	3251	rBV	293	161	0.02%	0.002%
84	11.561	3261	3272	3292	rBV	538125	838141	84.94%	10.476%
85	11.956	3392	3395	3396	rBV	431	297	0.03%	0.004%
86	12.020	3412	3415	3416	rBV	346	169	0.02%	0.002%
87	12.075	3430	3432	3433	rBV	210	82	0.01%	0.001%
88	12.098	3437	3439	3440	rBV	339	160	0.02%	0.002%
89	12.146	3451	3454	3457	rBV2	324	237	0.02%	0.003%
90	12.442	3544	3546	3550	rVB2	406	214	0.02%	0.003%
91	12.512	3566	3568	3572	rBV2	616	334	0.03%	0.004%
92	12.577	3587	3588	3589	rBV2	338	99	0.01%	0.001%
93	12.625	3601	3603	3606	rBV2	476	273	0.03%	0.003%
94	12.953	3703	3705	3707	rBV	273	151	0.02%	0.002%
95	13.201	3779	3782	3785	rBV3	675	607	0.06%	0.008%
96	13.294	3808	3811	3812	rBV2	442	242	0.02%	0.003%
97	13.532	3881	3885	3889	rBV4	620	642	0.07%	0.008%
98	13.554	3890	3892	3896	rVV	418	249	0.03%	0.003%
99	13.686	3927	3933	3938	rBV5	1025	1221	0.12%	0.015%
100	14.184	4084	4088	4093	rBV2	465	453	0.05%	0.006%




Sum of corrected areas: 8000614

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033031.D
Acq On : 20 Nov 2023 18:59
Operator : SY/MD
Sample : 05497-06
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

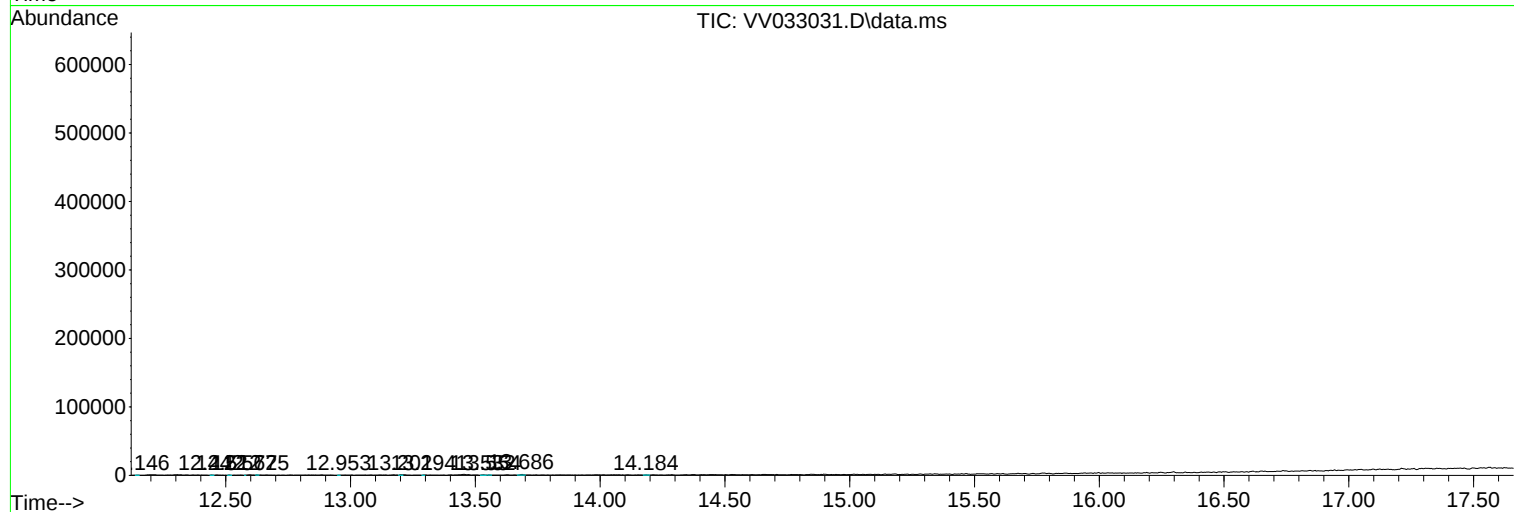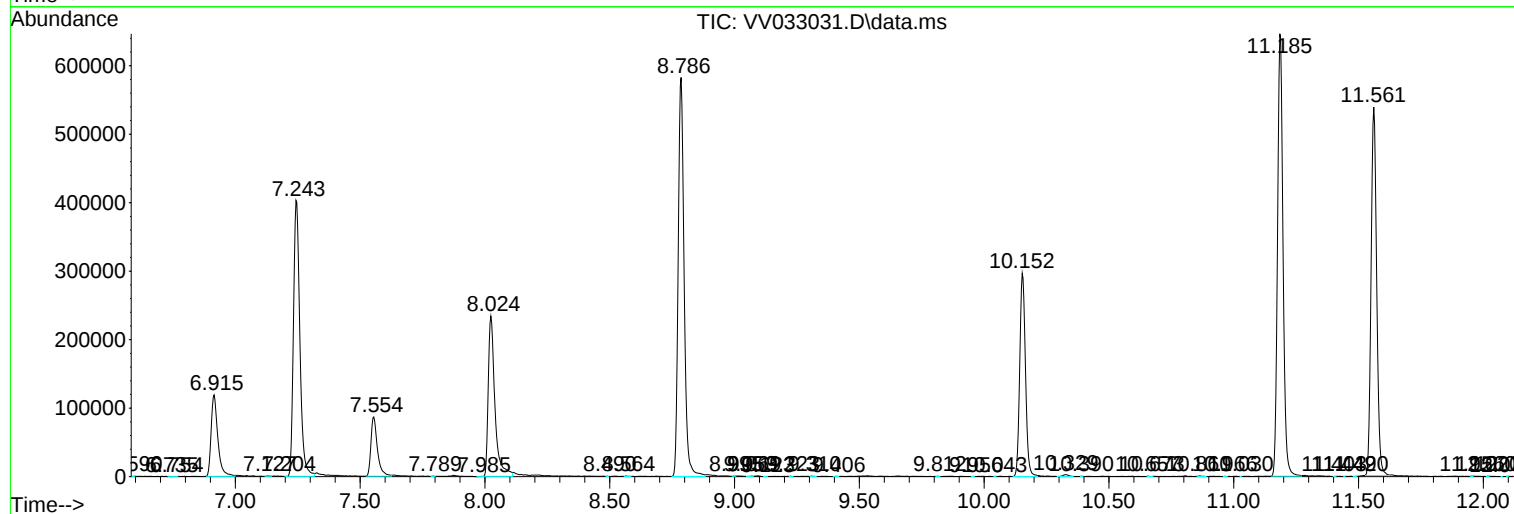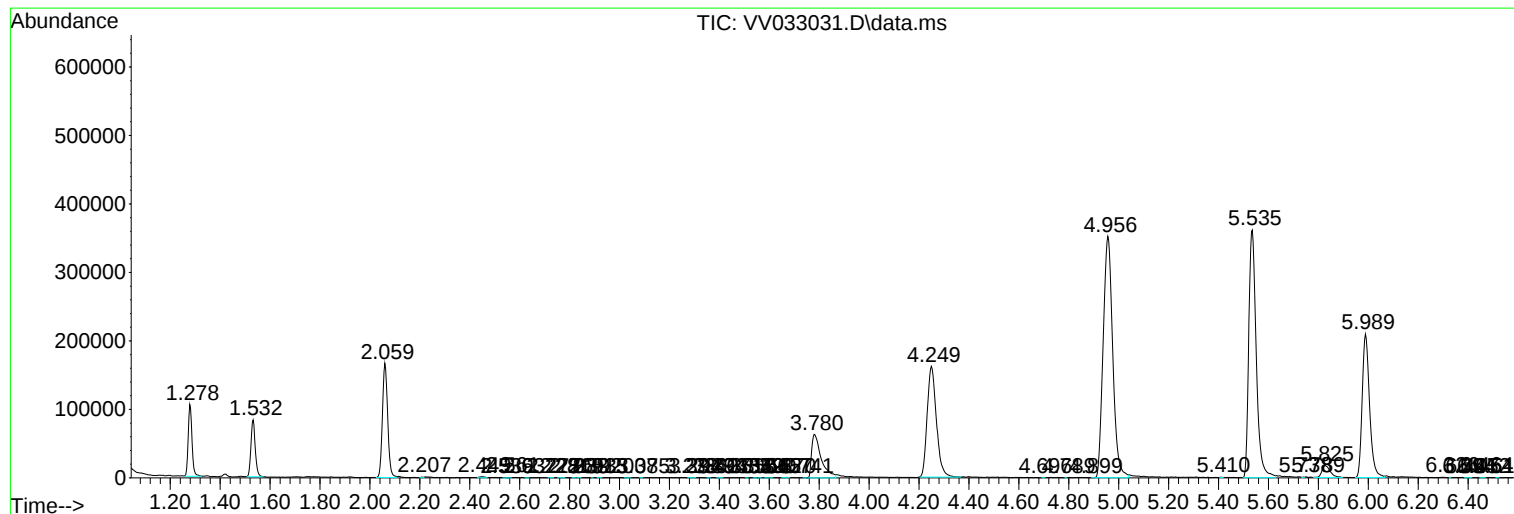

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033031.D
Acq On : 20 Nov 2023 18:59
Operator : SY/MD
Sample : 05497-06
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033031.D
Acq On : 20 Nov 2023 18:59
Operator : SY/MD
Sample : 05497-06
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc