

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033032.D
 Acq On : 20 Nov 2023 19:22
 Operator : SY/MD
 Sample : 05477-06
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M

Title : VOC Analysis

Signal : TIC: VV033032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	103883	109482	11.01%	1.367%
2	1.532	145	153	163	rBV	83643	99326	9.99%	1.240%
3	2.060	307	317	333	rBV	162197	238113	23.95%	2.973%
4	2.211	358	364	365	rBV2	1004	733	0.07%	0.009%
5	2.314	395	396	399	rBV	341	140	0.01%	0.002%
6	2.368	411	413	415	rBV	407	173	0.02%	0.002%
7	2.510	454	457	459	rBV2	293	192	0.02%	0.002%
8	2.558	469	472	476	rBV3	509	395	0.04%	0.005%
9	2.632	493	495	498	rVB	335	155	0.02%	0.002%
10	2.651	498	501	503	rBV	194	128	0.01%	0.002%
11	2.735	525	527	529	rBV	218	129	0.01%	0.002%
12	2.773	536	539	543	rVB	298	257	0.03%	0.003%
13	2.799	543	547	549	rBV	435	407	0.04%	0.005%
14	2.947	590	593	595	rBV2	231	178	0.02%	0.002%
15	3.011	609	613	615	rBV	331	349	0.04%	0.004%
16	3.053	624	626	632	rBV	429	271	0.03%	0.003%
17	3.137	648	652	656	rBV2	279	202	0.02%	0.003%
18	3.391	726	731	734	rBV2	260	280	0.03%	0.003%
19	3.410	734	737	740	rBV2	320	191	0.02%	0.002%
20	3.474	752	757	761	rBV2	374	378	0.04%	0.005%
21	3.568	784	786	789	rVB	411	196	0.02%	0.002%
22	3.587	790	792	795	rVV2	343	144	0.01%	0.002%
23	3.658	810	814	816	rBV	312	262	0.03%	0.003%
24	3.725	833	835	837	rBV	244	123	0.01%	0.002%
25	3.744	837	841	843	rBV2	272	202	0.02%	0.003%
26	3.780	844	852	887	rBV	64790	175107	17.61%	2.187%
27	4.249	984	998	1033	rVB2	160078	415686	41.80%	5.191%
28	4.757	1154	1156	1158	rBB2	381	129	0.01%	0.002%
29	4.773	1159	1161	1162	rBV	393	116	0.01%	0.001%
30	4.873	1190	1192	1196	rVB3	349	143	0.01%	0.002%
31	4.957	1202	1218	1245	rBV2	349577	942324	94.77%	11.767%
32	5.224	1299	1301	1307	rBV4	797	659	0.07%	0.008%
33	5.400	1354	1356	1361	rBV2	540	288	0.03%	0.004%
34	5.535	1385	1398	1424	rBV	363637	746190	75.04%	9.318%
35	5.825	1479	1488	1510	rVB3	16495	35658	3.59%	0.445%
36	5.989	1526	1539	1565	rBV	203973	428756	43.12%	5.354%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033032.D
 Acq On : 20 Nov 2023 19:22
 Operator : SY/MD
 Sample : 05477-06
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	6.285	1629	1631	1632	rBV	342	136	0.01%	0.002%
38	6.339	1645	1648	1650	rBV	355	199	0.02%	0.002%
39	6.375	1657	1659	1662	rBV3	331	226	0.02%	0.003%
40	6.391	1662	1664	1667	rVV	327	199	0.02%	0.002%
41	6.410	1668	1670	1673	rBV2	421	206	0.02%	0.003%
42	6.487	1691	1694	1695	rBV2	373	222	0.02%	0.003%
43	6.542	1709	1711	1714	rBV2	244	144	0.01%	0.002%
44	6.561	1714	1717	1719	rVV	222	135	0.01%	0.002%
45	6.600	1725	1729	1730	rBV	316	240	0.02%	0.003%
46	6.664	1745	1749	1752	rBV2	408	393	0.04%	0.005%
47	6.722	1764	1767	1770	rBV	433	313	0.03%	0.004%
48	6.805	1788	1793	1796	rBV	179	235	0.02%	0.003%
49	6.915	1816	1827	1847	rBV	117644	219335	22.06%	2.739%
50	7.246	1917	1930	1959	rBV	406387	726679	73.08%	9.074%
51	7.555	2016	2026	2046	rBV	85128	154950	15.58%	1.935%
52	7.799	2099	2102	2105	rBV3	501	379	0.04%	0.005%
53	7.937	2142	2145	2147	rBV	359	169	0.02%	0.002%
54	8.024	2163	2172	2205	rBV	233140	429506	43.19%	5.363%
55	8.410	2291	2292	2296	rVB2	378	135	0.01%	0.002%
56	8.519	2324	2326	2327	rBV	273	108	0.01%	0.001%
57	8.786	2397	2409	2440	rBV	580280	954538	95.99%	11.919%
58	9.066	2495	2496	2498	rBV	358	180	0.02%	0.002%
59	9.227	2545	2546	2548	rBV2	477	208	0.02%	0.003%
60	9.407	2600	2602	2604	rBV2	254	143	0.01%	0.002%
61	9.420	2604	2606	2611	rVB2	336	264	0.03%	0.003%
62	9.487	2623	2627	2629	rBV	271	158	0.02%	0.002%
63	9.500	2629	2631	2632	rBV	285	154	0.02%	0.002%
64	9.532	2638	2641	2644	rBV2	287	193	0.02%	0.002%
65	9.741	2702	2706	2707	rBV	300	181	0.02%	0.002%
66	9.828	2731	2733	2735	rBV2	273	140	0.01%	0.002%
67	9.911	2758	2759	2761	rBV	436	178	0.02%	0.002%
68	9.963	2774	2775	2780	rVB	652	386	0.04%	0.005%
69	9.985	2780	2782	2783	rBV	275	114	0.01%	0.001%
70	10.008	2787	2789	2791	rBV2	260	117	0.01%	0.001%
71	10.153	2823	2834	2855	rBV	302902	470433	47.31%	5.874%
72	10.329	2881	2889	2899	rVV5	2124	3324	0.33%	0.042%
73	10.391	2903	2908	2909	rBV2	397	305	0.03%	0.004%
74	10.429	2918	2920	2923	rBV2	311	128	0.01%	0.002%
75	10.747	3017	3019	3020	rBV	297	140	0.01%	0.002%
76	10.857	3050	3053	3058	rBV2	437	432	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033032.D
 Acq On : 20 Nov 2023 19:22
 Operator : SY/MD
 Sample : 05477-06
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	10.905	3064	3068	3070	rBV2	247	211	0.02%	0.003%
78	10.960	3083	3085	3088	rBV	279	176	0.02%	0.002%
79	10.982	3090	3092	3097	rVB	395	216	0.02%	0.003%
80	11.030	3104	3107	3108	rBV2	252	121	0.01%	0.002%
81	11.043	3108	3111	3115	rVB2	555	347	0.03%	0.004%
82	11.185	3143	3155	3179	rBV	628930	994366	100.00%	12.417%
83	11.519	3255	3259	3260	rBV2	267	166	0.02%	0.002%
84	11.561	3260	3272	3299	rBV	536393	844074	84.89%	10.540%
85	11.944	3389	3391	3396	rBV	253	190	0.02%	0.002%
86	12.005	3407	3410	3412	rBV	323	239	0.02%	0.003%
87	12.043	3419	3422	3423	rBV	283	179	0.02%	0.002%
88	12.069	3429	3430	3433	rBV2	271	130	0.01%	0.002%
89	12.107	3438	3442	3444	rBV2	430	312	0.03%	0.004%
90	12.342	3514	3515	3518	rBV	383	143	0.01%	0.002%
91	12.513	3565	3568	3570	rBV	312	231	0.02%	0.003%
92	12.587	3589	3591	3598	rVB5	984	902	0.09%	0.011%
93	12.616	3598	3600	3603	rBV2	397	218	0.02%	0.003%
94	12.853	3673	3674	3677	rBV2	248	134	0.01%	0.002%
95	13.503	3873	3876	3877	rBV2	384	180	0.02%	0.002%
96	13.686	3925	3933	3936	rBV4	1189	1500	0.15%	0.019%
97	13.802	3966	3969	3971	rBV3	459	301	0.03%	0.004%
98	13.908	4000	4002	4004	rBV2	422	263	0.03%	0.003%
99	13.976	4021	4023	4025	rBV	282	121	0.01%	0.002%
100	14.342	4134	4137	4139	rBV2	808	572	0.06%	0.007%




Sum of corrected areas: 8008379

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033032.D
Acq On : 20 Nov 2023 19:22
Operator : SY/MD
Sample : 05477-06
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

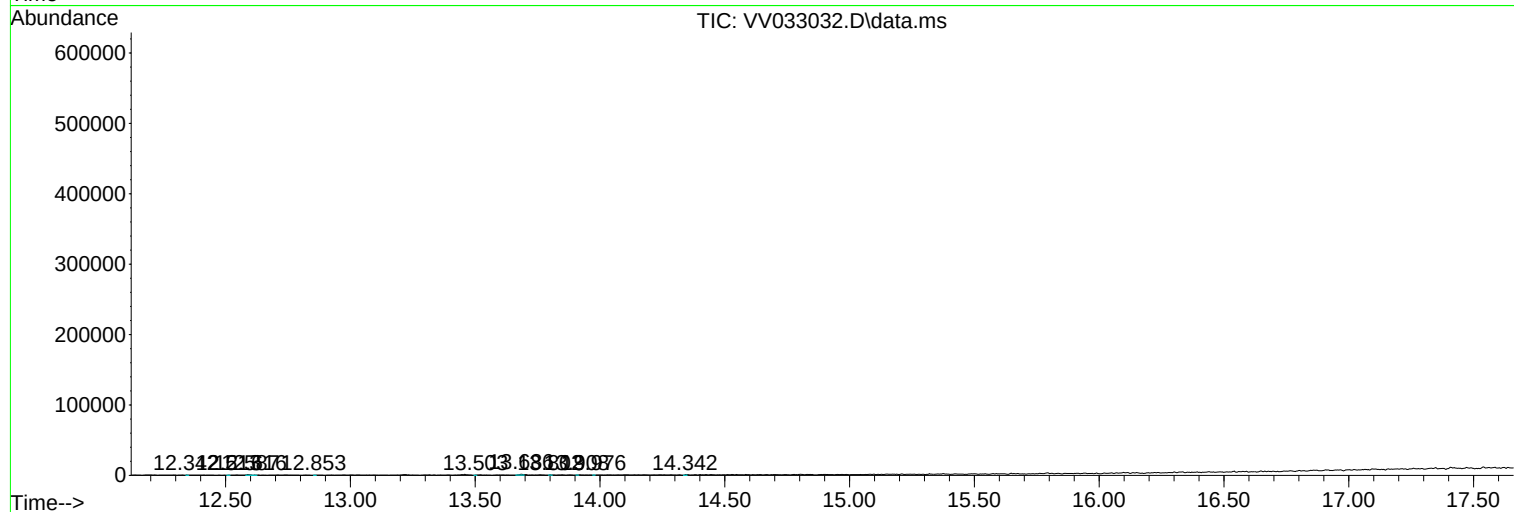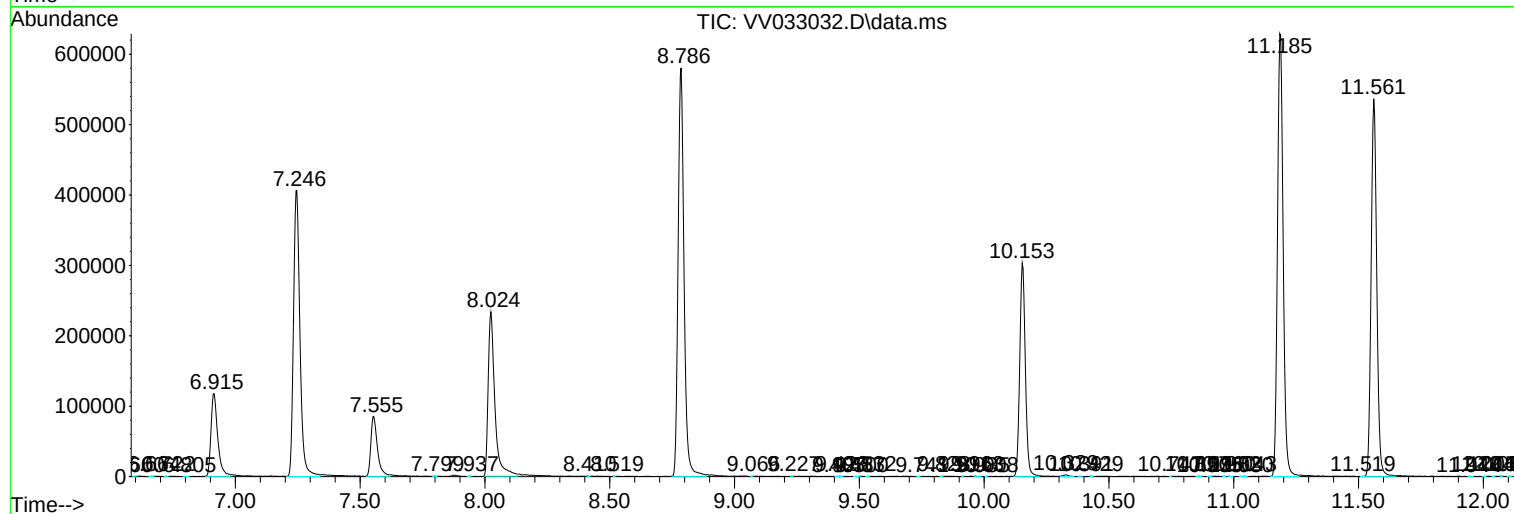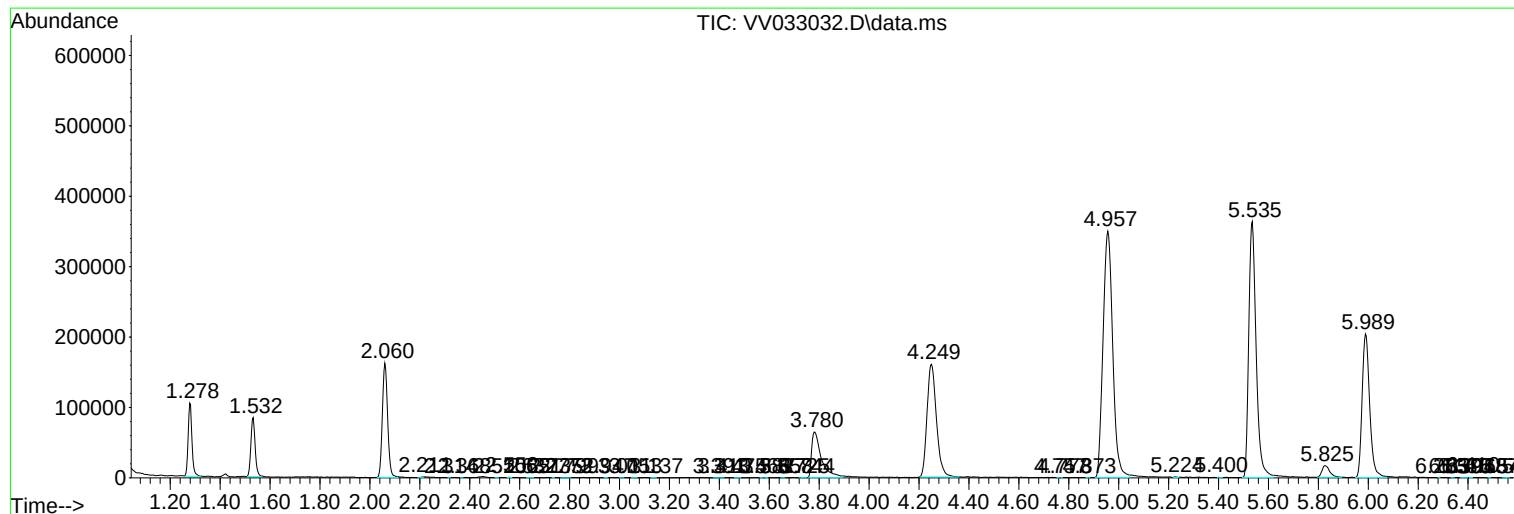

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033032.D
Acq On : 20 Nov 2023 19:22
Operator : SY/MD
Sample : 05477-06
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033032.D
Acq On : 20 Nov 2023 19:22
Operator : SY/MD
Sample : 05477-06
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc