

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033033.D
 Acq On : 20 Nov 2023 19:45
 Operator : SY/MD
 Sample : 05436-11 10X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M

Title : VOC Analysis

Signal : TIC: VV033033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rVB	97053	105386	7.95%	1.137%
2	1.532	145	153	167	rVB	79057	96798	7.30%	1.044%
3	1.979	290	292	294	rBV	367	198	0.01%	0.002%
4	2.059	307	317	334	rBV	160715	235375	17.75%	2.539%
5	2.153	344	346	347	rBV	447	235	0.02%	0.003%
6	2.449	430	438	448	rBV	4900	7443	0.56%	0.080%
7	2.625	490	493	494	rBV	230	147	0.01%	0.002%
8	2.635	494	496	502	rVB	556	424	0.03%	0.005%
9	2.664	502	505	507	rBV	213	128	0.01%	0.001%
10	2.703	511	517	520	rBV3	592	544	0.04%	0.006%
11	2.821	552	554	556	rVV2	293	118	0.01%	0.001%
12	2.992	601	607	608	rBV	347	243	0.02%	0.003%
13	3.053	621	626	628	rBV2	307	259	0.02%	0.003%
14	3.108	636	643	645	rBV3	904	812	0.06%	0.009%
15	3.204	670	673	676	rVB2	234	121	0.01%	0.001%
16	3.239	681	684	686	rBV2	238	178	0.01%	0.002%
17	3.481	756	759	761	rBV2	307	189	0.01%	0.002%
18	3.542	774	778	781	rBV2	489	347	0.03%	0.004%
19	3.561	781	784	785	rBV2	268	170	0.01%	0.002%
20	3.571	785	787	791	rVB	351	149	0.01%	0.002%
21	3.648	808	811	817	rVB2	509	345	0.03%	0.004%
22	3.741	837	840	842	rBV	242	175	0.01%	0.002%
23	3.783	843	853	882	rBV	63812	184901	13.94%	1.995%
24	4.249	983	998	1023	rBV	160853	408087	30.78%	4.402%
25	4.641	1117	1120	1122	rBV	544	288	0.02%	0.003%
26	4.715	1141	1143	1145	rBV	275	122	0.01%	0.001%
27	4.757	1155	1156	1159	rVB2	378	134	0.01%	0.001%
28	4.892	1195	1198	1201	rBV3	461	311	0.02%	0.003%
29	4.956	1201	1218	1246	rBV3	372074	986390	74.39%	10.640%
30	5.374	1346	1348	1351	rVB	486	258	0.02%	0.003%
31	5.391	1351	1353	1356	rBV	417	246	0.02%	0.003%
32	5.535	1386	1398	1423	rBV	328894	686443	51.77%	7.405%
33	5.831	1476	1490	1522	rBV	654531	1326024	100.00%	14.304%
34	5.989	1528	1539	1562	rVB2	215541	432473	32.61%	4.665%
35	6.342	1645	1649	1652	rBV2	343	292	0.02%	0.003%
36	6.423	1670	1674	1677	rBV	361	264	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033033.D
 Acq On : 20 Nov 2023 19:45
 Operator : SY/MD
 Sample : 05436-11 10X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	6.468	1686	1688	1691	rBV	276	159	0.01%	0.002%
38	6.577	1720	1722	1723	rBV	483	201	0.02%	0.002%
39	6.670	1749	1751	1754	rVB	464	156	0.01%	0.002%
40	6.689	1755	1757	1759	rVB	377	150	0.01%	0.002%
41	6.725	1765	1768	1770	rBV2	575	348	0.03%	0.004%
42	6.751	1774	1776	1780	rVB2	291	156	0.01%	0.002%
43	6.773	1780	1783	1785	rBV	300	162	0.01%	0.002%
44	6.915	1816	1827	1852	rBV	123487	233278	17.59%	2.516%
45	7.243	1918	1929	1957	rBV	450665	800251	60.35%	8.632%
46	7.554	2017	2026	2050	rBV	90188	163049	12.30%	1.759%
47	7.802	2100	2103	2104	rBV2	407	204	0.02%	0.002%
48	7.879	2117	2127	2136	rBV3	1733	2757	0.21%	0.030%
49	7.982	2154	2159	2163	rBV3	322	354	0.03%	0.004%
50	8.024	2163	2172	2193	rBV	231786	416121	31.38%	4.489%
51	8.387	2283	2285	2286	rBV2	492	213	0.02%	0.002%
52	8.442	2299	2302	2303	rBV	515	300	0.02%	0.003%
53	8.487	2312	2316	2321	rBV3	603	623	0.05%	0.007%
54	8.564	2338	2340	2341	rBV3	358	138	0.01%	0.001%
55	8.593	2347	2349	2350	rVB3	338	124	0.01%	0.001%
56	8.603	2350	2352	2353	rBV	383	187	0.01%	0.002%
57	8.622	2356	2358	2360	rBV2	306	161	0.01%	0.002%
58	8.715	2385	2387	2390	rBV2	493	220	0.02%	0.002%
59	8.786	2398	2409	2431	rBV	543634	887749	66.95%	9.576%
60	9.033	2484	2486	2489	rBV	351	147	0.01%	0.002%
61	9.156	2522	2524	2529	rBV2	434	391	0.03%	0.004%
62	9.210	2538	2541	2545	rBV2	267	237	0.02%	0.003%
63	9.271	2558	2560	2566	rVB2	454	255	0.02%	0.003%
64	9.522	2635	2638	2639	rBV	550	278	0.02%	0.003%
65	9.603	2661	2663	2665	rBV	367	121	0.01%	0.001%
66	9.622	2665	2669	2672	rBV2	343	272	0.02%	0.003%
67	9.635	2672	2673	2677	rVB	311	185	0.01%	0.002%
68	9.664	2677	2682	2683	rBV	420	259	0.02%	0.003%
69	9.795	2720	2723	2727	rBV2	384	373	0.03%	0.004%
70	9.831	2731	2734	2739	rBV3	392	417	0.03%	0.004%
71	9.959	2769	2774	2776	rBV2	446	332	0.03%	0.004%
72	10.152	2816	2834	2855	rBV	317563	496891	37.47%	5.360%
73	10.310	2880	2883	2884	rBV	391	224	0.02%	0.002%
74	10.480	2932	2936	2941	rBV4	396	402	0.03%	0.004%
75	10.599	2971	2973	2977	rVB2	538	312	0.02%	0.003%
76	10.622	2977	2980	2981	rBV	364	241	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112023\
 Data File : VW033033.D
 Acq On : 20 Nov 2023 19:45
 Operator : SY/MD
 Sample : 05436-11 10X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	10.683	2997	2999	3002	rBV2	337	154	0.01%	0.002%
78	10.779	3026	3029	3031	rBV2	432	182	0.01%	0.002%
79	10.792	3031	3033	3036	rVB2	315	135	0.01%	0.001%
80	10.889	3061	3063	3065	rVB	530	206	0.02%	0.002%
81	11.139	3134	3141	3144	rBV3	585	643	0.05%	0.007%
82	11.184	3144	3155	3185	rBV	595031	922331	69.56%	9.949%
83	11.561	3258	3272	3290	rBV	544143	856136	64.56%	9.235%
84	11.963	3395	3397	3400	rBV2	393	245	0.02%	0.003%
85	12.188	3463	3467	3469	rBV2	619	537	0.04%	0.006%
86	12.400	3530	3533	3540	rBV2	525	495	0.04%	0.005%
87	12.496	3561	3563	3567	rVB	326	152	0.01%	0.002%
88	12.561	3581	3583	3585	rBV	297	134	0.01%	0.001%
89	12.583	3588	3590	3591	rBV	544	192	0.01%	0.002%
90	12.625	3601	3603	3605	rBV	289	177	0.01%	0.002%
91	12.776	3648	3650	3651	rBV	321	132	0.01%	0.001%
92	13.075	3741	3743	3744	rBV	363	167	0.01%	0.002%
93	13.172	3771	3773	3779	rVB	518	385	0.03%	0.004%
94	13.204	3779	3783	3790	rBV5	1437	1889	0.14%	0.020%
95	13.368	3832	3834	3836	rBV	401	168	0.01%	0.002%
96	13.406	3844	3846	3849	rBV2	320	172	0.01%	0.002%
97	13.512	3876	3879	3885	rVB3	537	522	0.04%	0.006%
98	13.683	3929	3932	3933	rBV	670	357	0.03%	0.004%
99	14.091	4057	4059	4062	rVB3	442	222	0.02%	0.002%
100	14.384	4148	4150	4153	rVB	481	183	0.01%	0.002%




Sum of corrected areas: 9270331

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033033.D
Acq On : 20 Nov 2023 19:45
Operator : SY/MD
Sample : 05436-11 10X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

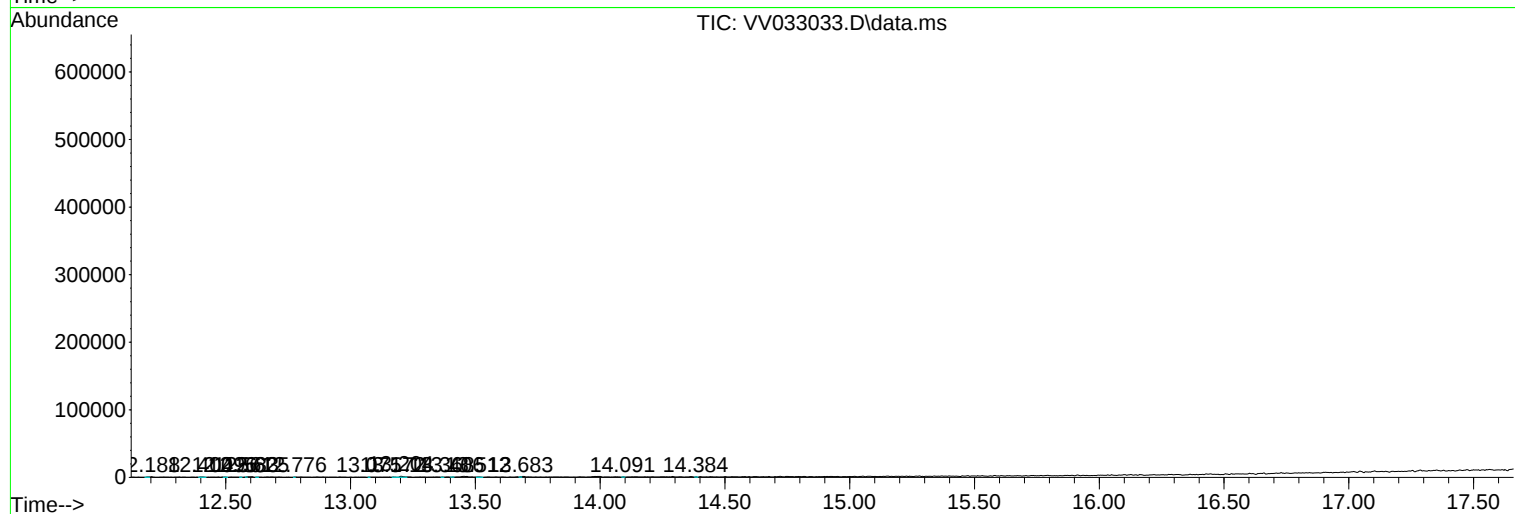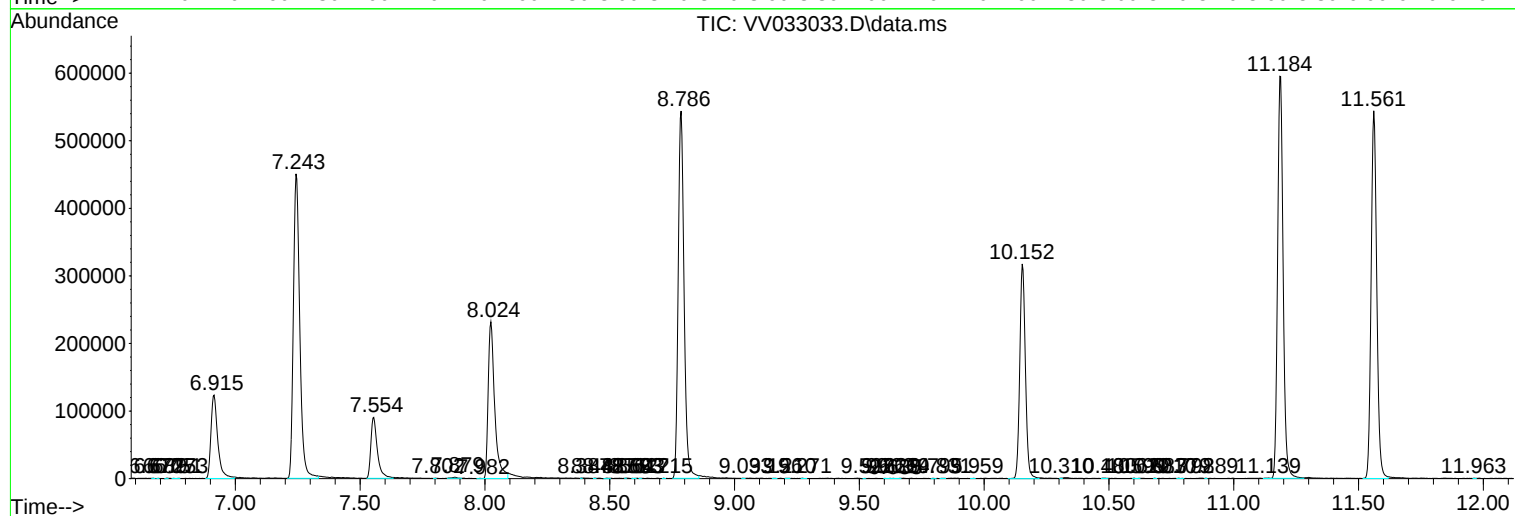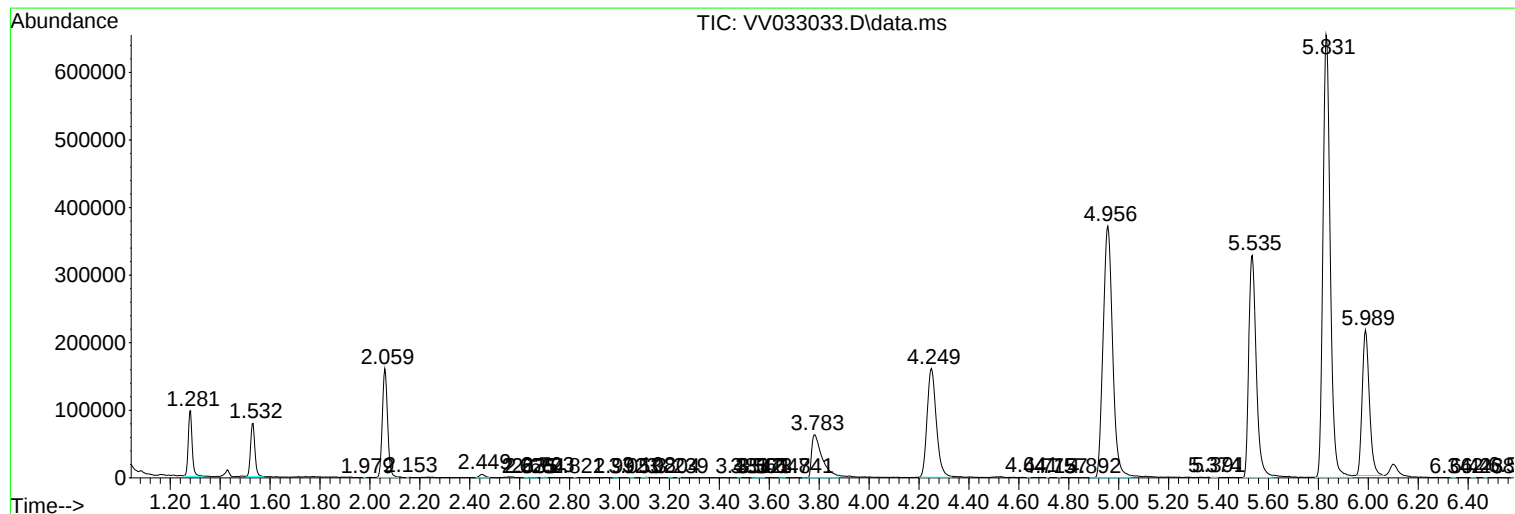

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033033.D
Acq On : 20 Nov 2023 19:45
Operator : SY/MD
Sample : 05436-11 10X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033033.D
Acq On : 20 Nov 2023 19:45
Operator : SY/MD
Sample : 05436-11 10X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc