

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033034.D
 Acq On : 20 Nov 2023 20:08
 Operator : SY/MD
 Sample : VIBLK253
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK253

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	86133	90839	10.40%	1.254%
2	1.420	112	118	125	rVB5	4446	4866	0.56%	0.067%
3	1.532	146	153	172	rVB	74821	89816	10.28%	1.239%
4	1.953	283	284	286	rBV	327	128	0.01%	0.002%
5	2.059	306	317	332	rBV	131075	191979	21.97%	2.649%
6	2.214	362	365	367	rBV2	724	568	0.07%	0.008%
7	2.448	430	438	450	rVB3	6913	11246	1.29%	0.155%
8	2.497	450	453	454	rBV2	220	127	0.01%	0.002%
9	2.542	463	467	468	rBV2	800	568	0.07%	0.008%
10	2.725	522	524	527	rBV2	281	179	0.02%	0.002%
11	2.802	545	548	550	rBV2	250	143	0.02%	0.002%
12	2.940	590	591	594	rBV2	257	143	0.02%	0.002%
13	2.966	596	599	601	rBV	258	173	0.02%	0.002%
14	3.002	605	610	613	rBV	313	316	0.04%	0.004%
15	3.156	656	658	662	rBV	411	393	0.04%	0.005%
16	3.220	673	678	680	rBV2	387	259	0.03%	0.004%
17	3.288	697	699	702	rVB	416	247	0.03%	0.003%
18	3.313	703	707	710	rBV	324	282	0.03%	0.004%
19	3.426	740	742	746	rBV2	245	172	0.02%	0.002%
20	3.477	755	758	764	rVB2	275	217	0.02%	0.003%
21	3.513	764	769	773	rBV3	368	345	0.04%	0.005%
22	3.555	778	782	785	rBV2	265	249	0.03%	0.003%
23	3.584	788	791	794	rVB2	192	125	0.01%	0.002%
24	3.596	794	795	799	rBV	262	135	0.02%	0.002%
25	3.783	841	853	881	rBV	65701	182403	20.88%	2.517%
26	4.133	960	962	965	rVB3	833	426	0.05%	0.006%
27	4.249	982	998	1023	rBV2	150339	387204	44.32%	5.343%
28	4.513	1077	1080	1082	rBV2	733	564	0.06%	0.008%
29	4.593	1100	1105	1109	rBV2	731	783	0.09%	0.011%
30	4.612	1109	1111	1113	rBV	506	294	0.03%	0.004%
31	4.667	1126	1128	1130	rBV2	318	214	0.02%	0.003%
32	4.706	1138	1140	1143	rVB2	547	262	0.03%	0.004%
33	4.764	1155	1158	1160	rBV	278	176	0.02%	0.002%
34	4.879	1191	1194	1196	rBV	363	217	0.02%	0.003%
35	4.956	1202	1218	1251	rBV2	325254	873639	100.00%	12.056%
36	5.371	1345	1347	1349	rBV2	636	296	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112023\
 Data File : VW033034.D
 Acq On : 20 Nov 2023 20:08
 Operator : SY/MD
 Sample : VIBLK253
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK253

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	5.410	1357	1359	1364	rVB3	504	289	0.03%	0.004%
38	5.436	1364	1367	1370	rBV	451	333	0.04%	0.005%
39	5.535	1382	1398	1425	rBV	315823	658115	75.33%	9.082%
40	5.834	1479	1491	1507	rVB6	10757	25434	2.91%	0.351%
41	5.989	1517	1539	1560	rBV	194595	404168	46.26%	5.577%
42	6.252	1617	1621	1625	rVB3	585	481	0.06%	0.007%
43	6.394	1662	1665	1670	rBV2	377	312	0.04%	0.004%
44	6.574	1717	1721	1722	rBV	239	124	0.01%	0.002%
45	6.638	1739	1741	1746	rVB2	385	302	0.03%	0.004%
46	6.915	1808	1827	1848	rBV	108505	204463	23.40%	2.821%
47	7.143	1896	1898	1899	rBV	524	250	0.03%	0.003%
48	7.185	1909	1911	1913	rBV	578	266	0.03%	0.004%
49	7.246	1918	1930	1956	rBV	353426	634363	72.61%	8.754%
50	7.554	2016	2026	2052	rBV	78980	145670	16.67%	2.010%
51	7.837	2110	2114	2118	rBV	422	303	0.03%	0.004%
52	7.853	2118	2119	2120	rBV	542	179	0.02%	0.002%
53	8.024	2163	2172	2193	rBV	229968	408588	46.77%	5.638%
54	8.361	2268	2277	2287	rBV5	3699	6965	0.80%	0.096%
55	8.451	2303	2305	2308	rBV	426	200	0.02%	0.003%
56	8.484	2313	2315	2318	rBV2	420	189	0.02%	0.003%
57	8.516	2322	2325	2329	rBV3	488	430	0.05%	0.006%
58	8.596	2347	2350	2352	rBV	260	185	0.02%	0.003%
59	8.686	2375	2378	2385	rVB2	434	401	0.05%	0.006%
60	8.728	2385	2391	2393	rBV3	544	454	0.05%	0.006%
61	8.786	2398	2409	2434	rBV	511222	838871	96.02%	11.576%
62	9.053	2490	2492	2494	rBV2	340	179	0.02%	0.002%
63	9.078	2499	2500	2503	rBV	330	167	0.02%	0.002%
64	9.123	2512	2514	2517	rBV	444	220	0.03%	0.003%
65	9.291	2564	2566	2570	rVB2	548	345	0.04%	0.005%
66	9.365	2588	2589	2591	rBV2	354	165	0.02%	0.002%
67	9.480	2623	2625	2627	rBV2	409	225	0.03%	0.003%
68	9.532	2639	2641	2644	rBV	552	427	0.05%	0.006%
69	9.924	2759	2763	2765	rBV	371	248	0.03%	0.003%
70	9.966	2773	2776	2777	rBV	227	130	0.01%	0.002%
71	10.024	2792	2794	2797	rBV	362	242	0.03%	0.003%
72	10.152	2823	2834	2859	rVV	300661	477873	54.70%	6.594%
73	10.377	2901	2904	2907	rBV	371	306	0.04%	0.004%
74	10.416	2913	2916	2921	rBV	443	481	0.06%	0.007%
75	10.580	2961	2967	2969	rBV	281	315	0.04%	0.004%
76	10.747	3016	3019	3021	rBV	271	181	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033034.D
 Acq On : 20 Nov 2023 20:08
 Operator : SY/MD
 Sample : VIBLK253
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK253

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	10.786	3028	3031	3032	rBV	301	163	0.02%	0.002%
78	10.815	3036	3040	3043	rBV2	354	292	0.03%	0.004%
79	10.860	3052	3054	3058	rVB2	482	332	0.04%	0.005%
80	11.188	3145	3156	3182	rBV	540388	839580	96.10%	11.586%
81	11.461	3239	3241	3244	rBV	341	272	0.03%	0.004%
82	11.490	3247	3250	3255	rBV2	396	360	0.04%	0.005%
83	11.561	3261	3272	3291	rBV	477791	746932	85.50%	10.307%
84	11.979	3400	3402	3404	rBV	420	244	0.03%	0.003%
85	12.020	3413	3415	3416	rBV	382	148	0.02%	0.002%
86	12.178	3461	3464	3465	rBV2	235	136	0.02%	0.002%
87	12.194	3465	3469	3472	rBV4	786	731	0.08%	0.010%
88	12.226	3477	3479	3480	rBV	310	148	0.02%	0.002%
89	12.339	3510	3514	3515	rBV	378	249	0.03%	0.003%
90	12.638	3605	3607	3611	rBV2	333	276	0.03%	0.004%
91	12.696	3621	3625	3628	rBV2	463	402	0.05%	0.006%
92	12.776	3648	3650	3652	rBV2	407	138	0.02%	0.002%
93	12.847	3669	3672	3676	rVB3	620	453	0.05%	0.006%
94	13.014	3721	3724	3728	rBV2	660	421	0.05%	0.006%
95	13.123	3756	3758	3763	rBV	249	167	0.02%	0.002%
96	13.496	3871	3874	3879	rBV2	578	506	0.06%	0.007%
97	13.618	3909	3912	3914	rBV3	488	290	0.03%	0.004%
98	13.972	4017	4022	4023	rBV2	601	496	0.06%	0.007%
99	14.294	4119	4122	4123	rBV	742	427	0.05%	0.006%
100	15.358	4450	4453	4456	rBV2	1196	726	0.08%	0.010%




Sum of corrected areas: 7246721

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033034.D
Acq On : 20 Nov 2023 20:08
Operator : SY/MD
Sample : VIBLK253
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

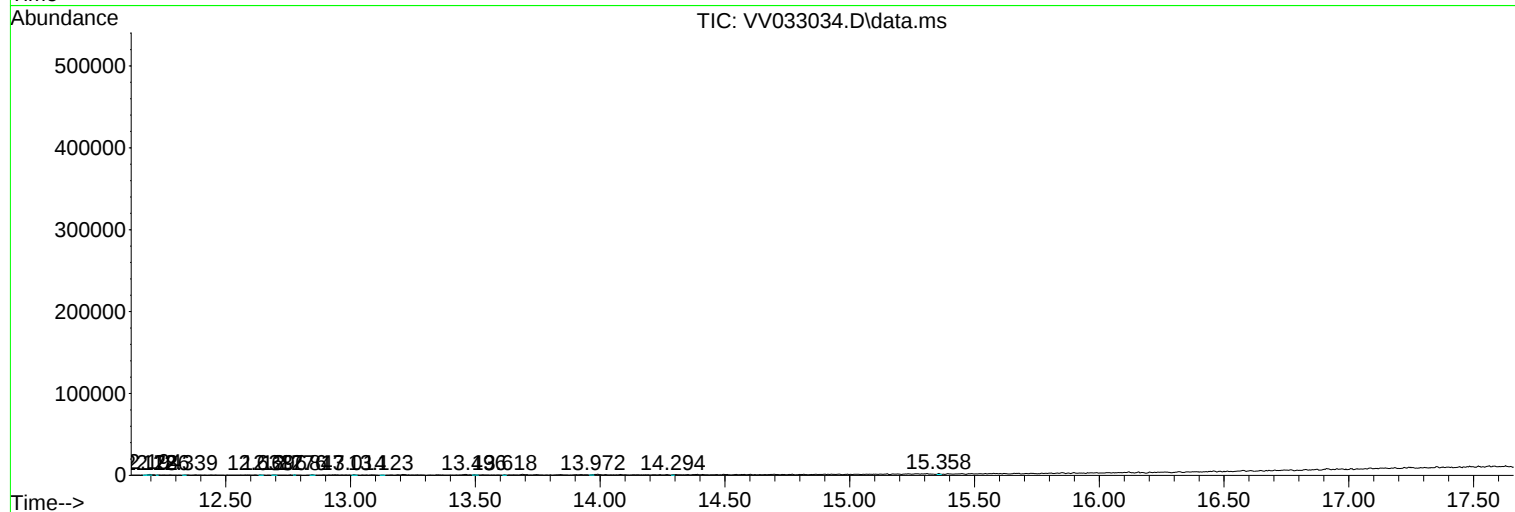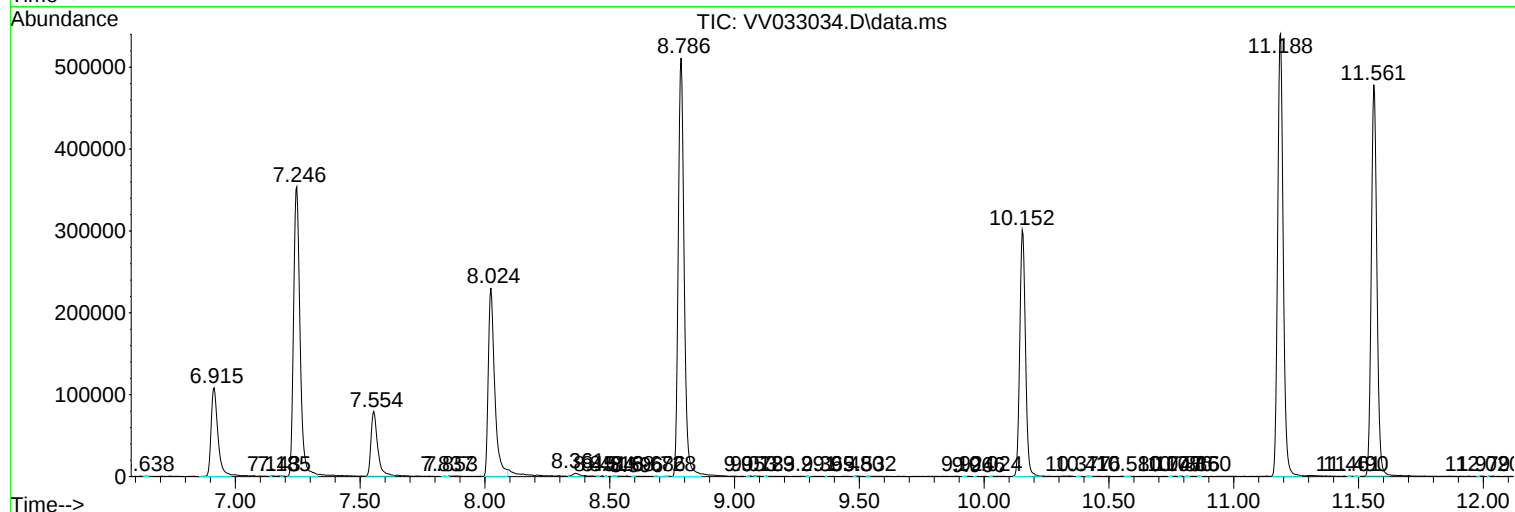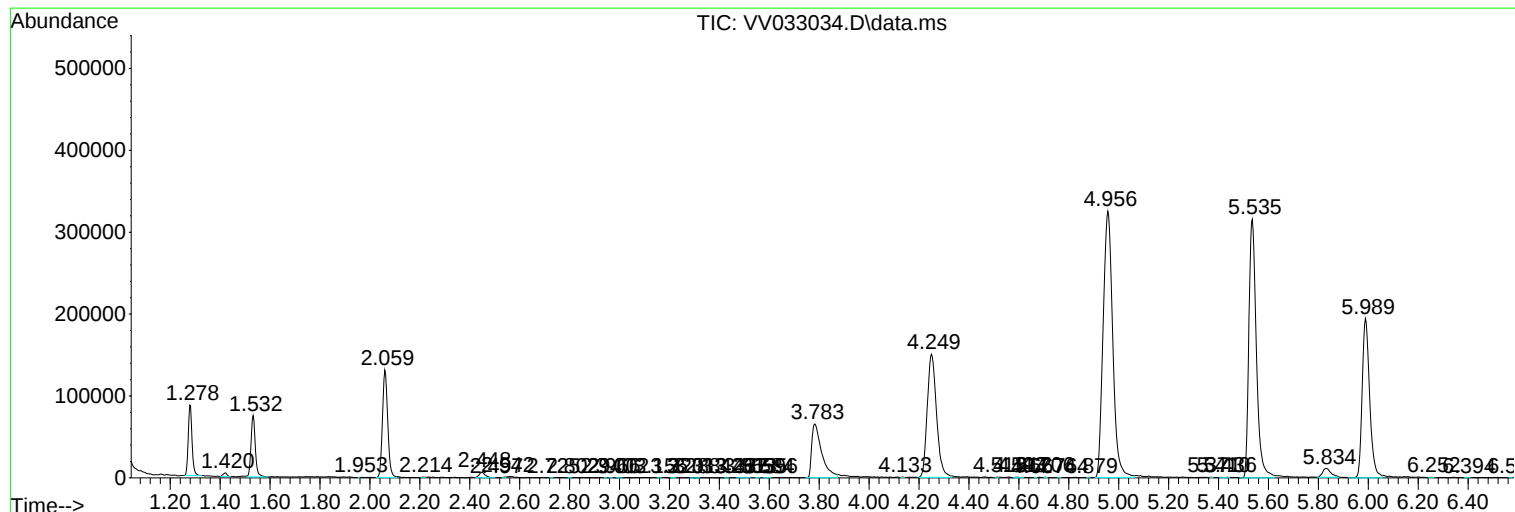

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033034.D
Acq On : 20 Nov 2023 20:08
Operator : SY/MD
Sample : VIBLK253
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033034.D
Acq On : 20 Nov 2023 20:08
Operator : SY/MD
Sample : VIBLK253
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc