

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033035.D
 Acq On : 20 Nov 2023 20:31
 Operator : SY/MD
 Sample : 05436-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1C1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M

Title : VOC Analysis

Signal : TIC: VV033035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	109129	115609	11.99%	1.442%
2	1.532	146	153	168	rVB	84818	101012	10.48%	1.260%
3	1.963	286	287	290	rVB2	447	198	0.02%	0.002%
4	1.998	296	298	302	rBV2	512	345	0.04%	0.004%
5	2.060	306	317	338	rBV	166055	243379	25.25%	3.037%
6	2.162	347	349	352	rVB2	422	208	0.02%	0.003%
7	2.269	379	382	384	rBV3	310	188	0.02%	0.002%
8	2.388	417	419	422	rVB	363	164	0.02%	0.002%
9	2.452	432	439	445	rVB4	1748	2372	0.25%	0.030%
10	2.516	457	459	463	rVB2	384	217	0.02%	0.003%
11	2.561	470	473	477	rVB2	464	376	0.04%	0.005%
12	2.806	545	549	555	rBV2	296	371	0.04%	0.005%
13	2.928	584	587	588	rBV	299	134	0.01%	0.002%
14	2.944	588	592	593	rVV2	221	147	0.02%	0.002%
15	3.047	621	624	626	rBV	340	136	0.01%	0.002%
16	3.121	644	647	651	rVV2	678	474	0.05%	0.006%
17	3.201	667	672	673	rBV	262	184	0.02%	0.002%
18	3.230	679	681	683	rBV	220	141	0.01%	0.002%
19	3.256	687	689	691	rBV	237	140	0.01%	0.002%
20	3.381	725	728	731	rVB3	449	212	0.02%	0.003%
21	3.429	739	743	745	rBV	319	331	0.03%	0.004%
22	3.564	781	785	787	rVB	160	123	0.01%	0.002%
23	3.648	808	811	816	rBV2	355	433	0.04%	0.005%
24	3.722	833	834	838	rBB	237	143	0.01%	0.002%
25	3.783	841	853	890	rBV	61972	173503	18.00%	2.165%
26	4.249	982	998	1028	rBV	167973	429367	44.54%	5.357%
27	4.487	1069	1072	1074	rBV2	604	393	0.04%	0.005%
28	4.584	1099	1102	1105	rBV3	518	396	0.04%	0.005%
29	4.651	1121	1123	1130	rBV2	380	247	0.03%	0.003%
30	4.767	1156	1159	1163	rBV3	466	376	0.04%	0.005%
31	4.879	1189	1194	1197	rBV2	418	331	0.03%	0.004%
32	4.957	1201	1218	1245	rBV2	360949	963982	100.00%	12.028%
33	5.310	1326	1328	1331	rBV2	379	184	0.02%	0.002%
34	5.420	1360	1362	1368	rVB4	707	403	0.04%	0.005%
35	5.535	1386	1398	1420	rBV	337288	692279	71.81%	8.638%
36	5.838	1479	1492	1512	rBV6	37828	87566	9.08%	1.093%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112023\
 Data File : VW033035.D
 Acq On : 20 Nov 2023 20:31
 Operator : SY/MD
 Sample : 05436-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1C1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	5.989	1525	1539	1569	rBV	210175	440280	45.67%	5.494%
38	6.307	1636	1638	1645	rVB3	495	382	0.04%	0.005%
39	6.339	1645	1648	1650	rBV	243	155	0.02%	0.002%
40	6.596	1725	1728	1730	rBV2	324	195	0.02%	0.002%
41	6.625	1735	1737	1740	rBV2	607	335	0.03%	0.004%
42	6.641	1740	1742	1743	rBV	418	173	0.02%	0.002%
43	6.693	1754	1758	1762	rBV2	341	344	0.04%	0.004%
44	6.860	1806	1810	1813	rBV	345	333	0.03%	0.004%
45	6.915	1816	1827	1851	rBV	121203	225384	23.38%	2.812%
46	7.108	1885	1887	1891	rBV3	504	427	0.04%	0.005%
47	7.243	1915	1929	1949	rBV	416802	737866	76.54%	9.207%
48	7.555	2016	2026	2046	rBV	86670	156818	16.27%	1.957%
49	7.876	2118	2126	2140	rVB3	3887	6819	0.71%	0.085%
50	7.966	2152	2154	2158	rBV	372	174	0.02%	0.002%
51	8.024	2162	2172	2190	rBV	234040	412395	42.78%	5.146%
52	8.313	2258	2262	2265	rBV2	545	493	0.05%	0.006%
53	8.394	2285	2287	2290	rBV	424	300	0.03%	0.004%
54	8.436	2298	2300	2302	rVB	489	207	0.02%	0.003%
55	8.448	2302	2304	2306	rBV	311	200	0.02%	0.002%
56	8.509	2319	2323	2328	rBV2	444	467	0.05%	0.006%
57	8.574	2339	2343	2346	rBV2	303	193	0.02%	0.002%
58	8.638	2361	2363	2368	rVB2	392	251	0.03%	0.003%
59	8.786	2397	2409	2428	rBV	544433	895323	92.88%	11.171%
60	8.998	2473	2475	2477	rVB	519	181	0.02%	0.002%
61	9.075	2497	2499	2500	rBV	508	188	0.02%	0.002%
62	9.127	2513	2515	2518	rBV2	387	195	0.02%	0.002%
63	9.153	2521	2523	2526	rVB2	255	149	0.02%	0.002%
64	9.188	2531	2534	2537	rVB	309	184	0.02%	0.002%
65	9.210	2537	2541	2545	rBV4	558	585	0.06%	0.007%
66	9.265	2554	2558	2561	rBV3	568	473	0.05%	0.006%
67	9.323	2573	2576	2579	rBV2	316	270	0.03%	0.003%
68	9.342	2579	2582	2583	rBV2	185	124	0.01%	0.002%
69	9.413	2601	2604	2606	rBV	474	276	0.03%	0.003%
70	9.490	2626	2628	2630	rBV	527	286	0.03%	0.004%
71	9.561	2648	2650	2654	rBV2	304	225	0.02%	0.003%
72	9.699	2690	2693	2696	rBV3	344	245	0.03%	0.003%
73	9.873	2744	2747	2748	rBV	462	212	0.02%	0.003%
74	10.085	2811	2813	2814	rBV	361	130	0.01%	0.002%
75	10.152	2821	2834	2859	rBV	329267	510746	52.98%	6.373%
76	10.326	2880	2888	2897	rBV4	4218	6829	0.71%	0.085%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
 Data File : VV033035.D
 Acq On : 20 Nov 2023 20:31
 Operator : SY/MD
 Sample : 05436-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1C1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	10.419	2913	2917	2921	rBV3	565	530	0.05%	0.007%
78	10.570	2960	2964	2967	rBV	323	289	0.03%	0.004%
79	10.956	3080	3084	3085	rBV	391	297	0.03%	0.004%
80	11.056	3111	3115	3119	rBV3	350	380	0.04%	0.005%
81	11.117	3132	3134	3135	rBV3	352	149	0.02%	0.002%
82	11.127	3135	3137	3141	rVV2	585	376	0.04%	0.005%
83	11.185	3143	3155	3182	rBV	587980	921926	95.64%	11.503%
84	11.394	3215	3220	3224	rBV2	533	575	0.06%	0.007%
85	11.468	3240	3243	3245	rBV	386	268	0.03%	0.003%
86	11.561	3258	3272	3296	rBV	552850	867331	89.97%	10.822%
87	11.773	3336	3338	3343	rBV3	443	421	0.04%	0.005%
88	12.194	3465	3469	3483	rVB4	1427	1947	0.20%	0.024%
89	12.304	3501	3503	3505	rBV	370	205	0.02%	0.003%
90	12.342	3513	3515	3516	rBV	399	180	0.02%	0.002%
91	12.493	3560	3562	3567	rVB	455	276	0.03%	0.003%
92	12.519	3567	3570	3571	rBV	287	157	0.02%	0.002%
93	12.783	3649	3652	3653	rBV	233	142	0.01%	0.002%
94	12.831	3665	3667	3669	rBV3	550	251	0.03%	0.003%
95	12.969	3708	3710	3711	rBV2	391	168	0.02%	0.002%
96	13.049	3733	3735	3738	rVB2	423	214	0.02%	0.003%
97	13.082	3743	3745	3746	rBV	400	178	0.02%	0.002%
98	13.329	3819	3822	3825	rBV2	483	383	0.04%	0.005%
99	13.696	3931	3936	3940	rBV4	736	698	0.07%	0.009%
100	14.438	4165	4167	4170	rBV2	509	303	0.03%	0.004%




Sum of corrected areas: 8014520

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033035.D
Acq On : 20 Nov 2023 20:31
Operator : SY/MD
Sample : 05436-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1C1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

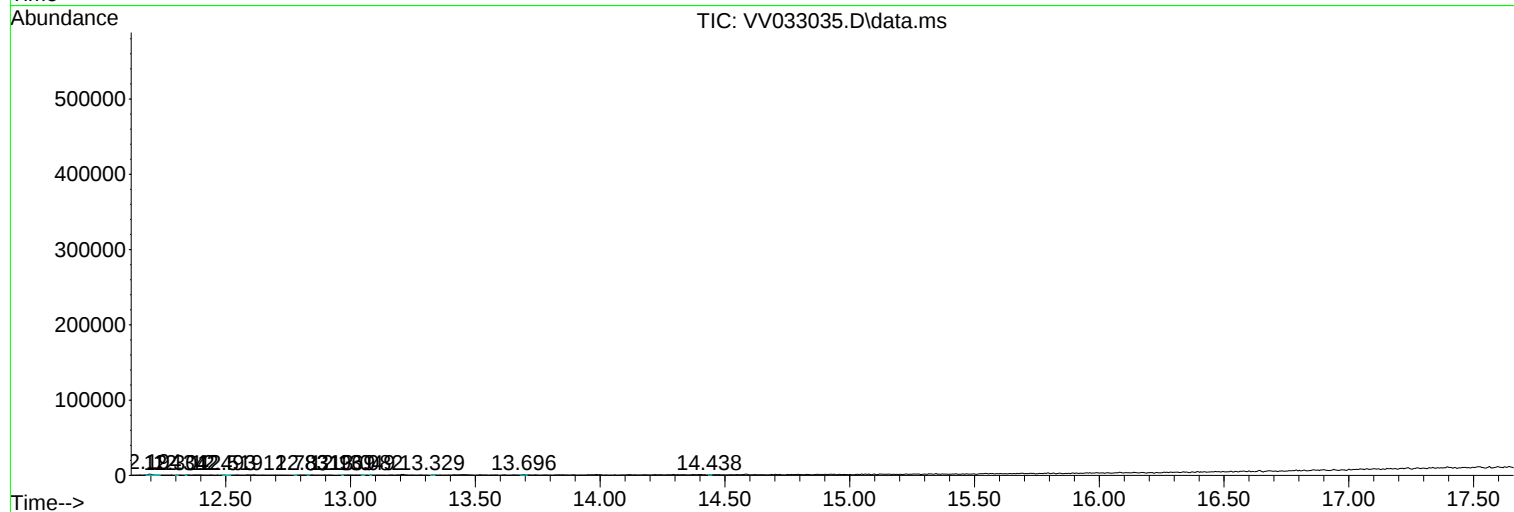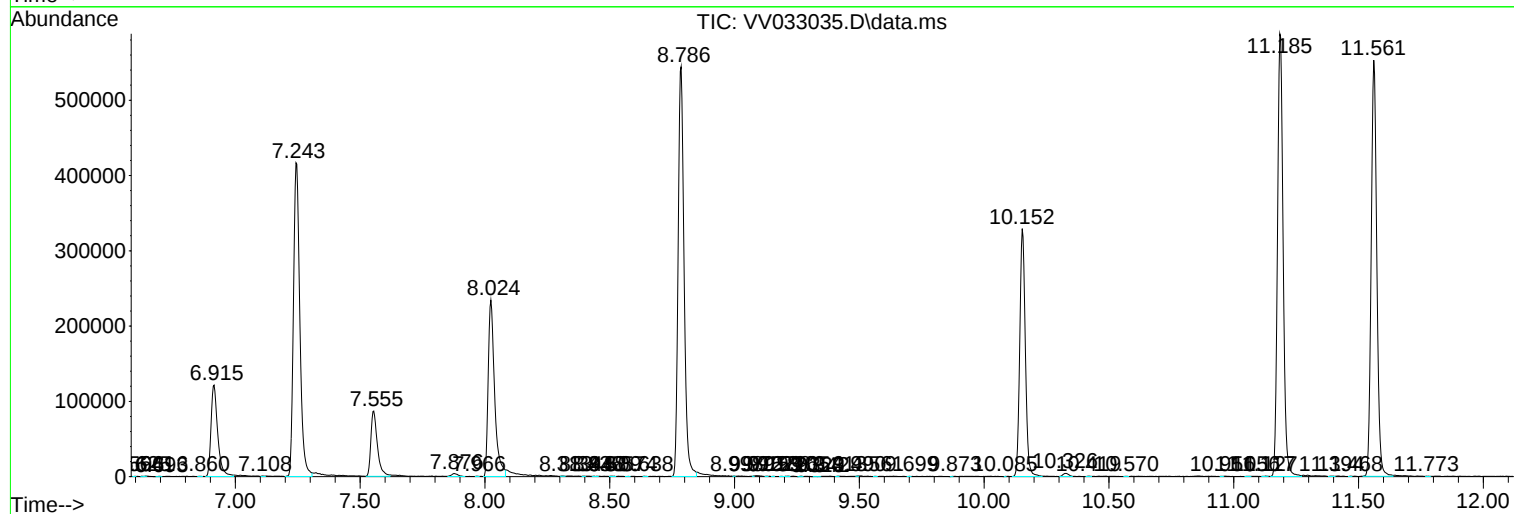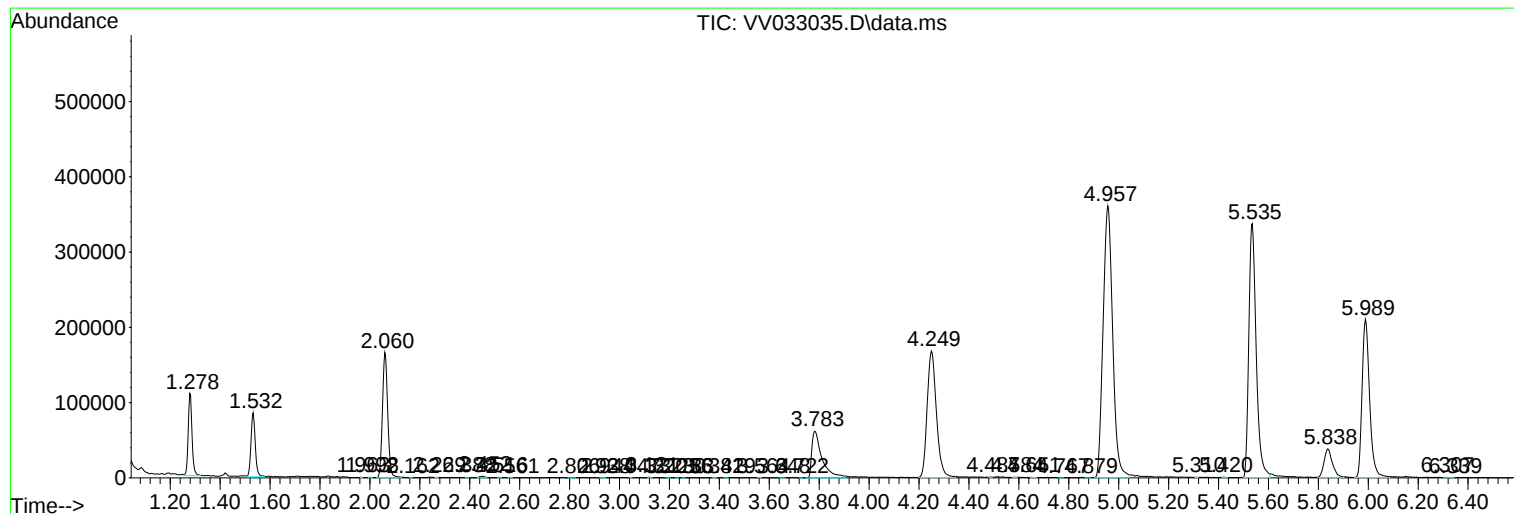

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033035.D
Acq On : 20 Nov 2023 20:31
Operator : SY/MD
Sample : 05436-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1C1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033035.D
Acq On : 20 Nov 2023 20:31
Operator : SY/MD
Sample : 05436-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1C1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------