


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112023\
Data File : VV033011.D
Acq On : 20 Nov 2023 08:40
Operator : SY/MD
Sample : BFB234
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB234

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Title : VOC Analysis
Last Update : Mon Nov 20 23:40:05 2023

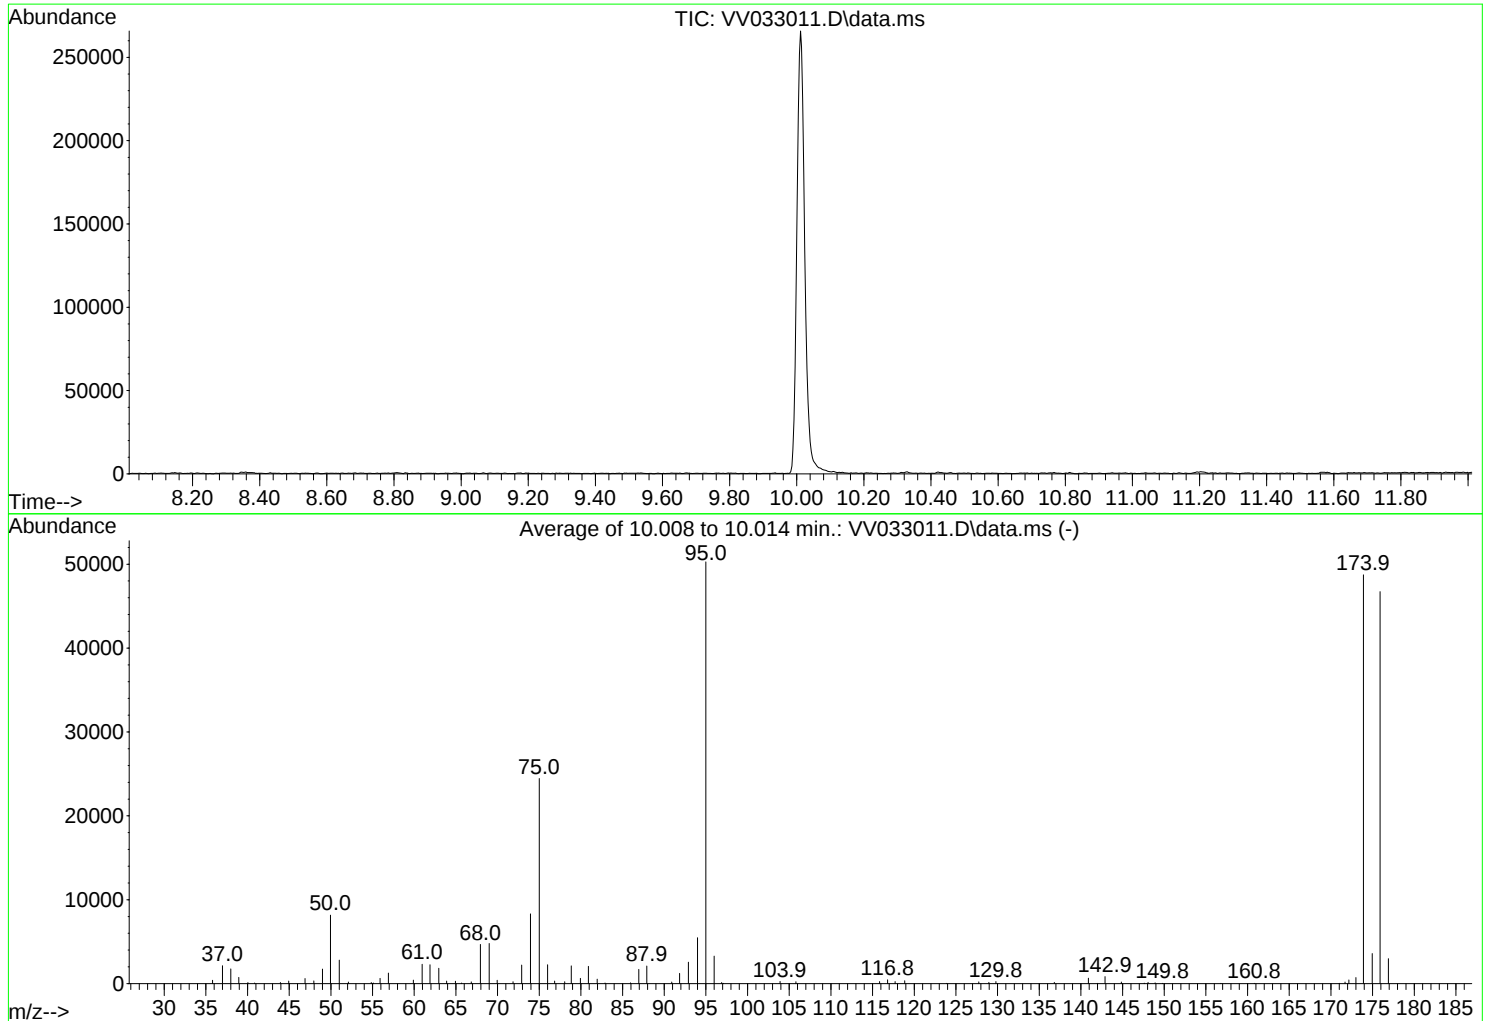

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	8158	PASS
75	95	30	80	48.6	24461	PASS
95	95	100	100	100.0	50280	PASS
96	95	5	9	6.5	3285	PASS
173	174	0.00	2	1.5	726	PASS
174	95	50	120	96.9	48739	PASS
175	174	5	9	7.3	3578	PASS
176	174	95	105	95.9	46725	PASS
177	176	5	10	6.4	2981	PASS

m/z	Abundance
39.80	156.0
43.90	224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
35.80	398.0
37.00	2177.0
38.00	1771.0
39.00	839.0
40.10	166.0
44.00	334.0
44.90	284.0
46.90	571.0
48.00	287.0
49.00	1670.0
49.90	8206.0
51.00	2947.0
52.10	182.0
54.80	205.0
55.90	561.0
56.90	1309.0
59.90	420.0
61.00	2332.0
61.90	2274.0
62.90	1764.0
63.90	331.0
65.00	243.0
66.80	208.0
67.90	4559.0
69.00	4765.0
70.00	356.0
71.80	247.0
72.90	2237.0
73.90	8289.0
75.00	23368.0
76.00	2274.0
76.80	284.0
78.10	205.0
78.90	2135.0
79.90	600.0
80.90	2051.0
82.00	464.0
82.90	136.0
86.00	107.0
86.90	1586.0
87.90	1976.0
90.90	192.0
91.90	1255.0
92.90	2539.0
94.00	5393.0
95.00	49968.0
96.00	3201.0
96.90	117.0
97.10	118.0
103.90	241.0
105.80	199.0
115.80	265.0
116.80	407.0
117.70	252.0
118.80	300.0
127.70	237.0
129.00	168.0
129.80	225.0
136.80	134.0
140.90	567.0
142.00	117.0
142.90	843.0
144.90	222.0
147.60	151.0
148.10	139.0
148.90	171.0
172.10	414.0
173.00	656.0
173.90	47216.0
174.90	3526.0
175.90	44472.0
176.90	3058.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
35.80	421.0
37.00	2224.0
38.00	1780.0
39.00	766.0
40.10	145.0
40.80	104.0
44.00	364.0
45.00	322.0
46.90	644.0
47.90	312.0
49.00	1772.0
50.00	8455.0
51.00	2881.0
52.10	194.0
54.90	196.0
55.90	640.0
56.90	1309.0
59.90	440.0
60.90	2368.0
61.90	2378.0
63.00	1856.0
63.90	311.0
65.00	285.0
65.70	104.0
66.90	205.0
67.90	4770.0
69.00	4849.0
70.00	417.0
71.80	215.0
72.90	2297.0
74.00	8602.0
75.00	25248.0
76.00	2359.0
76.90	295.0
78.10	239.0
78.80	2160.0
79.90	673.0
80.90	2129.0
81.90	575.0
82.90	100.0
86.00	103.0
87.00	1736.0
87.90	2190.0
90.90	189.0
91.80	1234.0
92.90	2632.0
94.00	5520.0
95.00	51656.0
96.00	3375.0
96.90	143.0
103.90	258.0
105.80	213.0
115.90	251.0
116.80	452.0
117.70	285.0
118.90	356.0
123.90	103.0
127.70	220.0
129.00	152.0
129.80	251.0
136.80	158.0
140.90	685.0
142.90	854.0
144.80	189.0
148.00	145.0
148.90	133.0
171.70	302.0
172.20	483.0
173.00	786.0
173.90	50440.0
174.90	3678.0
175.90	48280.0
176.90	2963.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
35.80	371.0
37.00	2030.0
38.00	1725.0
38.90	646.0
40.00	108.0
40.90	102.0
44.00	373.0
45.00	317.0
46.90	638.0
47.90	348.0
49.00	1770.0
50.00	7812.0
51.00	2566.0
52.10	181.0
55.10	216.0
55.90	668.0
56.90	1188.0
59.90	407.0
60.90	2222.0
61.90	2120.0
63.00	1904.0
63.90	251.0
64.90	320.0
65.70	102.0
66.90	197.0
68.00	4676.0
69.00	4737.0
69.90	412.0
71.90	206.0
72.90	2103.0
74.00	8085.0
75.00	24768.0
76.00	2148.0
76.90	323.0
78.00	218.0
78.80	2043.0
80.00	628.0
80.90	2006.0
81.90	593.0
85.90	103.0
87.00	1767.0
87.90	2135.0
90.90	164.0
91.90	1152.0
92.90	2503.0
94.00	5539.0
95.00	49216.0
96.00	3278.0
96.90	143.0
103.90	280.0
105.80	251.0
115.90	208.0
116.80	500.0
117.70	241.0
118.90	379.0
127.80	185.0
128.90	117.0
129.80	268.0
136.80	156.0
140.90	692.0
142.90	801.0
144.80	175.0
148.00	178.0
149.80	123.0
156.80	111.0
160.80	131.0
171.00	110.0
171.70	299.0
172.10	444.0
173.00	735.0
173.90	48560.0
175.00	3531.0
175.90	47424.0
176.90	2923.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234