
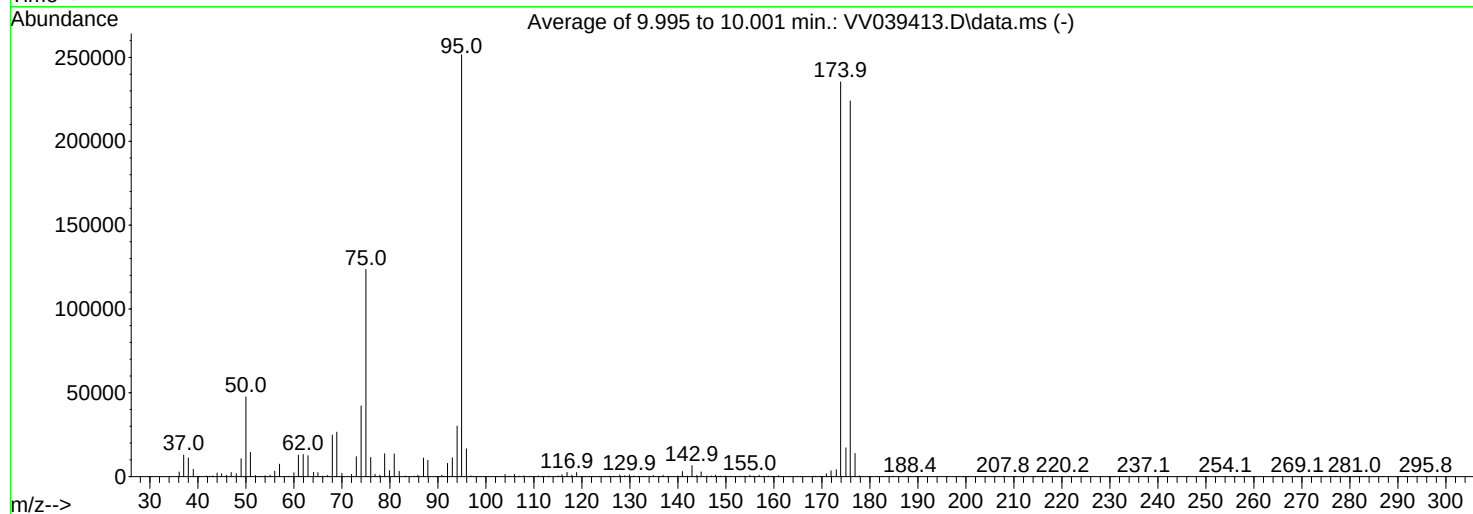


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112025\
Data File : VV039413.D
Acq On : 20 Nov 2025 08:07
Operator : SY/MD
Sample : BFB214
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB214

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111925WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 21 03:08:38 2025

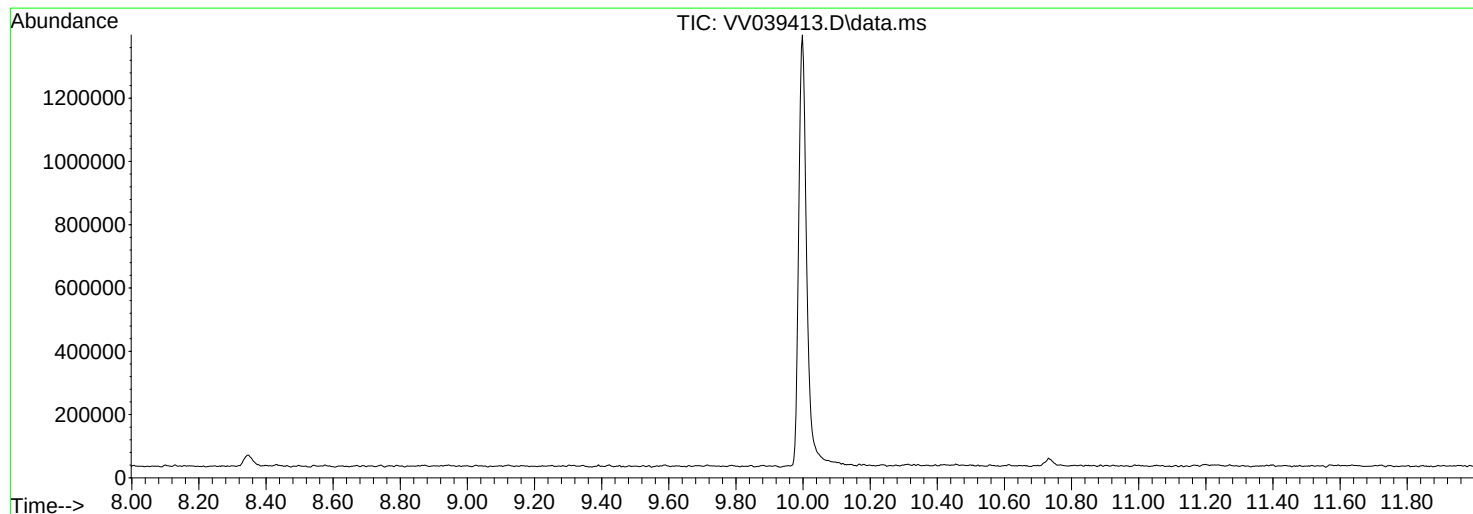

AutoFind: Scans 2785, 2786, 2787; Background Corrected with Scan 2770

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	47579	PASS
75	95	30	80	49.1	123557	PASS
95	95	100	100	100.0	251568	PASS
96	95	5	9	6.6	16596	PASS
173	174	0.00	2	1.7	4101	PASS
174	95	50	120	93.5	235328	PASS
175	174	5	9	7.3	17143	PASS
176	174	95	105	95.2	224003	PASS
177	176	5	10	6.2	13852	PASS