


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112118\
Data File : VV008688.D
Acq On : 21 Nov 2018 08:41
Operator : SY/MD
Sample : BFB01
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB01

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Nov 26 07:58:07 2018

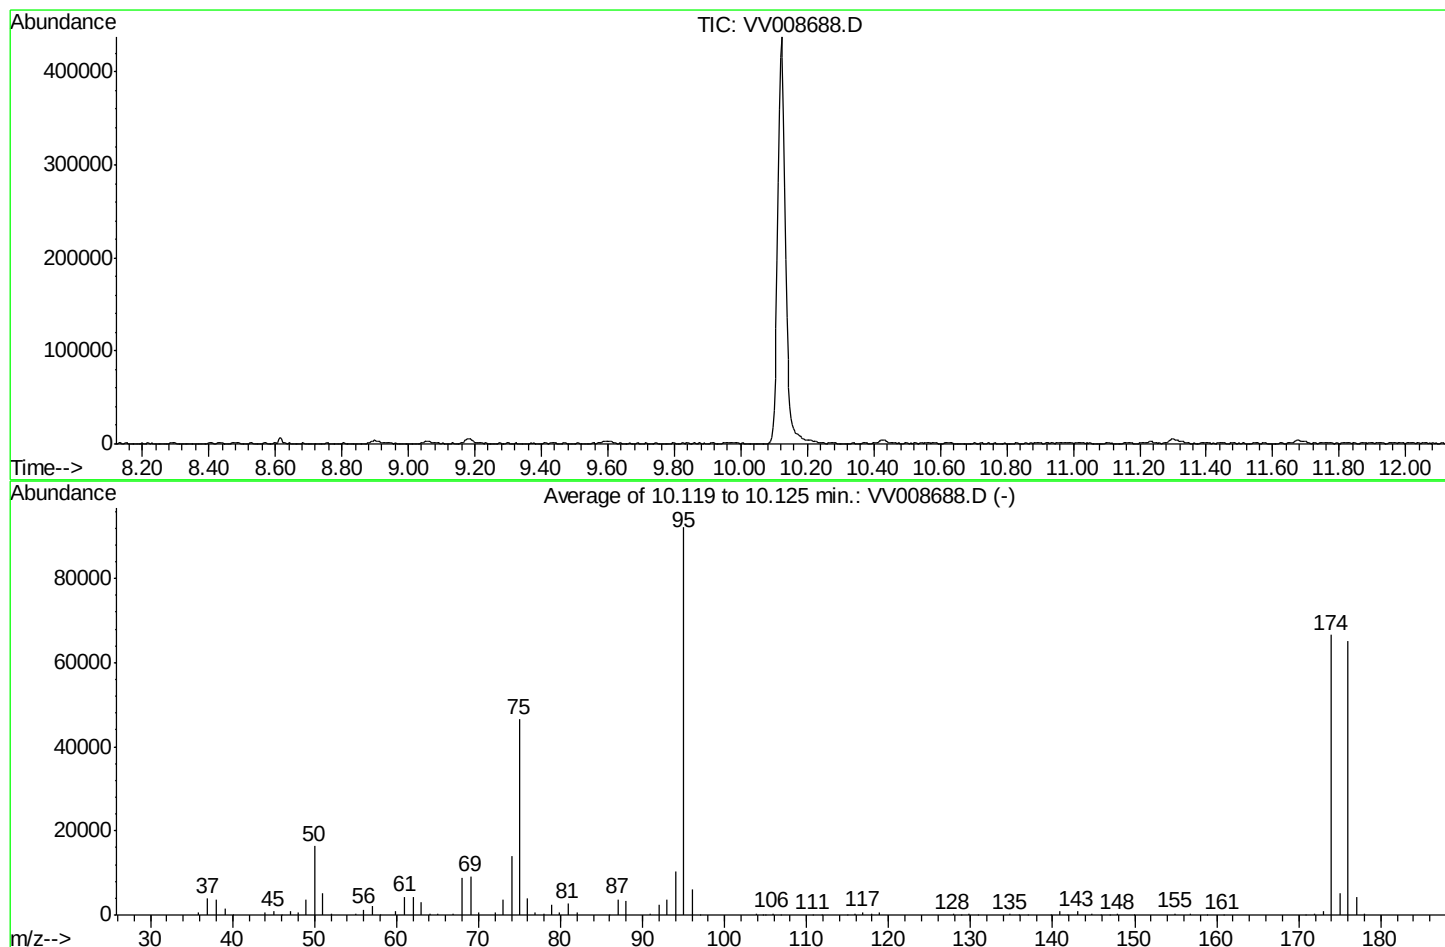

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	16347	PASS
75	95	30	80	50.5	46562	PASS
95	95	100	100	100.0	92176	PASS
96	95	5	9	6.6	6083	PASS
173	174	0.00	2	1.5	973	PASS
174	95	50	120	72.3	66621	PASS
175	174	5	9	7.6	5041	PASS
176	174	95	101	97.7	65064	PASS
177	176	5	9	6.7	4327	PASS

m/z	Abundance
40.00	302.0
44.00	306.0

Instrument :
MSVOA_V
ClientSampleId :
BFB01

m/z	Abundance
35.90	701.0
37.00	3769.0
38.00	3640.0
39.00	1407.0
40.00	390.0
44.00	911.0
45.00	886.0
46.00	128.0
47.00	988.0
48.00	582.0
49.00	3589.0
50.00	16220.0
51.00	5225.0
52.00	330.0
55.00	303.0
56.00	1202.0
57.00	2325.0
59.90	813.0
61.00	4417.0
62.00	4145.0
63.00	3041.0
64.00	365.0
65.00	275.0
66.90	315.0
68.00	8859.0
69.00	9097.0
70.00	676.0
72.00	522.0
73.00	3807.0
74.00	13759.0
75.00	46128.0
76.00	3796.0
76.90	586.0
77.90	372.0
78.90	2543.0
79.90	668.0
80.90	2581.0
82.00	577.0
87.00	3420.0
88.00	3181.0
90.90	312.0
92.00	2670.0
93.00	3700.0
94.00	10374.0
95.00	90504.0
96.00	6267.0
103.90	381.0
104.70	149.0
105.90	421.0
110.70	157.0
115.90	316.0
116.90	581.0
117.90	353.0
118.80	496.0
127.90	302.0
128.90	115.0
129.80	277.0
131.00	135.0
134.90	201.0
137.00	198.0
140.80	807.0
141.80	104.0
143.00	846.0
144.80	193.0
145.80	101.0
147.90	198.0
149.90	156.0
155.00	355.0
156.90	174.0
158.80	143.0
160.80	117.0
170.80	103.0
171.90	365.0
173.00	1006.0
174.00	64072.0
175.00	5006.0
176.00	63264.0
177.00	4265.0
178.00	186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB01

m/z	Abundance
35.90	722.0
37.00	3944.0
38.00	3687.0
39.00	1453.0
40.00	310.0
44.00	927.0
45.00	919.0
46.10	163.0
47.10	1064.0
47.90	579.0
49.00	3704.0
50.00	16928.0
51.00	5262.0
52.00	266.0
55.00	251.0
56.00	1288.0
57.00	2358.0
59.90	920.0
61.00	4533.0
62.00	4284.0
63.00	3243.0
64.00	418.0
65.00	311.0
67.00	364.0
68.00	9046.0
69.00	9290.0
70.00	645.0
72.00	487.0
73.00	3856.0
74.00	14362.0
75.00	48088.0
76.00	4031.0
76.90	653.0
78.00	387.0
78.90	2582.0
79.90	682.0
80.90	2733.0
81.90	566.0
86.00	105.0
87.00	3832.0
88.00	3338.0
90.90	298.0
92.00	2664.0
93.00	3829.0
94.00	10759.0
95.00	95448.0
96.00	6230.0
97.00	128.0
103.80	383.0
104.70	143.0
105.90	431.0
106.80	126.0
110.70	161.0
114.90	106.0
115.90	307.0
116.90	663.0
117.90	380.0
118.80	523.0
127.90	292.0
128.90	154.0
129.80	306.0
130.90	140.0
134.90	210.0
137.00	162.0
140.80	856.0
143.00	928.0
144.80	231.0
145.80	166.0
147.00	130.0
147.90	244.0
150.00	131.0
154.90	381.0
156.90	192.0
158.80	144.0
160.80	148.0
170.80	106.0
171.90	350.0
173.00	1032.0
174.00	68952.0
175.00	5227.0
176.00	67280.0
177.00	4519.0
178.00	177.0

Instrument :
MSVOA_V
ClientSampleId :
BFB01

m/z	Abundance
35.90	645.0
37.00	3785.0
38.00	3351.0
39.10	1326.0
40.00	215.0
44.00	898.0
45.00	782.0
46.10	146.0
47.10	949.0
47.90	449.0
49.00	3368.0
50.00	15893.0
51.00	4809.0
52.10	218.0
55.00	211.0
56.00	1280.0
57.00	2165.0
58.00	131.0
59.90	864.0
61.00	4156.0
62.00	3937.0
63.00	3120.0
64.10	383.0
65.00	317.0
67.00	324.0
68.00	8284.0
69.00	8736.0
70.00	577.0
72.00	434.0
73.00	3725.0
74.00	13861.0
75.00	45472.0
76.00	3977.0
76.90	662.0
78.00	388.0
78.90	2366.0
79.90	634.0
80.90	2612.0
81.90	550.0
87.00	3861.0
87.90	3228.0
91.00	255.0
92.00	2293.0
93.00	3573.0
94.00	10009.0
95.00	90576.0
96.00	5754.0
97.00	135.0
103.80	352.0
104.90	107.0
105.90	400.0
106.90	137.0
110.80	121.0
111.90	106.0
115.00	126.0
116.00	341.0
116.80	675.0
117.90	353.0
118.90	468.0
127.90	306.0
128.80	181.0
129.80	287.0
131.00	127.0
134.80	210.0
135.90	104.0
137.00	128.0
139.70	106.0
140.90	854.0
143.00	947.0
144.80	223.0
145.80	196.0
147.00	135.0
147.90	248.0
154.90	335.0
156.80	181.0
158.80	131.0
160.80	150.0
172.00	312.0
173.10	883.0
174.00	66840.0
175.00	4892.0
176.00	64648.0
177.00	4199.0
178.00	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB01