
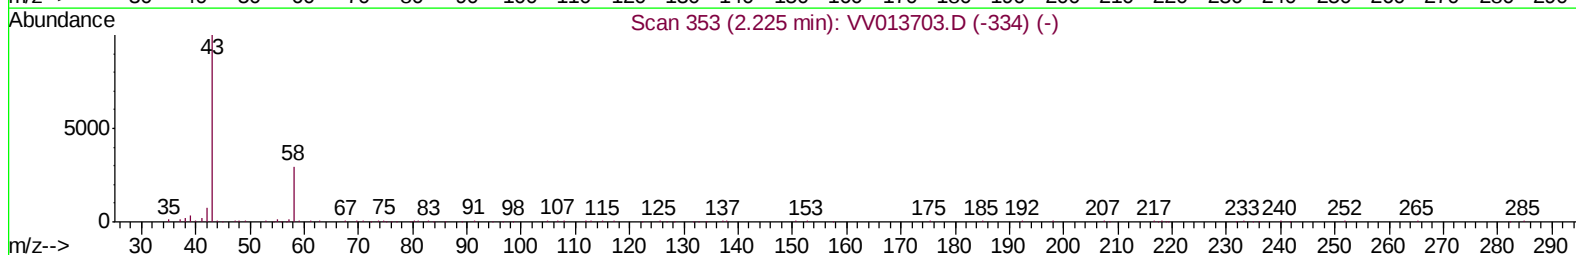
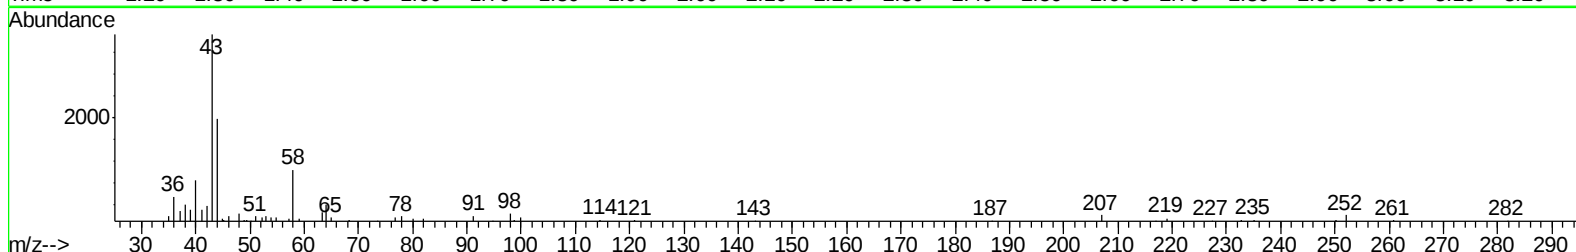


Data File : VV013714.D
Acq On : 21 Nov 2019 15:31
Operator : SY/MD
Sample : K5941-07 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Nov 22 03:59:39 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 22 03:55:18 2019
Response via : Initial Calibration

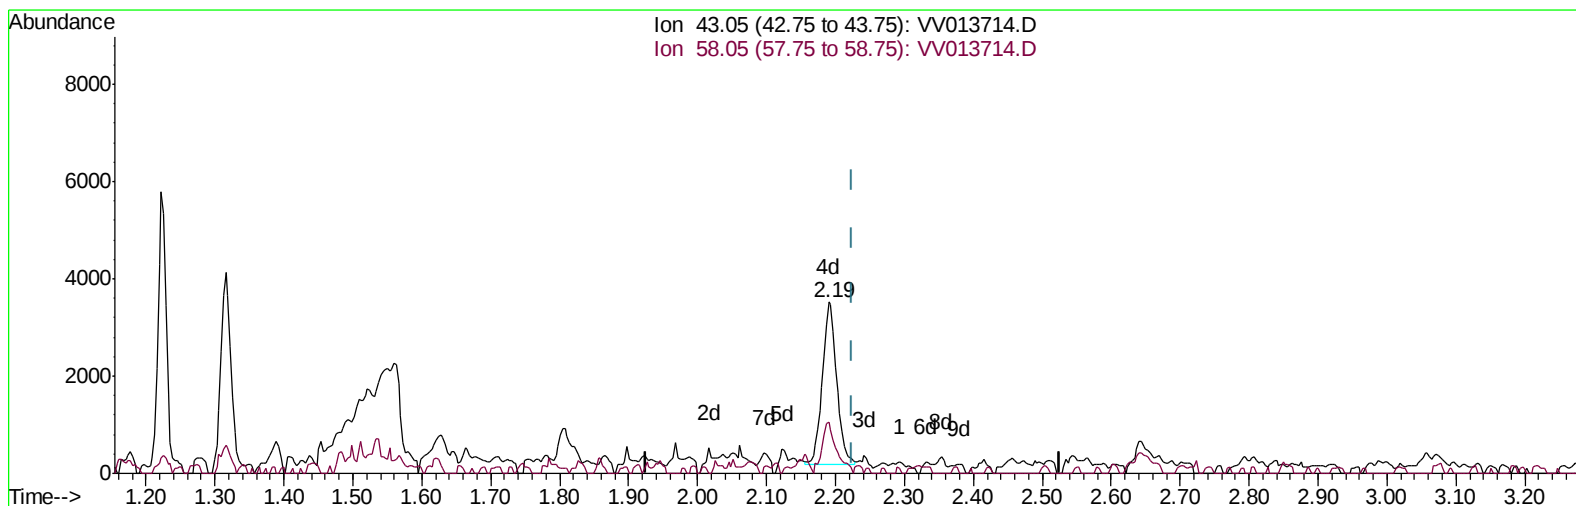

TIC: VV013714.D

(13) Acetone (T)

2.190min (-0.035) 1.56ug/L m

response 4767

Ion	Exp%	Act%
43.05	100	100
58.05	8.50	0.96
0.00	0.00	0.00
0.00	0.00	0.00