
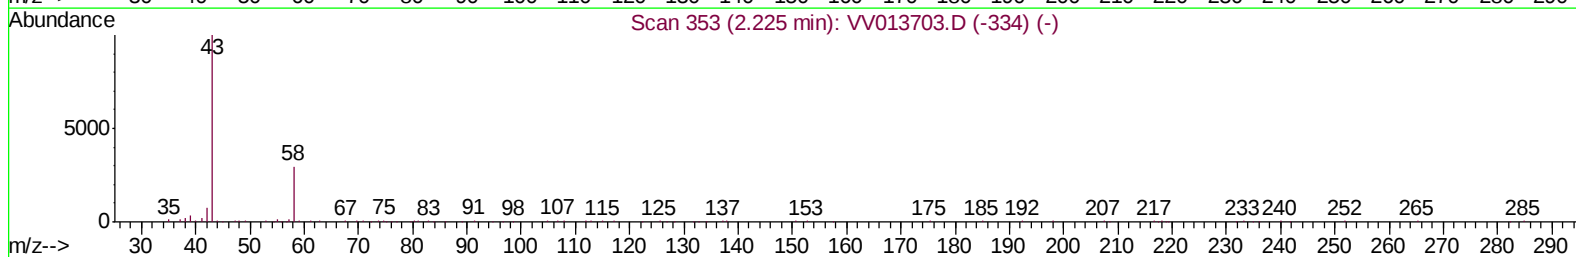
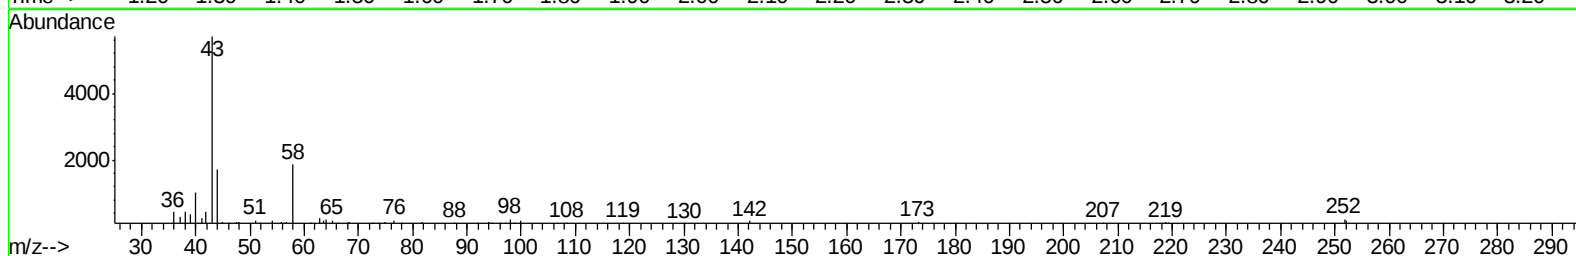


Data File : VV013720.D
Acq On : 21 Nov 2019 18:18
Operator : SY/MD
Sample : K5941-14 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Nov 22 04:00:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 22 03:55:18 2019
Response via : Initial Calibration

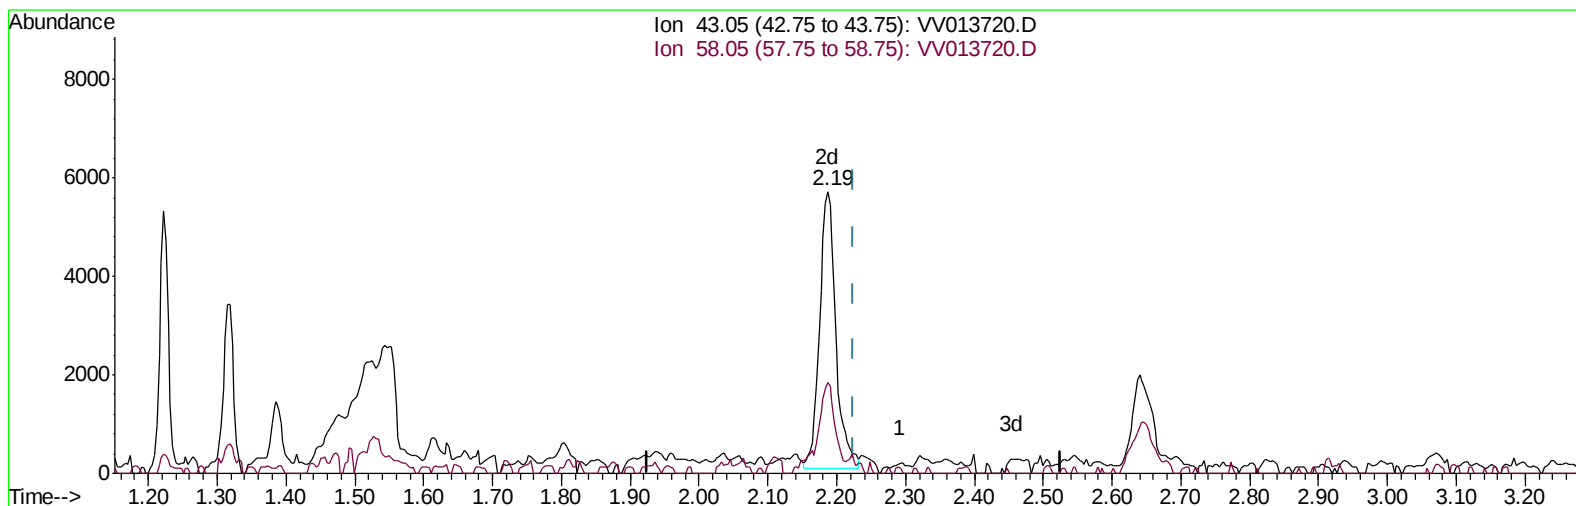

TIC: VV013720.D

(13) Acetone (T)

2.187min (-0.039) 3.15ug/L m

response 9206

Ion	Exp%	Act%
43.05	100	100
58.05	8.50	3.89
0.00	0.00	0.00
0.00	0.00	0.00