




Data File : VV013720.D
Acq On : 21 Nov 2019 18:18
Operator : SY/MD
Sample : K5941-14 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC6

Manual Integrations
APPROVED

MMDadoda
11/22/2019 9:48:55 AM

Quant Time: Nov 22 04:00:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 22 03:55:18 2019
Response via : Initial Calibration

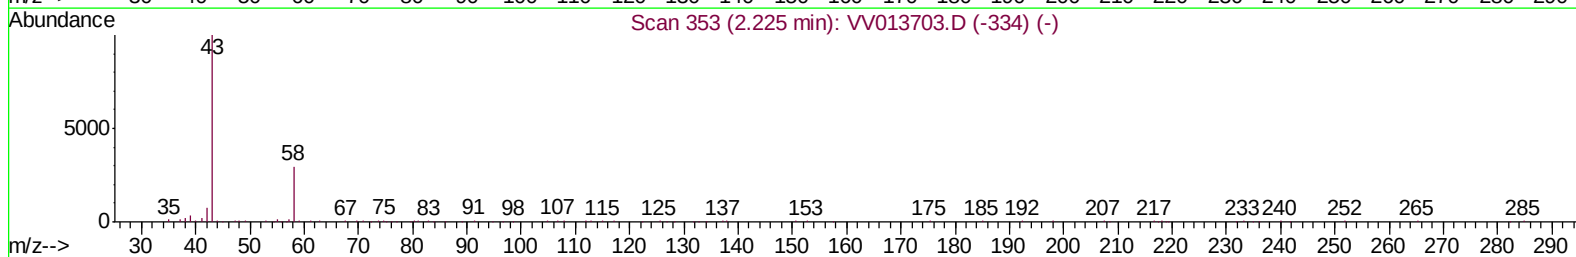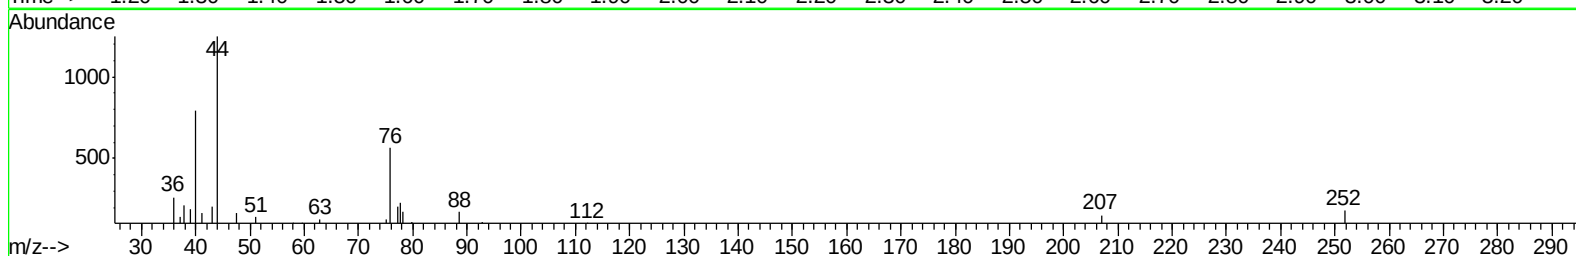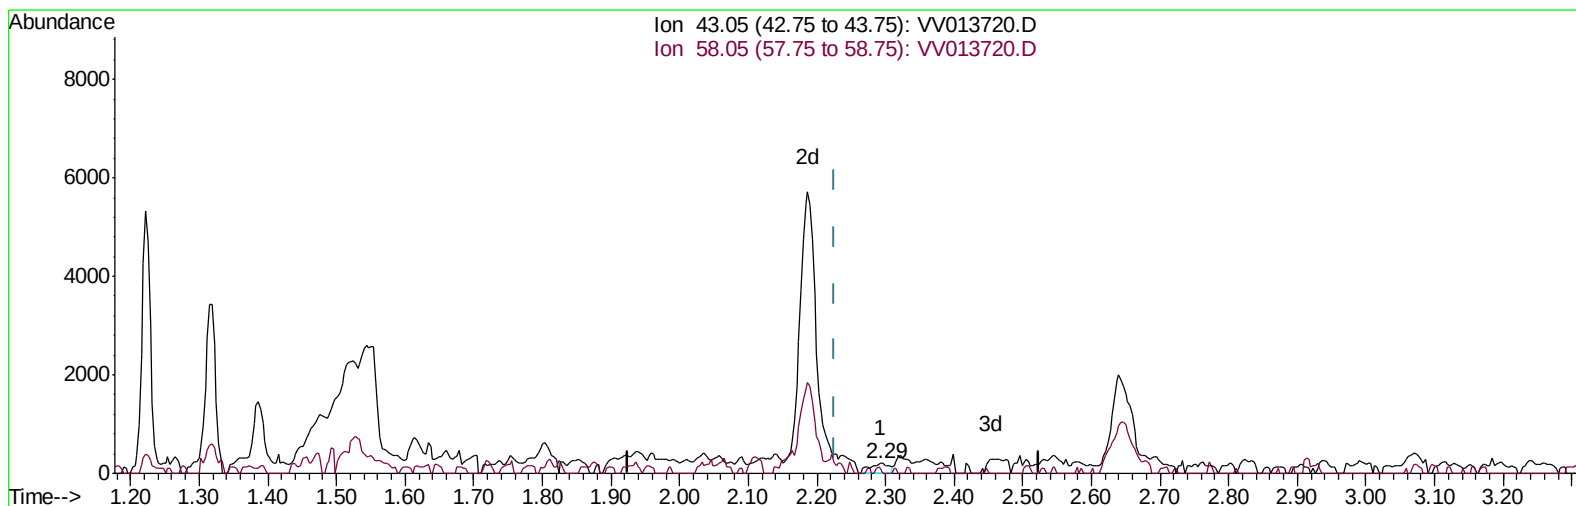

TIC: VV013720.D

(13) Acetone (T)

2.293min (+0.067) 0.14ug/L

response 403

Ion	Exp%	Act%
43.05	100	100
58.05	8.50	88.83#
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VV013720.D
Acq On : 21 Nov 2019 18:18
Operator : SY/MD
Sample : K5941-14 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC6

Manual Integrations
APPROVED

MMDadoda
11/22/2019 9:48:55 AM

Quant Time: Nov 22 04:00:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 22 03:55:18 2019
Response via : Initial Calibration

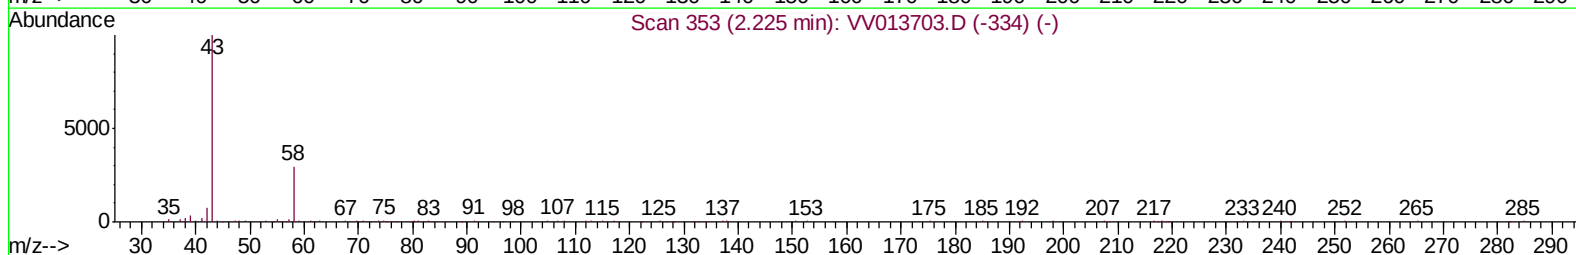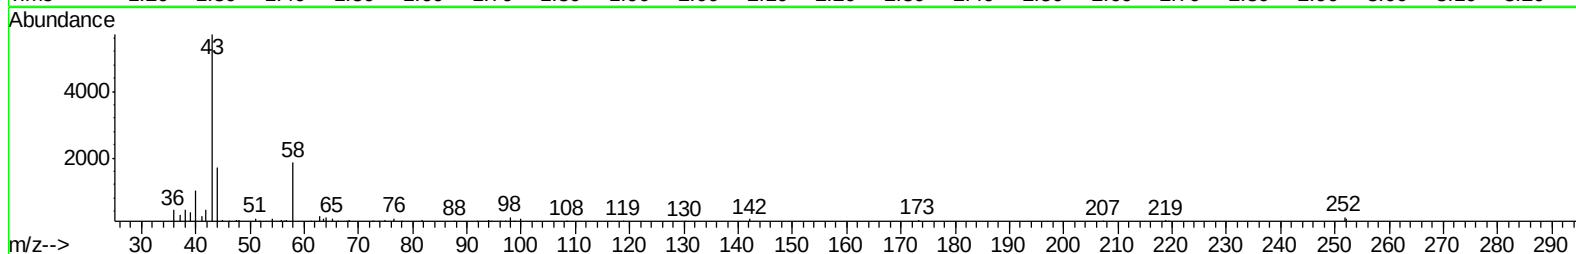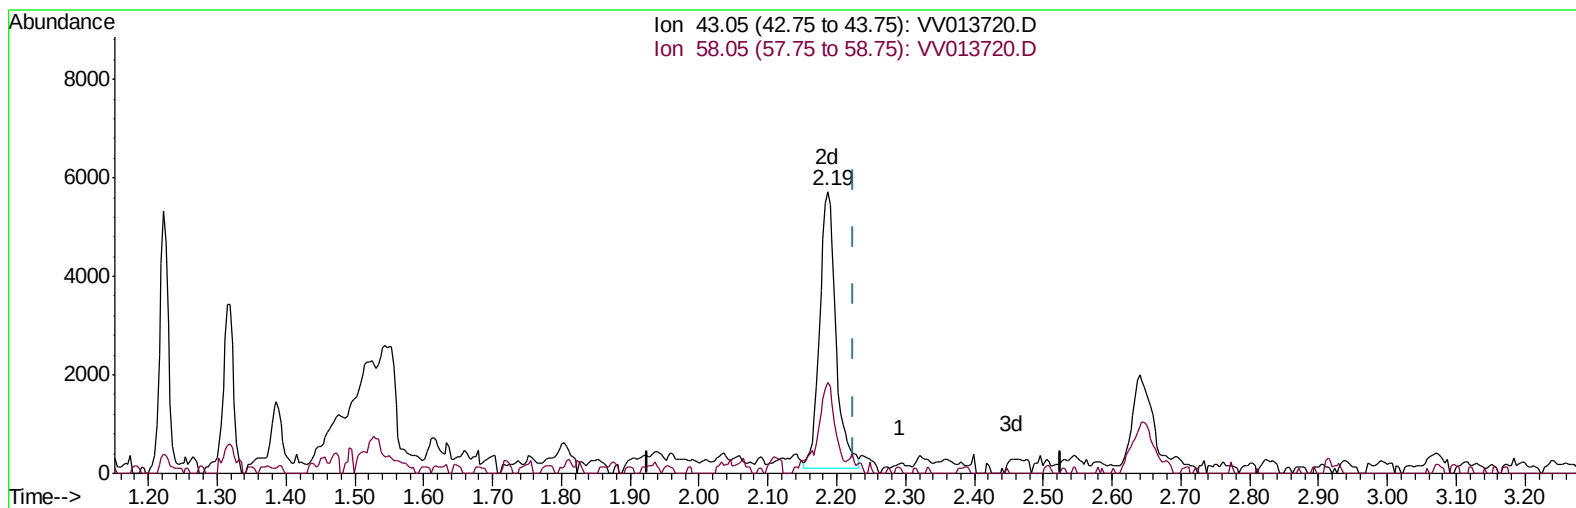

TIC: VV013720.D

(13) Acetone (T)

2.187min (-0.039) 3.15ug/L m

response 9206

Ion	Exp%	Act%
43.05	100	100
58.05	8.50	3.89
0.00	0.00	0.00
0.00	0.00	0.00

Data File : VV013720.D
Acq On : 21 Nov 2019 18:18
Operator : SY/MD
Sample : K5941-14 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC6

Manual Integrations
APPROVED

MMDadoda
11/22/2019 9:48:55 AM

Quant Time: Nov 22 05:48:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 22 03:55:18 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	324534	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	310946	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	162371	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	116392	5.80	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	116.00%
7) Chloroethane-d5	1.55	69	82080	4.59	ug/L	-0.03
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.12	63	161997	4.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.20%
20) 2-Butanone-d5	3.92	46	319288	68.87	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	137.74%#
24) Chloroform-d	4.39	84	237201	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.00%
26) 1,2-Dichloroethane-d4	5.07	65	125970	5.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.40%
32) Benzene-d6	5.09	84	500925	5.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.60%
36) 1,2-Dichloropropane-d6	6.11	67	152026	5.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	118.80%
41) Toluene-d8	7.35	98	437620	5.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.60%
43) trans-1,3-Dichloropropene-	7.66	79	52384	5.32	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	106.40%
46) 2-Hexanone-d5	8.13	63	238069	63.82	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	127.64%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	112278	6.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	121.20%#
64) 1,2-Dichlorobenzene-d4	11.67	152	191595	6.13	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	122.60%#

Target Compounds

					Qvalue
13) Acetone	2.19	43	9206m	3.147	ug/L
25) Chloroform	4.42	83	51570	0.892	ug/L
34) Trichloroethene	5.96	95	3466	0.138	ug/L
38) Bromodichloromethane	6.55	83	14762	0.470	ug/L
49) Dibromochloromethane	8.29	129	7649	0.371	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV013720.D
Acq On : 21 Nov 2019 18:18
Operator : SY/MD
Sample : K5941-14 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC6

Manual Integrations
APPROVED

MMDadoda
11/22/2019 9:48:55 AM

Quant Time: Nov 22 05:48:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 22 03:55:18 2019
Response via : Initial Calibration

