




Data File : VV013721.D
Acq On : 21 Nov 2019 18:42
Operator : SY/MD
Sample : K5941-15 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC9

Manual Integrations
APPROVED

MMDadoda
11/22/2019 9:49:00 AM

Quant Time: Nov 22 04:00:59 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 22 03:55:18 2019
Response via : Initial Calibration

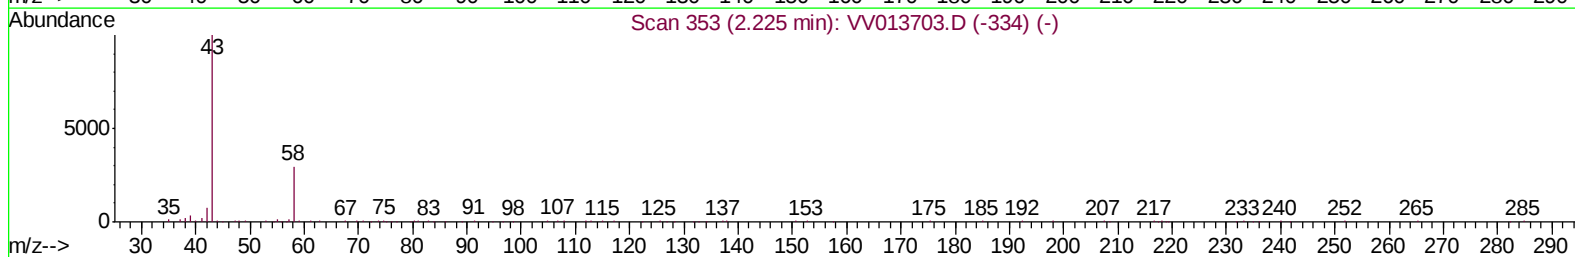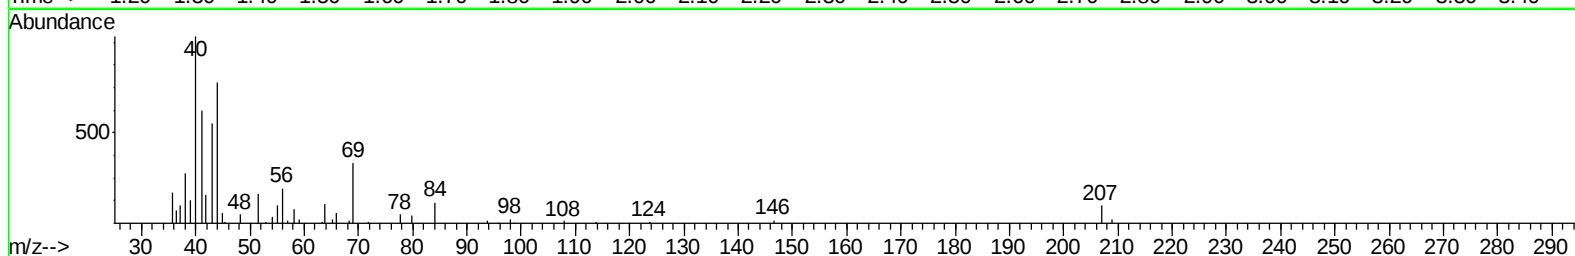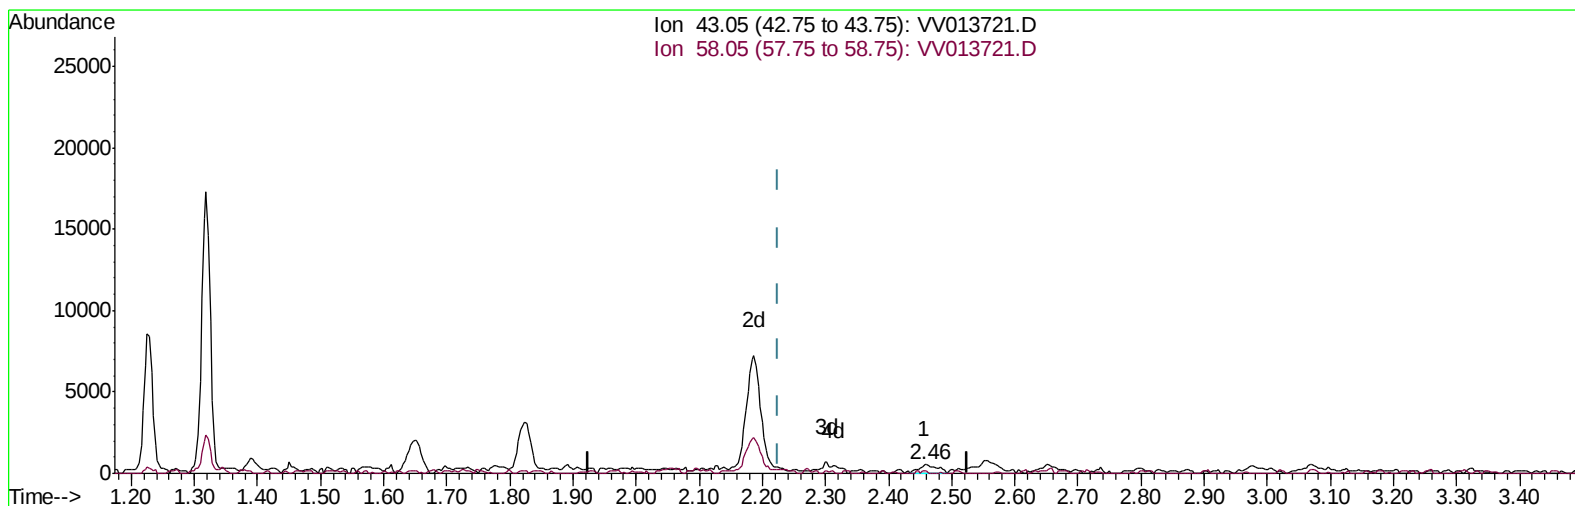

TIC: VV013721.D

(13) Acetone (T)

2.457min (+0.231) 0.36ug/L

response 1103

Ion	Exp%	Act%
43.05	100	100
58.05	8.50	11.06
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VV013721.D
Acq On : 21 Nov 2019 18:42
Operator : SY/MD
Sample : K5941-15 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC9

Manual Integrations
APPROVED

MMDadoda
11/22/2019 9:49:00 AM

Quant Time: Nov 22 04:00:59 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 22 03:55:18 2019
Response via : Initial Calibration

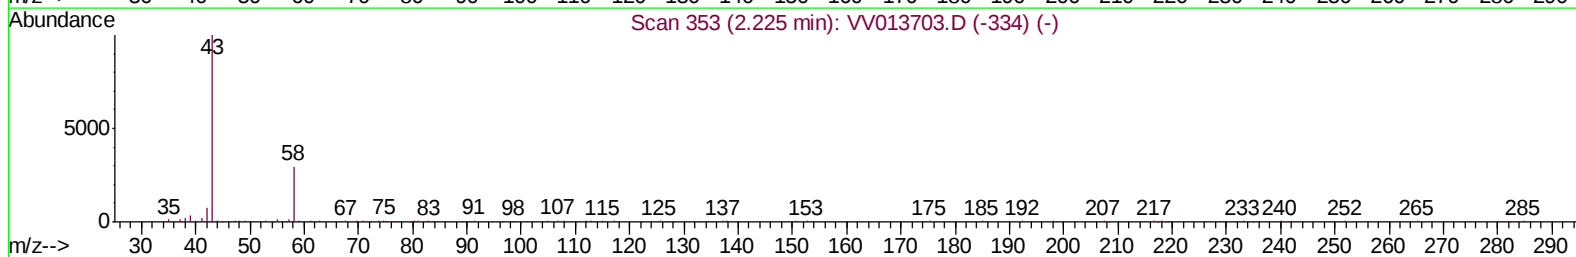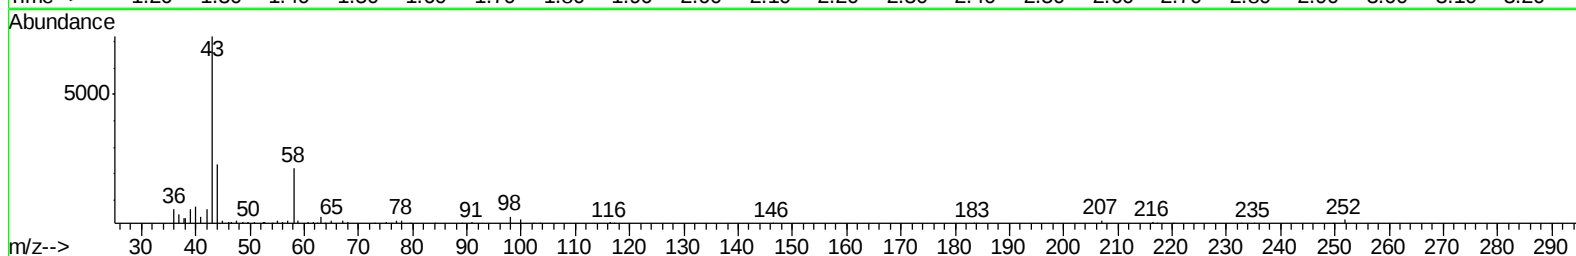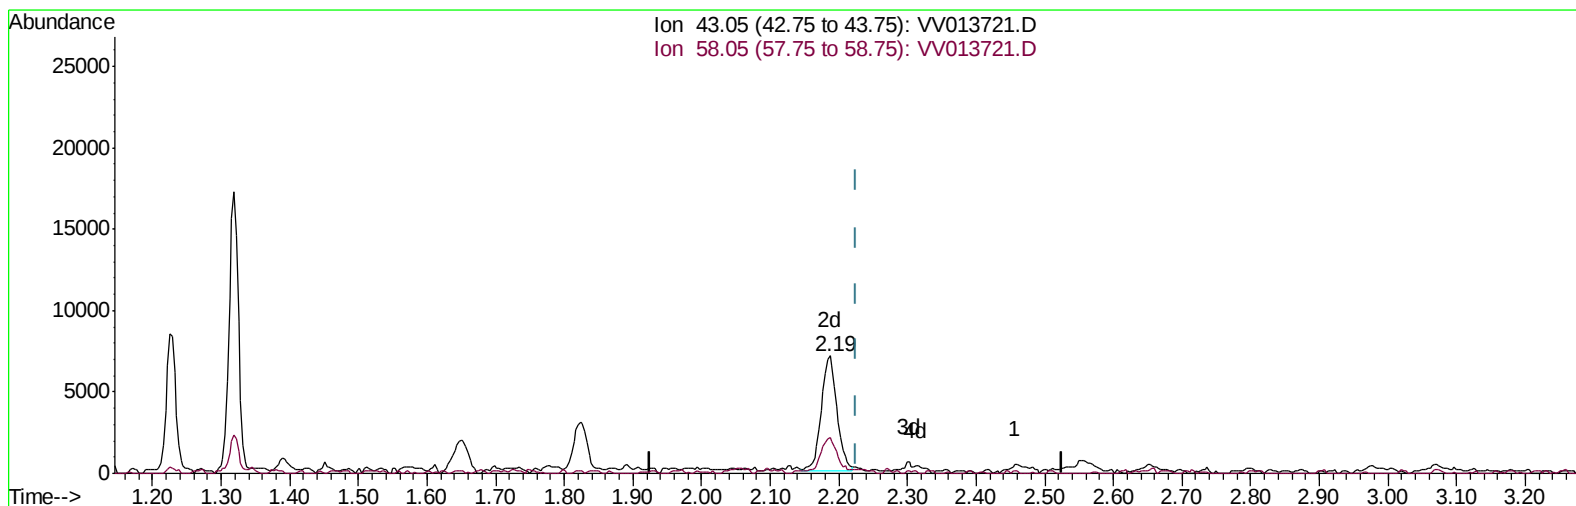

TIC: VV013721.D

(13) Acetone (T)

2.187min (-0.039) 3.69ug/L m

response 11438

Ion	Exp%	Act%
43.05	100	100
58.05	8.50	1.07
0.00	0.00	0.00
0.00	0.00	0.00

Data File : VV013721.D
Acq On : 21 Nov 2019 18:42
Operator : SY/MD
Sample : K5941-15 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC9

Manual Integrations
APPROVED

MMDadoda
11/22/2019 9:49:00 AM

Quant Time: Nov 22 05:53:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 22 03:55:18 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	343514	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	347007	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	156476	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	120449	5.67	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	113.40%
7) Chloroethane-d5	1.58	69	112110	5.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	118.40%
11) 1,1-Dichloroethene-d2	2.13	63	168688	4.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.60%
20) 2-Butanone-d5	3.92	46	308313	62.83	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.66%
24) Chloroform-d	4.40	84	253585	5.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.20%
26) 1,2-Dichloroethane-d4	5.08	65	126336	5.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.00%
32) Benzene-d6	5.10	84	511320	5.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.80%
36) 1,2-Dichloropropane-d6	6.11	67	157940	5.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.60%
41) Toluene-d8	7.36	98	445415	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
43) trans-1,3-Dichloropropene-	7.66	79	54458	4.95	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.00%
46) 2-Hexanone-d5	8.13	63	217167	52.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.34%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	108121	5.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	180347	5.99	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.80%

Target Compounds					Qvalue
13) Acetone	2.19	43	11438m	3.694	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV013721.D
Acq On : 21 Nov 2019 18:42
Operator : SY/MD
Sample : K5941-15 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC9

Manual Integrations
APPROVED

MMDadoda
11/22/2019 9:49:00 AM

Quant Time: Nov 22 05:53:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 22 03:55:18 2019
Response via : Initial Calibration

