

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112119\
 Data File : VV013718.D
 Acq On : 21 Nov 2019 17:06
 Operator : SY/MD
 Sample : K5941-11 10X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AC3

Quant Time: Nov 22 05:32:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 22 03:55:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	298526	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	286592	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	132904	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	117349	6.36	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	127.20%
7) Chloroethane-d5	1.58	69	111921	6.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	136.00%#
11) 1,1-Dichloroethene-d2	2.13	63	169350	5.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	102.40%
20) 2-Butanone-d5	3.95	46	253899	59.54	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.08%
24) Chloroform-d	4.40	84	259991	6.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	127.60%#
26) 1,2-Dichloroethane-d4	5.08	65	126961	6.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	129.60%
32) Benzene-d6	5.09	84	524805	6.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	131.40%#
36) 1,2-Dichloropropane-d6	6.12	67	156436	6.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	132.60%
41) Toluene-d8	7.36	98	452215	6.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	121.80%
43) trans-1,3-Dichloropropene-	7.66	79	53637	5.91	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	118.20%
46) 2-Hexanone-d5	8.14	63	202843	59.00	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	118.00%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	105242	6.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	123.20%#
64) 1,2-Dichlorobenzene-d4	11.67	152	177770	6.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	139.00%#


Target Compounds				Ovalue
13) Acetone	2.21	43	4464	1.659 ug/L # 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV112119\
Data File : VV013718.D
Acq On : 21 Nov 2019 17:06
Operator : SY/MD
Sample : K5941-11 10X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC3

Quant Time: Nov 22 05:32:08 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 22 03:55:18 2019
Response via : Initial Calibration

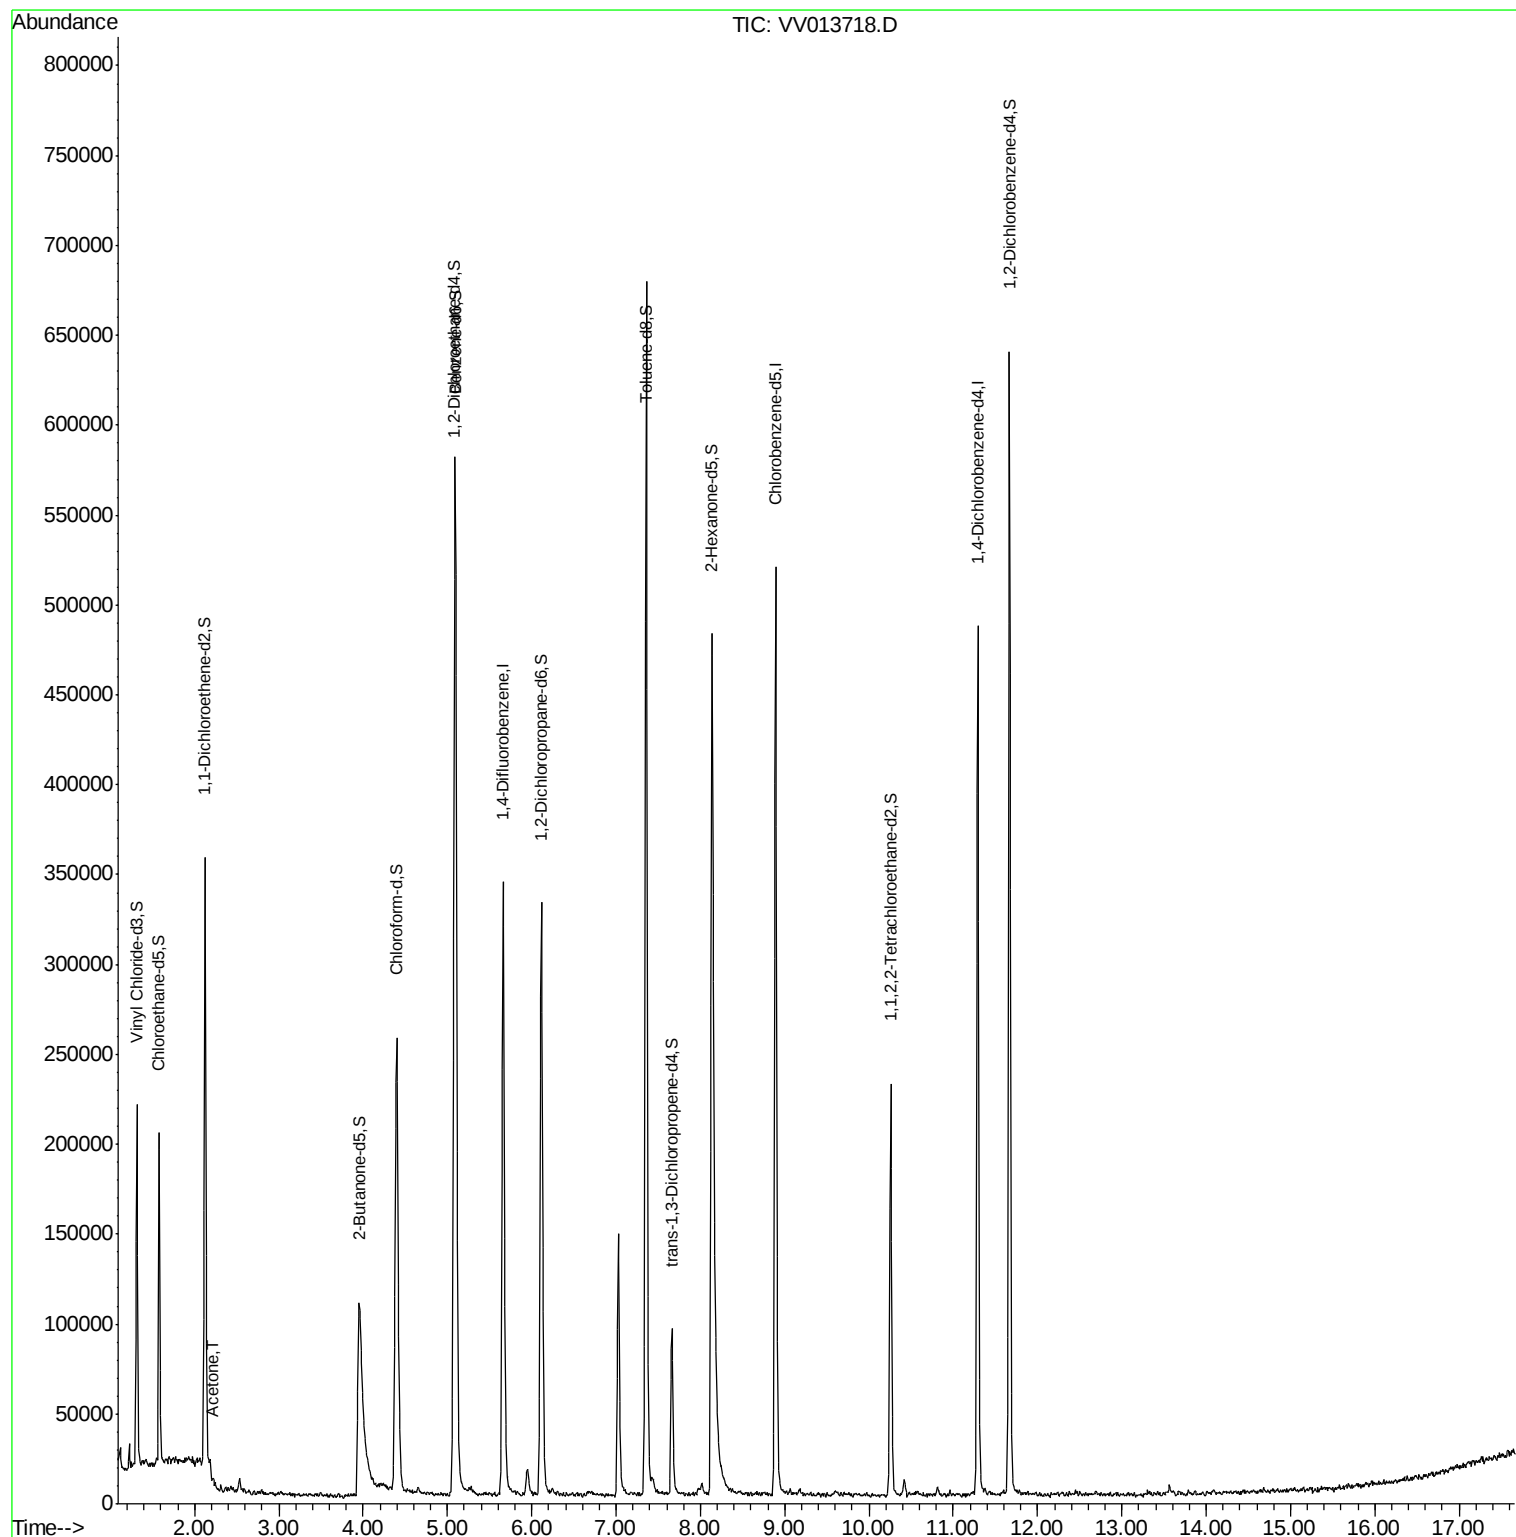

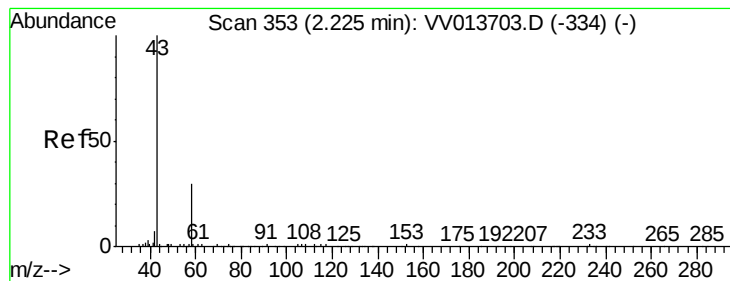

#13

Acetone

Concen: 1.659 ug/L

RT: 2.21 min Scan# 349

Delta R.T. -0.01 min

Lab File: VV013718.D

Acq: 21 Nov 2019 17:06


Instrument :
MSVOA_V
ClientSampleId :
B0AC3

Tot Ion: 43 Resp: 4464

Ion Ratio Lower Upper

43 100

58 19.3 0.0 17.0#

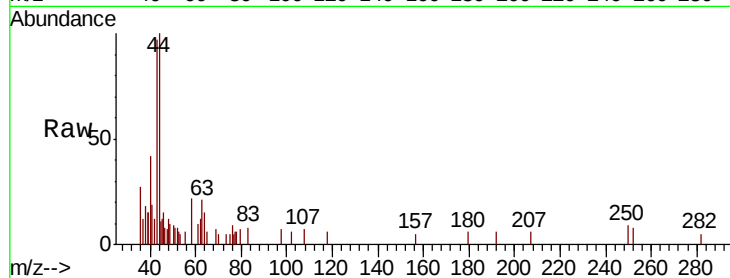

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

