

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112119\
 Data File : VV013722.D
 Acq On : 21 Nov 2019 19:06
 Operator : SY/MD
 Sample : K5941-12 10X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AC4

Quant Time: Nov 22 05:55:15 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 22 03:55:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	317318	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	302867	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	144081	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	115006	5.86	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	117.20%
7) Chloroethane-d5	1.55	69	97534	5.57	ug/L	-0.03
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.40%
11) 1,1-Dichloroethene-d2	2.12	63	156042	4.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.80%
20) 2-Butanone-d5	3.92	46	271223	59.83	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.66%
24) Chloroform-d	4.39	84	236001	5.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.00%
26) 1,2-Dichloroethane-d4	5.07	65	120856	5.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.00%
32) Benzene-d6	5.09	84	495398	5.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	117.40%
36) 1,2-Dichloropropane-d6	6.11	67	147318	5.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	118.20%
41) Toluene-d8	7.35	98	432947	5.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.40%
43) trans-1,3-Dichloropropene-	7.66	79	49057	5.11	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.20%
46) 2-Hexanone-d5	8.13	63	195303	53.75	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.50%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	98414	5.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	178046	6.42	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	128.40%#


Target Compounds				Ovalue
13) Acetone	2.18	43	6350	2.220 ug/L # 34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV112119\
Data File : VV013722.D
Acq On : 21 Nov 2019 19:06
Operator : SY/MD
Sample : K5941-12 10X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AC4

Quant Time: Nov 22 05:55:15 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 22 03:55:18 2019
Response via : Initial Calibration

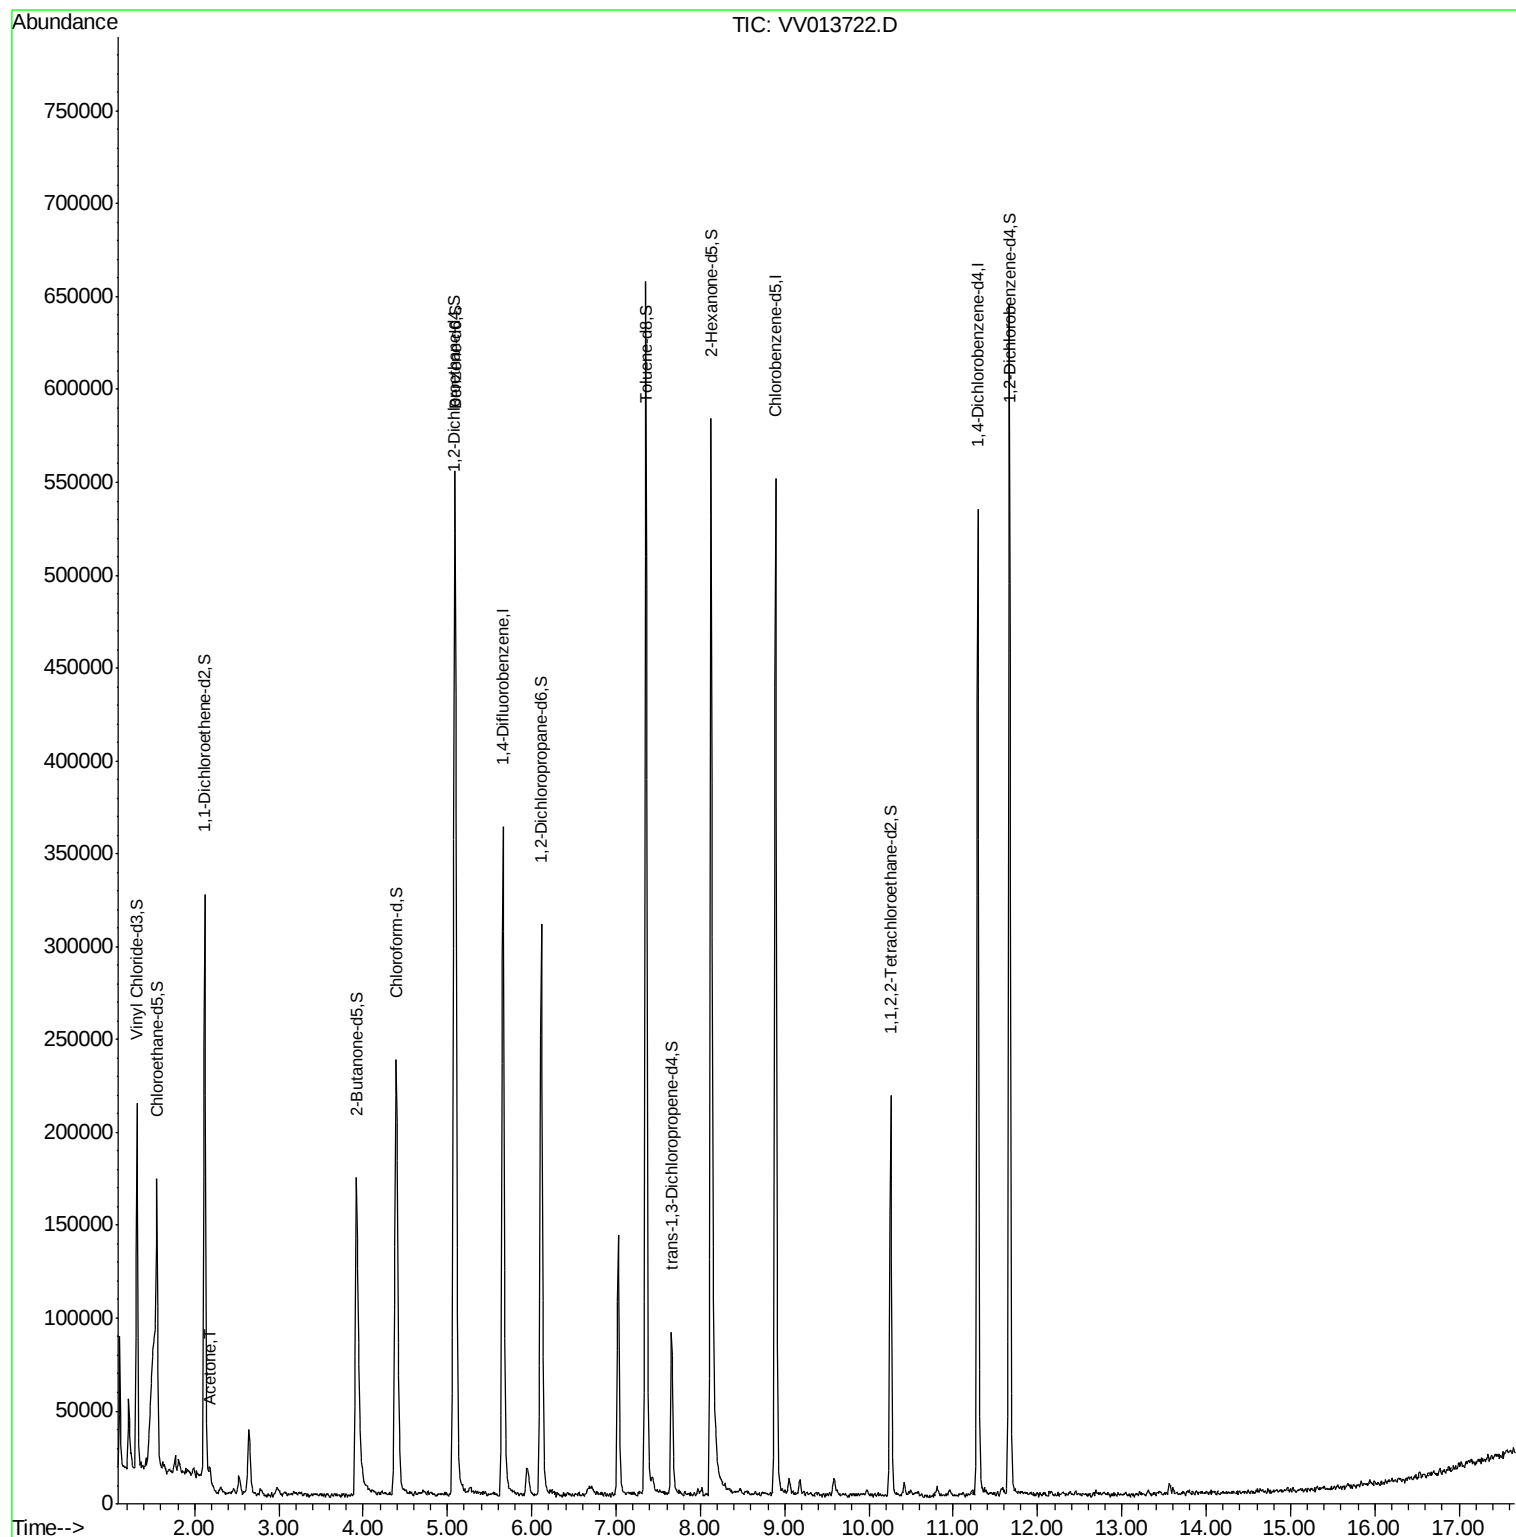

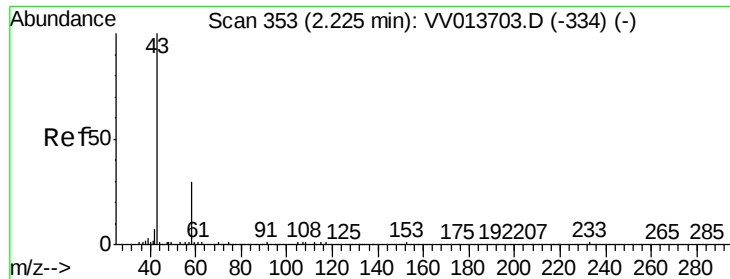

#13

Acetone

Concen: 2.220 ug/L

RT: 2.18 min Scan# 340

Delta R.T. -0.04 min

Lab File: VV013722.D

Acq: 21 Nov 2019 19:06

Instrument :

MSVOA_V

ClientSampleId :

B0AC4

Tot Ion: 43 Resp: 6350

Ion Ratio Lower Upper

43 100

58 31.9 0.0 17.0#

