


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV112119\
 Data File : VV013702.D
 Acq On : 21 Nov 2019 08:29
 Operator : SY/MD
 Sample : BFB36
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB36

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Nov 25 13:56:54 2019

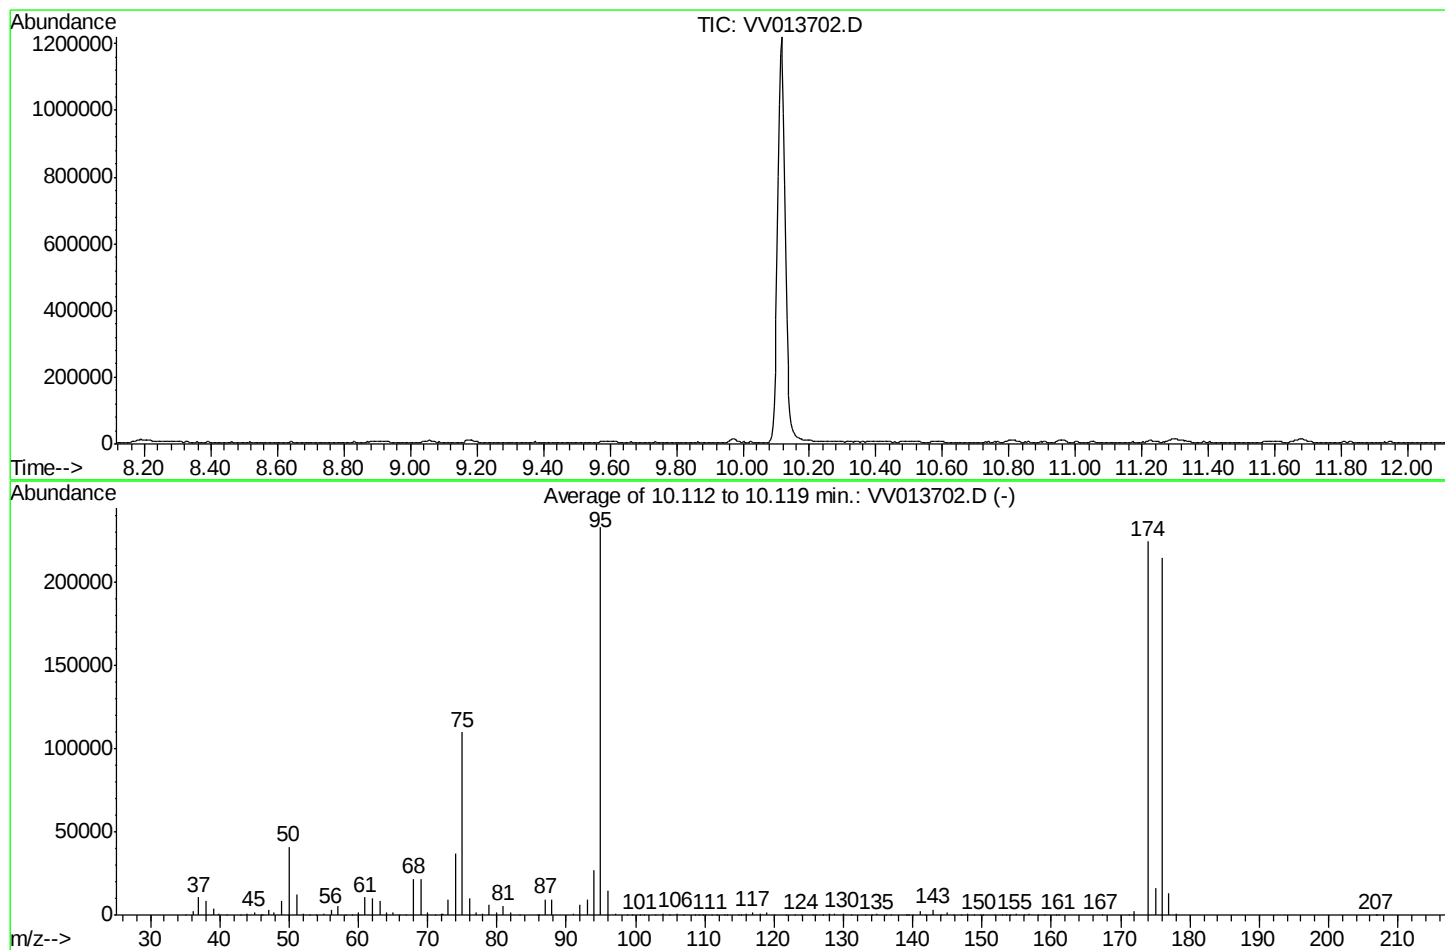

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	41114	PASS
75	95	30	80	47.1	109924	PASS
95	95	100	100	100.0	233258	PASS
96	95	5	9	6.2	14571	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	96.3	224640	PASS
175	174	5	9	7.0	15821	PASS
176	174	95	101	95.7	214976	PASS
177	176	5	9	6.2	13341	PASS

141.00	2041.0
141.90	346.0
143.00	3047.0
144.00	307.0
144.90	1104.0
145.80	437.0
147.00	182.0
147.90	660.0
149.00	230.0
149.70	165.0
150.10	176.0
151.90	200.0
152.90	143.0
153.50	261.0
154.90	610.0
156.80	514.0
158.10	156.0
159.00	365.0
160.60	139.0
161.10	263.0
167.30	119.0
172.00	2581.0
174.00	222848.0
175.00	16095.0
176.00	213056.0
177.00	13281.0
177.90	466.0
207.00	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
35.80	152.0
40.10	509.0
41.40	118.0
41.90	126.0
42.30	133.0
43.10	187.0
44.10	720.0
48.50	132.0
49.00	156.0
51.20	102.0
51.70	137.0
58.20	122.0
60.20	104.0
69.20	114.0
70.50	102.0
75.10	182.0
79.90	113.0
81.10	130.0
84.70	101.0
86.00	121.0
102.40	106.0
105.00	108.0
108.20	111.0
125.30	115.0
216.60	130.0
277.70	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
35.20	127.0
36.10	2283.0
37.00	10580.0
38.10	8615.0
39.10	3964.0
39.90	1021.0
40.90	153.0
41.80	119.0
43.10	234.0
44.00	1593.0
45.00	1735.0
46.20	443.0
47.00	2988.0
47.90	1313.0
49.00	9065.0
50.00	40560.0
51.00	12378.0
52.00	695.0
53.00	242.0
54.00	128.0
55.10	744.0
56.10	3182.0
57.00	5387.0
58.10	336.0
60.00	2088.0
61.00	10659.0
62.00	10385.0
63.10	8964.0
64.10	1469.0
65.00	1747.0
66.00	181.0
66.90	403.0
68.00	21704.0
69.10	21056.0
70.00	1726.0
71.10	153.0
72.00	1106.0
72.20	1117.0
73.00	9091.0
74.10	36744.0
75.00	109912.0
76.10	9744.0
76.90	1542.0
77.90	1088.0
78.90	5891.0
79.90	1663.0
80.90	5986.0
82.00	1255.0
83.30	227.0
86.10	459.0
87.00	9349.0
88.00	8999.0
91.00	1148.0
92.00	6370.0
93.00	9375.0
94.00	25976.0
95.00	234176.0
96.00	15407.0
97.00	651.0
99.50	115.0
103.00	138.0
103.90	731.0
104.80	250.0
105.90	909.0
106.90	296.0
109.70	138.0
110.10	123.0
111.00	180.0
111.80	150.0
112.80	134.0
113.20	129.0
114.90	287.0
115.90	922.0
116.90	1502.0
117.90	814.0
118.90	1314.0
120.00	164.0
121.80	127.0
123.00	149.0
123.90	132.0
125.60	161.0
127.00	134.0
127.90	909.0
128.80	493.0
130.00	985.0
131.10	311.0
133.10	107.0
134.00	150.0
134.80	425.0
136.00	157.0
136.80	280.0
139.10	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

139.40	138.0
140.00	339.0
141.00	2344.0
141.90	376.0
142.90	3093.0
144.00	313.0
145.00	1311.0
145.90	366.0
147.00	169.0
147.80	734.0
148.80	215.0
149.70	249.0
151.90	113.0
152.80	191.0
153.50	239.0
154.00	216.0
154.90	666.0
156.00	149.0
156.90	485.0
159.00	325.0
161.00	301.0
171.10	476.0
172.00	2737.0
174.00	218752.0
175.00	15226.0
176.00	209536.0
177.00	13049.0
178.00	670.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
35.10	137.0
36.10	2217.0
37.00	10891.0
38.10	8821.0
39.10	3860.0
39.90	987.0
40.90	163.0
43.00	222.0
44.00	1669.0
45.00	1982.0
46.20	442.0
47.00	3442.0
47.90	1229.0
49.00	8996.0
50.00	42960.0
51.00	12838.0
52.00	648.0
52.90	195.0
54.00	112.0
55.10	742.0
56.00	3311.0
57.00	5424.0
58.10	376.0
60.00	1929.0
61.00	10864.0
62.00	10747.0
63.10	8530.0
64.00	1347.0
65.00	1757.0
65.80	175.0
68.00	22432.0
69.10	22032.0
70.00	1794.0
71.20	197.0
72.10	1226.0
73.00	9754.0
74.10	38408.0
75.00	113136.0
76.10	10202.0
76.90	1423.0
77.90	1067.0
78.90	6323.0
79.90	1735.0
81.00	6025.0
82.00	1370.0
83.30	232.0
86.00	438.0
87.00	9706.0
88.00	9219.0
91.00	988.0
92.00	6764.0
93.00	9941.0
94.00	27688.0
95.00	240704.0
96.00	14865.0
97.10	624.0
98.70	118.0
100.70	109.0
101.20	108.0
102.80	164.0
103.90	876.0
104.80	344.0
105.90	1062.0
106.90	322.0
109.20	102.0
110.10	145.0
110.90	196.0
111.80	117.0
112.80	153.0
113.20	152.0
114.80	282.0
115.30	262.0
116.00	896.0
116.90	1677.0
118.00	823.0
119.00	1355.0
119.90	184.0
121.70	133.0
123.10	115.0
124.00	145.0
125.60	147.0
127.00	139.0
127.90	880.0
128.80	502.0
130.00	1000.0
131.10	351.0
134.00	139.0
134.80	473.0
136.00	204.0
136.90	336.0
139.30	197.0
140.00	355.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

141.00	2266.0
141.90	386.0
143.00	3308.0
144.00	355.0
145.00	1266.0
145.80	385.0
147.00	140.0
147.90	780.0
148.90	204.0
149.70	251.0
151.80	149.0
152.90	130.0
153.40	319.0
154.90	645.0
156.80	543.0
158.10	139.0
159.00	387.0
161.00	282.0
167.30	128.0
172.00	2817.0
174.00	232320.0
175.00	16143.0
176.00	222336.0
177.00	13695.0
178.00	613.0
206.80	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
35.00	149.0
36.10	1897.0
37.00	10001.0
38.10	8283.0
39.10	3407.0
39.90	949.0
40.90	158.0
43.00	206.0
44.00	1639.0
45.00	1832.0
45.90	368.0
47.00	3406.0
47.90	1106.0
49.00	8101.0
50.00	39824.0
51.10	11460.0
52.00	570.0
52.90	179.0
53.90	119.0
55.10	626.0
56.00	3191.0
57.00	4697.0
58.10	368.0
59.00	108.0
60.00	1793.0
61.00	9949.0
62.00	10088.0
63.00	7314.0
64.00	1195.0
65.00	1633.0
65.80	169.0
68.00	20840.0
69.00	21424.0
70.10	1777.0
71.20	194.0
72.00	1272.0
73.00	9002.0
74.10	35928.0
75.10	107272.0
76.10	9362.0
77.00	1237.0
78.00	1021.0
78.90	6145.0
80.00	1775.0
80.90	5669.0
82.00	1362.0
83.20	184.0
85.80	387.0
87.00	9115.0
87.90	8970.0
91.00	725.0
92.00	6098.0
93.00	9376.0
94.00	26464.0
95.00	224896.0
96.10	13441.0
97.10	559.0
98.70	111.0
100.70	142.0
101.20	111.0
102.80	185.0
103.90	950.0
104.80	366.0
105.90	1100.0
107.00	311.0
108.60	131.0
109.10	128.0
110.10	129.0
110.80	184.0
112.80	174.0
113.20	177.0
114.80	285.0
115.30	253.0
116.00	847.0
117.00	1826.0
118.00	729.0
119.00	1320.0
120.00	142.0
121.70	118.0
124.00	165.0
126.00	108.0
127.00	132.0
127.90	780.0
128.80	489.0
129.90	901.0
130.90	321.0
134.10	123.0
134.90	513.0
136.10	188.0
136.90	372.0
139.20	208.0
139.90	334.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36