

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033041.D
 Acq On : 21 Nov 2023 09:29
 Operator : SY/MD
 Sample : VV1121MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK225

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rVB	131449	134008	12.11%	1.478%
2	1.532	146	153	168	rVB	97573	115807	10.47%	1.277%
3	1.979	290	292	295	rBV3	395	226	0.02%	0.002%
4	2.060	302	317	332	rBV	200433	297337	26.88%	3.279%
5	2.159	344	348	351	rBV2	540	419	0.04%	0.005%
6	2.179	351	354	357	rVV3	607	389	0.04%	0.004%
7	2.275	382	384	386	rBV	315	177	0.02%	0.002%
8	2.333	398	402	404	rBV2	436	293	0.03%	0.003%
9	2.401	422	423	425	rBV	482	163	0.01%	0.002%
10	2.455	428	440	449	rBV6	3250	5478	0.50%	0.060%
11	2.542	463	467	468	rBV	728	522	0.05%	0.006%
12	2.597	483	484	488	rBV	339	179	0.02%	0.002%
13	2.658	499	503	504	rBV	491	239	0.02%	0.003%
14	2.770	536	538	540	rBV2	421	176	0.02%	0.002%
15	2.841	554	560	561	rBV2	388	340	0.03%	0.004%
16	2.944	588	592	595	rBV	451	431	0.04%	0.005%
17	2.989	603	606	608	rBV	410	226	0.02%	0.002%
18	3.034	617	620	622	rBV	192	147	0.01%	0.002%
19	3.082	631	635	637	rBV2	303	217	0.02%	0.002%
20	3.201	670	672	674	rBV	299	174	0.02%	0.002%
21	3.256	687	689	691	rBV	258	146	0.01%	0.002%
22	3.384	727	729	732	rVB2	425	198	0.02%	0.002%
23	3.404	732	735	738	rBV3	348	253	0.02%	0.003%
24	3.494	760	763	768	rVB	370	250	0.02%	0.003%
25	3.519	768	771	773	rBV2	225	175	0.02%	0.002%
26	3.581	787	790	793	rVV	337	207	0.02%	0.002%
27	3.780	843	852	889	rBV2	64574	181843	16.44%	2.006%
28	4.085	943	947	955	rBV5	638	987	0.09%	0.011%
29	4.246	980	997	1026	rBV	180133	462877	41.84%	5.105%
30	4.507	1076	1078	1080	rBV3	368	220	0.02%	0.002%
31	4.535	1085	1087	1089	rBV2	525	284	0.03%	0.003%
32	4.838	1175	1181	1184	rBV2	551	562	0.05%	0.006%
33	4.953	1194	1217	1249	rBV2	413620	1106265	100.00%	12.201%
34	5.301	1323	1325	1327	rBV	459	255	0.02%	0.003%
35	5.529	1382	1396	1420	rBV	399219	815730	73.74%	8.997%
36	5.828	1477	1489	1506	rBV3	14938	34284	3.10%	0.378%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033041.D
 Acq On : 21 Nov 2023 09:29
 Operator : SY/MD
 Sample : VV1121MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK225

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	5.986	1525	1538	1562	rBV	236724	490736	44.36%	5.412%
38	6.256	1619	1622	1625	rBV3	434	281	0.03%	0.003%
39	6.394	1661	1665	1669	rBV2	269	228	0.02%	0.003%
40	6.551	1711	1714	1716	rBV	315	265	0.02%	0.003%
41	6.590	1724	1726	1728	rBV2	487	260	0.02%	0.003%
42	6.754	1775	1777	1780	rVB	414	192	0.02%	0.002%
43	6.796	1788	1790	1793	rVB2	372	171	0.02%	0.002%
44	6.912	1815	1826	1855	rBV	133979	255245	23.07%	2.815%
45	7.111	1886	1888	1891	rBV2	321	174	0.02%	0.002%
46	7.133	1892	1895	1898	rBV3	808	602	0.05%	0.007%
47	7.243	1917	1929	1951	rBV	510499	898041	81.18%	9.904%
48	7.551	2016	2025	2047	rBV	98251	173204	15.66%	1.910%
49	7.847	2114	2117	2118	rBV	370	195	0.02%	0.002%
50	7.905	2133	2135	2138	rBV2	696	402	0.04%	0.004%
51	7.960	2151	2152	2155	rBV2	221	154	0.01%	0.002%
52	8.021	2157	2171	2201	rBV	219984	413990	37.42%	4.566%
53	8.516	2324	2325	2330	rBV2	373	195	0.02%	0.002%
54	8.548	2330	2335	2337	rBV2	292	259	0.02%	0.003%
55	8.619	2355	2357	2363	rVB2	570	407	0.04%	0.004%
56	8.651	2363	2367	2371	rBV2	557	521	0.05%	0.006%
57	8.783	2393	2408	2429	rBV	625430	1023953	92.56%	11.293%
58	9.153	2520	2523	2525	rVV2	458	276	0.02%	0.003%
59	9.178	2528	2531	2534	rVV2	363	180	0.02%	0.002%
60	9.307	2567	2571	2573	rVB2	471	339	0.03%	0.004%
61	9.320	2573	2575	2577	rBV	419	258	0.02%	0.003%
62	9.866	2742	2745	2746	rBV2	780	481	0.04%	0.005%
63	9.966	2773	2776	2778	rBV2	412	241	0.02%	0.003%
64	10.153	2823	2834	2856	rBV	306713	490767	44.36%	5.413%
65	10.262	2863	2868	2870	rBV2	657	521	0.05%	0.006%
66	10.323	2883	2887	2902	rVB4	1374	2171	0.20%	0.024%
67	10.532	2948	2952	2957	rVB2	397	329	0.03%	0.004%
68	10.558	2957	2960	2962	rBV	351	227	0.02%	0.003%
69	10.596	2968	2972	2976	rBV2	506	345	0.03%	0.004%
70	10.664	2991	2993	2995	rBV	323	184	0.02%	0.002%
71	10.725	3008	3012	3015	rBV2	287	242	0.02%	0.003%
72	10.744	3015	3018	3021	rBV2	389	372	0.03%	0.004%
73	10.860	3048	3054	3055	rBV3	1238	986	0.09%	0.011%
74	10.960	3083	3085	3088	rBV2	281	176	0.02%	0.002%
75	11.011	3099	3101	3105	rBV2	345	197	0.02%	0.002%
76	11.127	3129	3137	3143	rBV5	3000	4743	0.43%	0.052%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033041.D
 Acq On : 21 Nov 2023 09:29
 Operator : SY/MD
 Sample : VV1121MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK225

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	11.185	3144	3155	3177	rVV	701534	1089736	98.51%	12.019%
78	11.561	3259	3272	3295	rBV	602857	953043	86.15%	10.511%
79	11.763	3331	3335	3336	rBV	408	298	0.03%	0.003%
80	11.908	3378	3380	3383	rVB3	608	300	0.03%	0.003%
81	12.355	3513	3519	3521	rBV3	474	512	0.05%	0.006%
82	12.371	3521	3524	3531	rVB5	1324	1284	0.12%	0.014%
83	12.439	3543	3545	3548	rBV	445	231	0.02%	0.003%
84	12.468	3551	3554	3559	rVB3	447	417	0.04%	0.005%
85	12.500	3561	3564	3570	rVB2	466	334	0.03%	0.004%
86	12.542	3575	3577	3582	rBV2	316	159	0.01%	0.002%
87	12.590	3585	3592	3602	rVB5	4341	6258	0.57%	0.069%
88	12.667	3613	3616	3617	rVB	381	152	0.01%	0.002%
89	12.686	3618	3622	3624	rBV	343	239	0.02%	0.003%
90	12.860	3673	3676	3679	rBV2	462	396	0.04%	0.004%
91	12.927	3694	3697	3700	rBV	293	206	0.02%	0.002%
92	13.005	3719	3721	3729	rBV2	372	440	0.04%	0.005%
93	13.075	3739	3743	3746	rVB3	581	435	0.04%	0.005%
94	13.204	3770	3783	3794	rBV4	9974	16937	1.53%	0.187%
95	13.275	3803	3805	3809	rVB	381	214	0.02%	0.002%
96	13.442	3846	3857	3868	rBV	30784	50291	4.55%	0.555%
97	13.686	3924	3933	3943	rVB4	13178	20185	1.82%	0.223%
98	13.783	3960	3963	3965	rBV2	615	372	0.03%	0.004%
99	13.815	3970	3973	3976	rBV2	496	381	0.03%	0.004%
100	14.352	4138	4140	4141	rBV	766	324	0.03%	0.004%




Sum of corrected areas: 9067138

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033041.D
Acq On : 21 Nov 2023 09:29
Operator : SY/MD
Sample : VV1121MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK225

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

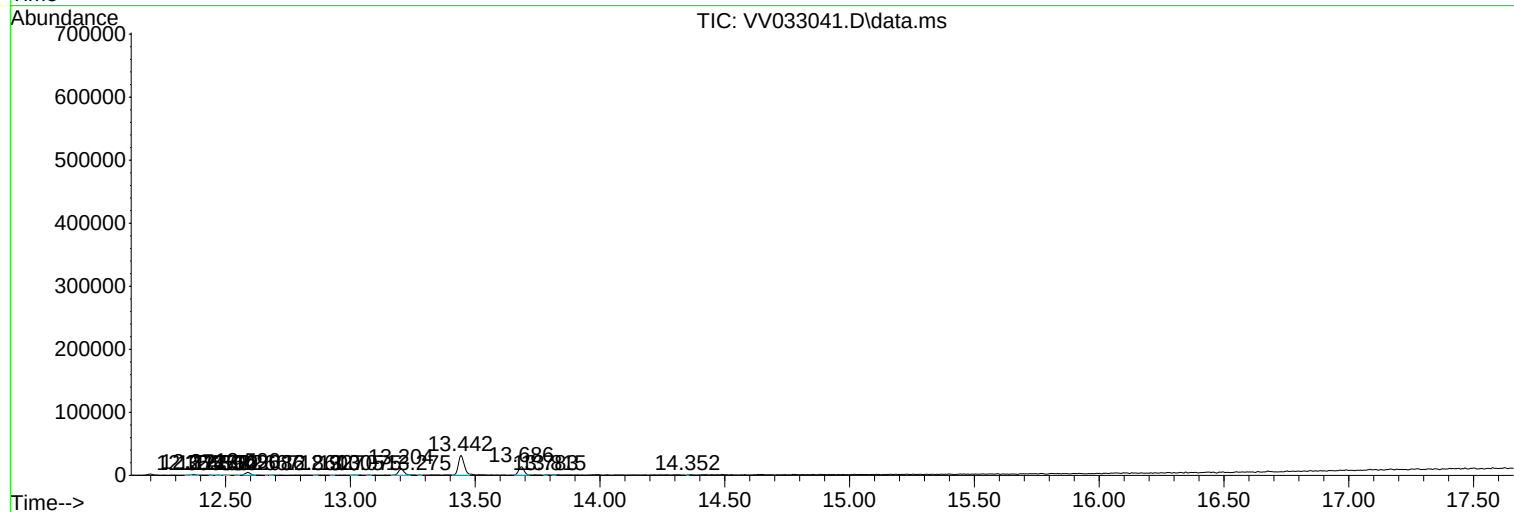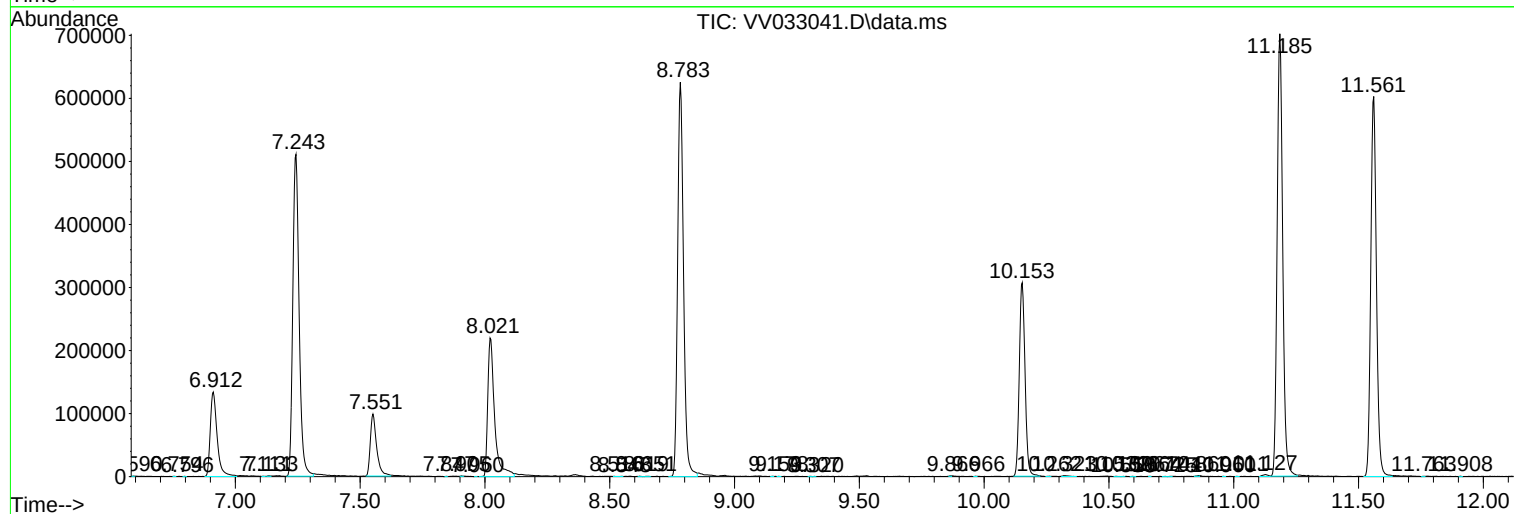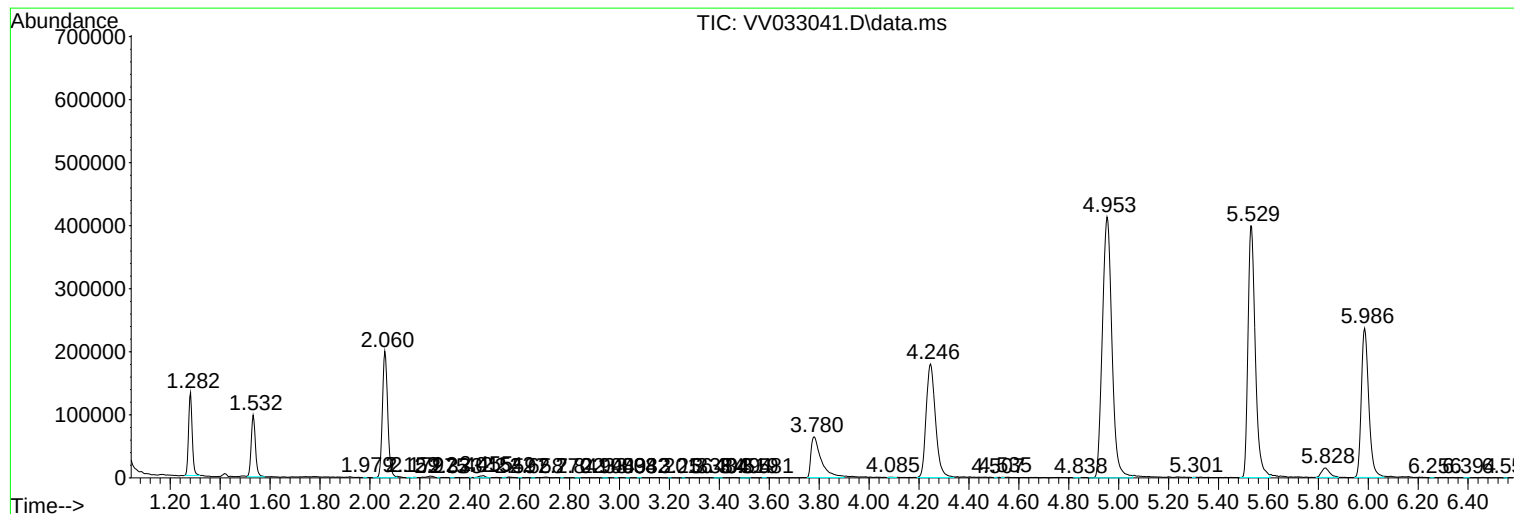

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033041.D
Acq On : 21 Nov 2023 09:29
Operator : SY/MD
Sample : VV1121MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK225

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033041.D
Acq On : 21 Nov 2023 09:29
Operator : SY/MD
Sample : VV1121MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK225

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc