

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033043.D
 Acq On : 21 Nov 2023 10:38
 Operator : SY/MD
 Sample : 05476-22
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033043.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	117430	126837	12.01%	1.520%
2	1.532	145	153	171	rVB	92138	110692	10.48%	1.327%
3	2.060	307	317	331	rBV	191892	280357	26.56%	3.361%
4	2.179	348	354	356	rBV2	732	721	0.07%	0.009%
5	2.384	414	418	422	rBV2	321	267	0.03%	0.003%
6	2.449	431	438	447	rVB5	2681	4389	0.42%	0.053%
7	2.484	447	449	452	rVB2	415	196	0.02%	0.002%
8	2.503	452	455	458	rVB	346	181	0.02%	0.002%
9	2.561	469	473	475	rBV3	381	349	0.03%	0.004%
10	2.632	493	495	496	rBV	319	156	0.01%	0.002%
11	2.674	505	508	510	rVB	333	167	0.02%	0.002%
12	2.696	510	515	516	rBV	411	235	0.02%	0.003%
13	2.851	561	563	567	rBV	395	204	0.02%	0.002%
14	2.876	568	571	575	rVB2	246	219	0.02%	0.003%
15	2.928	584	587	589	rBV2	397	301	0.03%	0.004%
16	2.979	601	603	607	rBV	312	178	0.02%	0.002%
17	3.079	631	634	635	rBV	293	156	0.01%	0.002%
18	3.124	644	648	649	rBV	452	234	0.02%	0.003%
19	3.204	670	673	675	rVB2	344	172	0.02%	0.002%
20	3.252	683	688	690	rBV2	302	222	0.02%	0.003%
21	3.343	713	716	718	rBV2	414	233	0.02%	0.003%
22	3.455	748	751	756	rBV2	186	185	0.02%	0.002%
23	3.539	775	777	782	rVV	467	326	0.03%	0.004%
24	3.603	795	797	800	rVB2	383	179	0.02%	0.002%
25	3.648	808	811	816	rVB2	362	323	0.03%	0.004%
26	3.728	833	836	841	rBV2	292	211	0.02%	0.003%
27	3.780	843	852	884	rBV	58118	156501	14.82%	1.876%
28	4.246	982	997	1028	rBV	175722	442841	41.95%	5.309%
29	4.613	1109	1111	1115	rBV3	467	280	0.03%	0.003%
30	4.725	1144	1146	1149	rVB	619	261	0.02%	0.003%
31	4.741	1149	1151	1154	rBV	440	272	0.03%	0.003%
32	4.760	1154	1157	1163	rBV2	351	314	0.03%	0.004%
33	4.815	1171	1174	1177	rBV2	520	358	0.03%	0.004%
34	4.953	1196	1217	1247	rBV2	392990	1055732	100.00%	12.656%
35	5.317	1328	1330	1333	rBV3	571	276	0.03%	0.003%
36	5.465	1373	1376	1379	rBV3	465	331	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033043.D
 Acq On : 21 Nov 2023 10:38
 Operator : SY/MD
 Sample : 05476-22
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	5.532	1385	1397	1429	rBV	350875	729488	69.10%	8.745%
38	5.825	1478	1488	1505	rBV3	15033	32946	3.12%	0.395%
39	5.985	1525	1538	1569	rBV2	223050	465901	44.13%	5.585%
40	6.188	1597	1601	1603	rBV5	802	655	0.06%	0.008%
41	6.381	1656	1661	1665	rBV3	555	488	0.05%	0.006%
42	6.625	1735	1737	1739	rBV	348	180	0.02%	0.002%
43	6.683	1752	1755	1761	rBV2	435	342	0.03%	0.004%
44	6.850	1803	1807	1809	rBV2	301	193	0.02%	0.002%
45	6.866	1809	1812	1813	rBV	362	189	0.02%	0.002%
46	6.912	1815	1826	1855	rBV	129398	243968	23.11%	2.925%
47	7.239	1917	1928	1949	rBV	483185	860114	81.47%	10.311%
48	7.551	2016	2025	2050	rBV	91585	164513	15.58%	1.972%
49	7.783	2094	2097	2100	rBV	390	282	0.03%	0.003%
50	7.873	2117	2125	2137	rVB3	2798	4388	0.42%	0.053%
51	8.021	2162	2171	2188	rBV	207176	368000	34.86%	4.411%
52	8.365	2276	2278	2280	rVB	609	248	0.02%	0.003%
53	8.452	2303	2305	2312	rVB5	586	476	0.05%	0.006%
54	8.503	2318	2321	2322	rBV	314	150	0.01%	0.002%
55	8.532	2327	2330	2333	rBV2	462	322	0.03%	0.004%
56	8.783	2395	2408	2437	rBV	571764	926239	87.73%	11.104%
57	9.079	2498	2500	2505	rBV3	487	386	0.04%	0.005%
58	9.136	2515	2518	2520	rBV	276	158	0.01%	0.002%
59	9.146	2520	2521	2525	rVV2	358	205	0.02%	0.002%
60	9.497	2627	2630	2632	rBV2	544	310	0.03%	0.004%
61	9.696	2689	2692	2696	rBV2	258	197	0.02%	0.002%
62	9.725	2699	2701	2706	rVB	373	263	0.02%	0.003%
63	9.757	2707	2711	2713	rBV2	316	327	0.03%	0.004%
64	9.808	2725	2727	2730	rVB	566	221	0.02%	0.003%
65	9.831	2730	2734	2736	rBV	264	167	0.02%	0.002%
66	9.850	2736	2740	2741	rBV2	191	144	0.01%	0.002%
67	9.995	2782	2785	2787	rBV	309	179	0.02%	0.002%
68	10.095	2812	2816	2818	rBV	299	165	0.02%	0.002%
69	10.153	2822	2834	2857	rVV	289700	460760	43.64%	5.523%
70	10.278	2871	2873	2875	rVB	479	167	0.02%	0.002%
71	10.326	2881	2888	2895	rBV4	2950	3949	0.37%	0.047%
72	10.435	2919	2922	2925	rBV	319	237	0.02%	0.003%
73	10.622	2977	2980	2981	rBV2	338	165	0.02%	0.002%
74	10.744	3012	3018	3020	rVB	464	460	0.04%	0.006%
75	10.760	3020	3023	3027	rBV2	336	266	0.03%	0.003%
76	10.802	3034	3036	3039	rBV	298	208	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033043.D
 Acq On : 21 Nov 2023 10:38
 Operator : SY/MD
 Sample : 05476-22
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	10.860	3051	3054	3055	rBV	506	268	0.03%	0.003%
78	10.902	3065	3067	3070	rBV	276	175	0.02%	0.002%
79	11.053	3110	3114	3118	rBV2	347	389	0.04%	0.005%
80	11.185	3144	3155	3176	rBV	630234	967520	91.64%	11.598%
81	11.419	3226	3228	3229	rBV	377	160	0.02%	0.002%
82	11.480	3243	3247	3248	rBV	416	247	0.02%	0.003%
83	11.561	3260	3272	3296	rBV	572816	907909	86.00%	10.884%
84	11.779	3339	3340	3344	rBV2	365	225	0.02%	0.003%
85	11.808	3346	3349	3352	rVB2	369	244	0.02%	0.003%
86	11.837	3352	3358	3361	rBV2	452	333	0.03%	0.004%
87	11.860	3361	3365	3366	rBV	306	185	0.02%	0.002%
88	12.011	3410	3412	3414	rVB2	394	164	0.02%	0.002%
89	12.172	3460	3462	3464	rBV2	341	159	0.02%	0.002%
90	12.310	3503	3505	3506	rBV2	499	230	0.02%	0.003%
91	12.587	3586	3591	3592	rBV2	697	569	0.05%	0.007%
92	12.625	3601	3603	3609	rVB	450	381	0.04%	0.005%
93	12.718	3630	3632	3634	rBV	250	146	0.01%	0.002%
94	12.914	3690	3693	3695	rBV	434	228	0.02%	0.003%
95	13.111	3752	3754	3755	rBV	392	162	0.02%	0.002%
96	13.214	3778	3786	3789	rBV4	1892	2568	0.24%	0.031%
97	13.451	3854	3860	3868	rVB5	3308	5427	0.51%	0.065%
98	13.612	3908	3910	3912	rVB	445	142	0.01%	0.002%
99	13.921	4000	4006	4010	rBV3	673	734	0.07%	0.009%
100	14.085	4054	4057	4063	rBV3	425	405	0.04%	0.005%


Sum of corrected areas: 8341842

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033043.D
Acq On : 21 Nov 2023 10:38
Operator : SY/MD
Sample : 05476-22
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

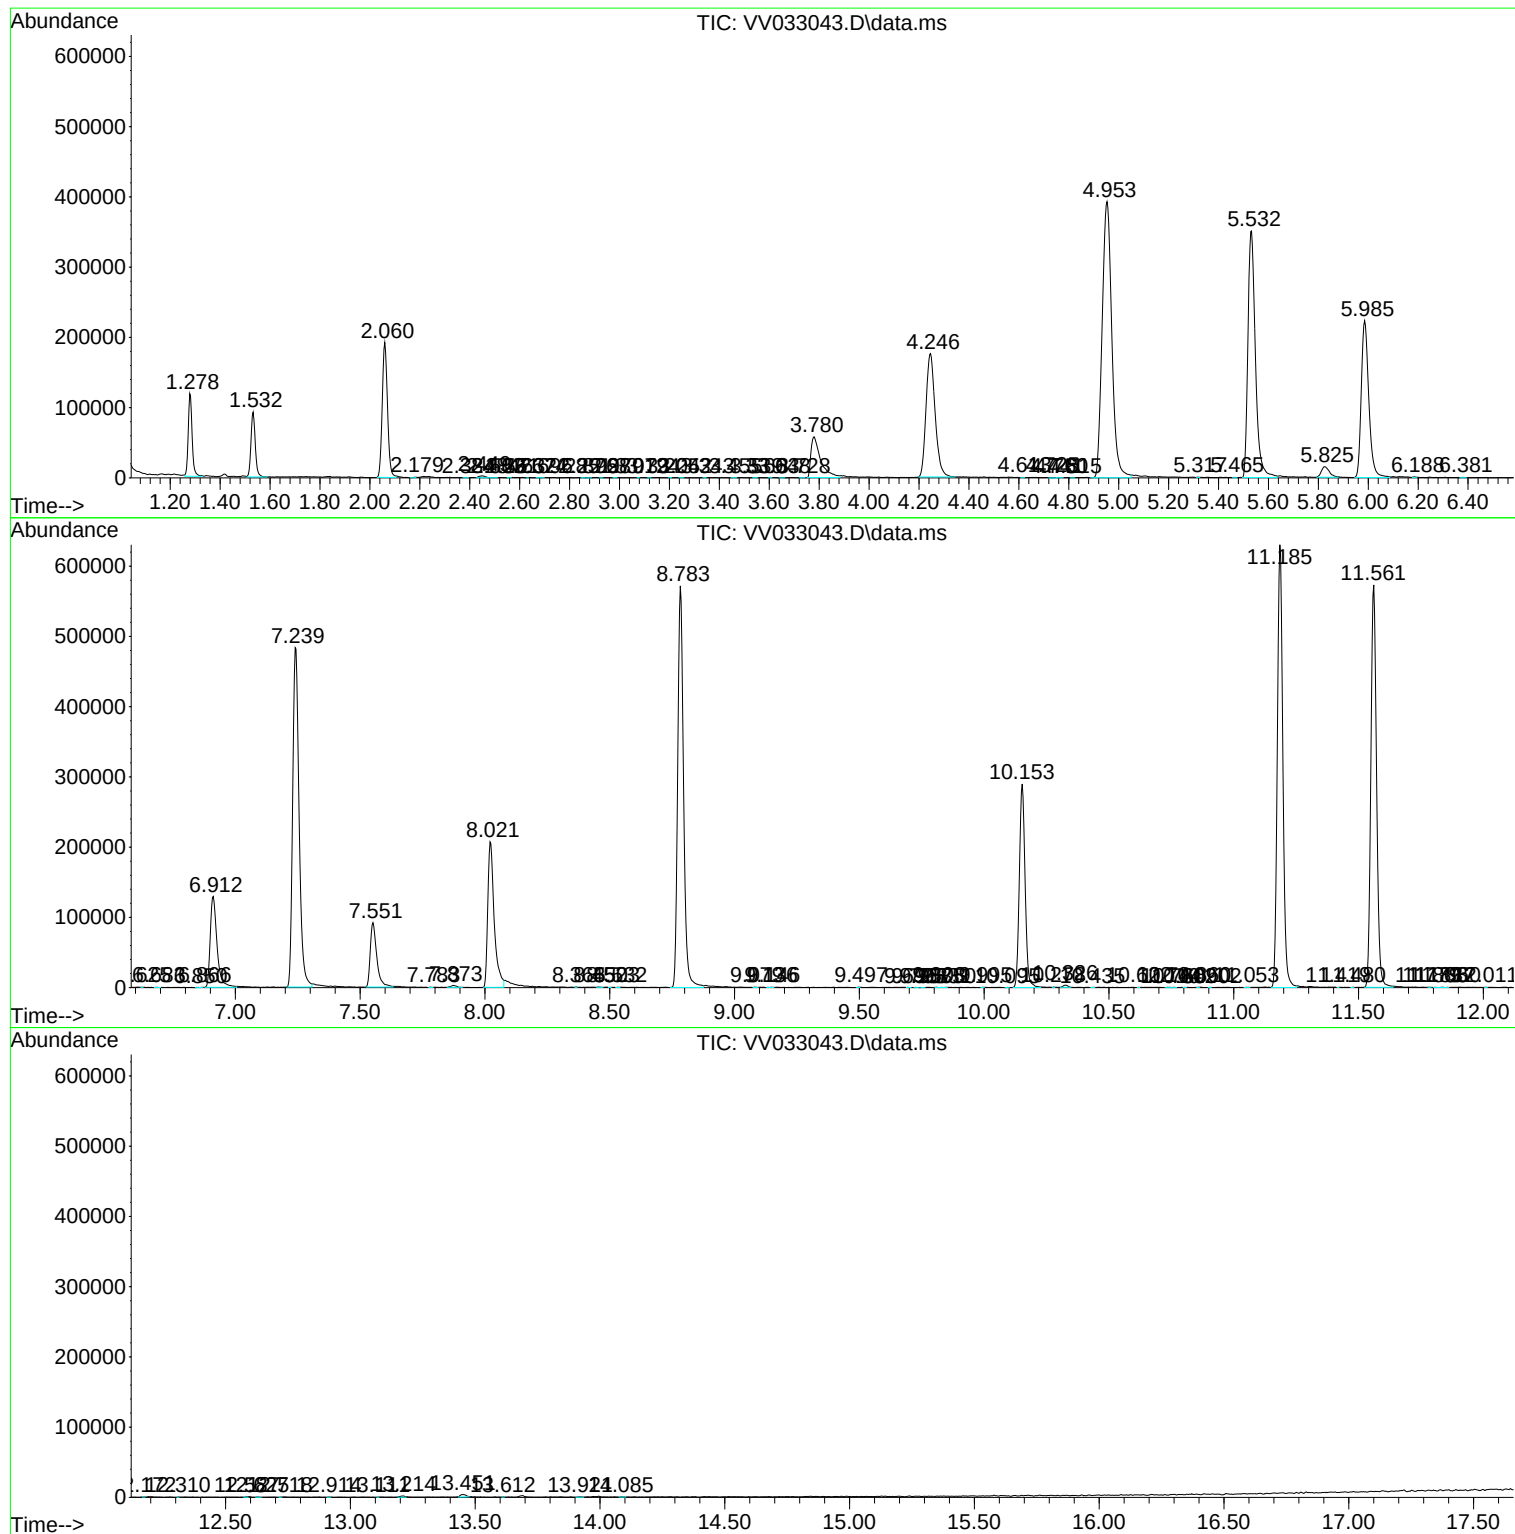

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033043.D
Acq On : 21 Nov 2023 10:38
Operator : SY/MD
Sample : 05476-22
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033043.D
Acq On : 21 Nov 2023 10:38
Operator : SY/MD
Sample : 05476-22
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc