

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033045.D
 Acq On : 21 Nov 2023 11:55
 Operator : SY/MD
 Sample : 05436-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	116145	121735	11.86%	1.501%
2	1.532	145	153	172	rVB	91720	110010	10.71%	1.357%
3	1.960	284	286	291	rVV	570	303	0.03%	0.004%
4	1.982	291	293	295	rVB2	454	237	0.02%	0.003%
5	2.060	307	317	333	rVB	188150	270466	26.34%	3.336%
6	2.220	360	367	370	rBV2	648	823	0.08%	0.010%
7	2.298	389	391	393	rVB2	557	262	0.03%	0.003%
8	2.400	420	423	426	rBV2	315	253	0.02%	0.003%
9	2.449	431	438	443	rBV3	2911	3861	0.38%	0.048%
10	2.494	449	452	454	rBV	351	195	0.02%	0.002%
11	2.664	500	505	506	rBV	349	257	0.03%	0.003%
12	2.773	535	539	541	rVB2	364	255	0.02%	0.003%
13	2.931	585	588	589	rBV2	333	218	0.02%	0.003%
14	3.076	629	633	636	rBV3	415	355	0.03%	0.004%
15	3.140	650	653	655	rBV	280	233	0.02%	0.003%
16	3.256	686	689	693	rVV	259	174	0.02%	0.002%
17	3.429	739	743	744	rBV2	322	192	0.02%	0.002%
18	3.513	767	769	777	rVB2	598	697	0.07%	0.009%
19	3.555	777	782	786	rBV2	363	488	0.05%	0.006%
20	3.699	824	827	832	rVB	254	199	0.02%	0.002%
21	3.725	832	835	838	rBV	294	184	0.02%	0.002%
22	3.777	843	851	880	rBV	54674	146080	14.23%	1.802%
23	4.243	980	996	1022	rBV	166660	440337	42.88%	5.431%
24	4.513	1074	1080	1083	rBV3	622	697	0.07%	0.009%
25	4.571	1096	1098	1102	rBV3	590	400	0.04%	0.005%
26	4.667	1126	1128	1133	rVV3	514	449	0.04%	0.006%
27	4.780	1159	1163	1164	rBV	329	251	0.02%	0.003%
28	4.953	1200	1217	1244	rBV2	385090	1026825	100.00%	12.664%
29	5.452	1370	1372	1373	rBV	842	272	0.03%	0.003%
30	5.532	1385	1397	1431	rBV	342427	708634	69.01%	8.739%
31	5.825	1478	1488	1506	rBV3	16611	35250	3.43%	0.435%
32	5.986	1525	1538	1564	rBV2	218234	454505	44.26%	5.605%
33	6.304	1633	1637	1639	rBV4	455	279	0.03%	0.003%
34	6.600	1727	1729	1733	rVB4	647	375	0.04%	0.005%
35	6.690	1752	1757	1758	rBV4	358	294	0.03%	0.004%
36	6.735	1769	1771	1772	rBV	357	169	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112123\
 Data File : VW033045.D
 Acq On : 21 Nov 2023 11:55
 Operator : SY/MD
 Sample : 05436-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	6.741	1772	1773	1776	rVV	473	231	0.02%	0.003%
38	6.866	1809	1812	1815	rVB2	284	186	0.02%	0.002%
39	6.912	1815	1826	1846	rBV	124577	235677	22.95%	2.907%
40	7.075	1872	1877	1882	rBV5	591	609	0.06%	0.008%
41	7.172	1905	1907	1910	rBV2	450	169	0.02%	0.002%
42	7.243	1916	1929	1952	rBV	472891	845087	82.30%	10.422%
43	7.551	2015	2025	2046	rBV	91930	164653	16.04%	2.031%
44	7.821	2105	2109	2113	rBV	435	280	0.03%	0.003%
45	7.947	2146	2148	2151	rVB2	410	206	0.02%	0.003%
46	8.021	2162	2171	2202	rBV	198087	373702	36.39%	4.609%
47	8.294	2254	2256	2261	rVB4	505	280	0.03%	0.003%
48	8.497	2317	2319	2321	rBV2	405	190	0.02%	0.002%
49	8.587	2341	2347	2348	rBV2	419	388	0.04%	0.005%
50	8.609	2352	2354	2357	rVB	377	191	0.02%	0.002%
51	8.706	2381	2384	2388	rBV	492	307	0.03%	0.004%
52	8.783	2397	2408	2433	rBV	547677	889945	86.67%	10.976%
53	9.021	2478	2482	2484	rBV2	658	503	0.05%	0.006%
54	9.056	2490	2493	2494	rBV2	341	200	0.02%	0.002%
55	9.098	2503	2506	2508	rBV2	300	208	0.02%	0.003%
56	9.207	2535	2540	2543	rBV3	347	339	0.03%	0.004%
57	9.278	2560	2562	2564	rBV	300	177	0.02%	0.002%
58	9.535	2640	2642	2644	rVV	417	226	0.02%	0.003%
59	9.558	2648	2649	2652	rVB2	424	178	0.02%	0.002%
60	9.651	2675	2678	2683	rBV2	362	242	0.02%	0.003%
61	9.767	2711	2714	2717	rBV	220	174	0.02%	0.002%
62	9.802	2720	2725	2728	rBV2	421	421	0.04%	0.005%
63	9.918	2757	2761	2763	rBV	208	183	0.02%	0.002%
64	10.153	2823	2834	2854	rBV	281699	441201	42.97%	5.441%
65	10.320	2878	2886	2895	rBV4	2107	3299	0.32%	0.041%
66	10.542	2950	2955	2964	rVB2	557	703	0.07%	0.009%
67	10.616	2975	2978	2981	rVB	404	267	0.03%	0.003%
68	10.751	3018	3020	3022	rBV2	335	175	0.02%	0.002%
69	10.783	3027	3030	3032	rBV2	495	257	0.03%	0.003%
70	10.796	3032	3034	3039	rVB3	644	406	0.04%	0.005%
71	10.857	3050	3053	3054	rBV	280	179	0.02%	0.002%
72	10.944	3078	3080	3083	rBV2	308	184	0.02%	0.002%
73	11.124	3132	3136	3138	rBV	466	375	0.04%	0.005%
74	11.185	3144	3155	3175	rBV	596239	927898	90.37%	11.444%
75	11.474	3241	3245	3247	rBV2	487	310	0.03%	0.004%
76	11.561	3260	3272	3296	rBV	564868	878990	85.60%	10.840%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033045.D
 Acq On : 21 Nov 2023 11:55
 Operator : SY/MD
 Sample : 05436-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	11.744	3327	3329	3330	rBV	452	201	0.02%	0.002%
78	11.760	3333	3334	3338	rVB3	645	284	0.03%	0.004%
79	11.863	3364	3366	3370	rBV2	338	253	0.02%	0.003%
80	12.136	3448	3451	3453	rBV	320	180	0.02%	0.002%
81	12.194	3459	3469	3481	rBV3	1469	2485	0.24%	0.031%
82	12.252	3483	3487	3490	rBV	502	327	0.03%	0.004%
83	12.320	3505	3508	3513	rVB2	369	218	0.02%	0.003%
84	12.349	3513	3517	3521	rBV2	527	443	0.04%	0.005%
85	12.509	3563	3567	3572	rBV2	329	300	0.03%	0.004%
86	12.583	3588	3590	3593	rBV3	656	401	0.04%	0.005%
87	12.934	3693	3699	3705	rBV4	658	932	0.09%	0.011%
88	13.207	3778	3784	3788	rBV3	1177	1457	0.14%	0.018%
89	13.567	3894	3896	3897	rBV	598	262	0.03%	0.003%
90	13.686	3928	3933	3936	rBV4	1296	1304	0.13%	0.016%
91	13.741	3947	3950	3952	rBV	362	246	0.02%	0.003%
92	13.789	3961	3965	3966	rBV	597	371	0.04%	0.005%
93	13.831	3976	3978	3981	rBV2	298	170	0.02%	0.002%
94	13.892	3995	3997	4006	rVB4	613	728	0.07%	0.009%
95	13.931	4006	4009	4010	rBV	369	190	0.02%	0.002%
96	13.959	4015	4018	4021	rBV2	718	581	0.06%	0.007%
97	14.233	4100	4103	4105	rBV3	463	312	0.03%	0.004%
98	14.336	4134	4135	4137	rBV2	462	200	0.02%	0.002%
99	14.712	4249	4252	4253	rBV2	588	334	0.03%	0.004%
100	15.287	4427	4431	4433	rBV4	1074	839	0.08%	0.010%




Sum of corrected areas: 8108428

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033045.D
Acq On : 21 Nov 2023 11:55
Operator : SY/MD
Sample : 05436-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

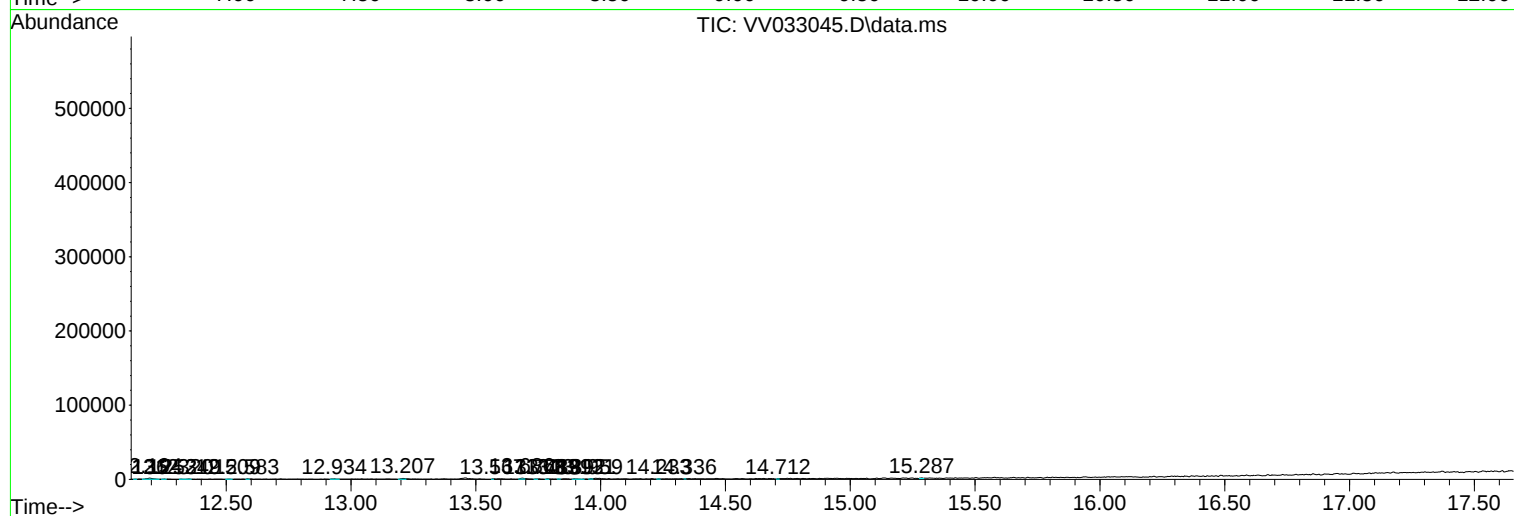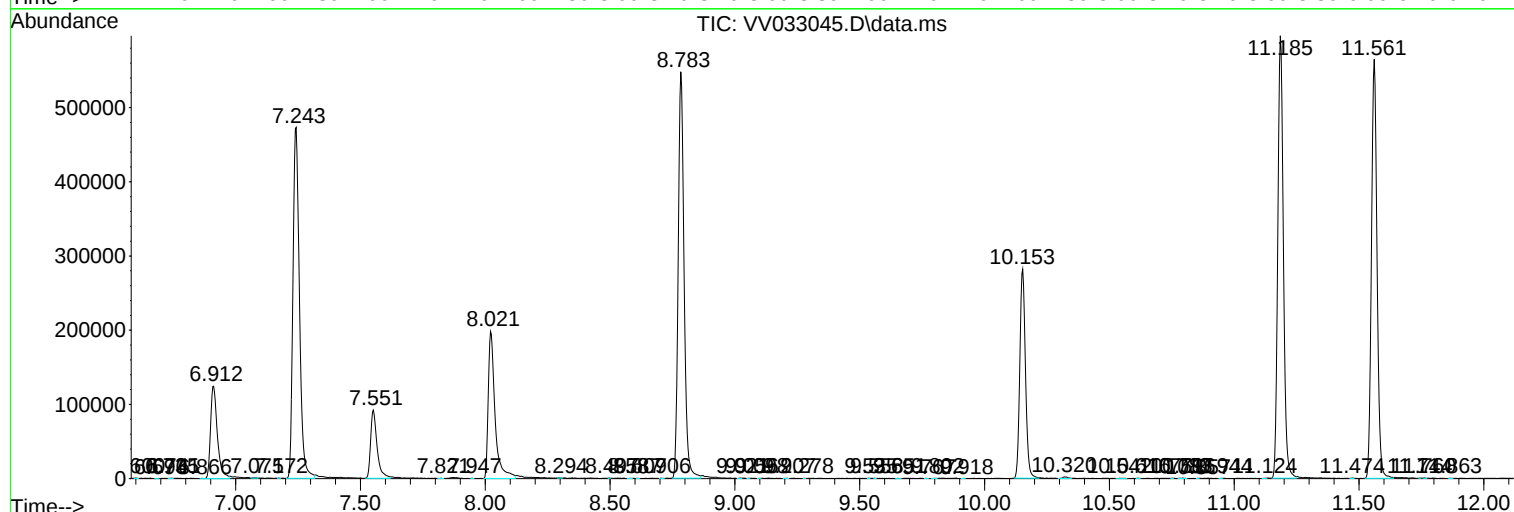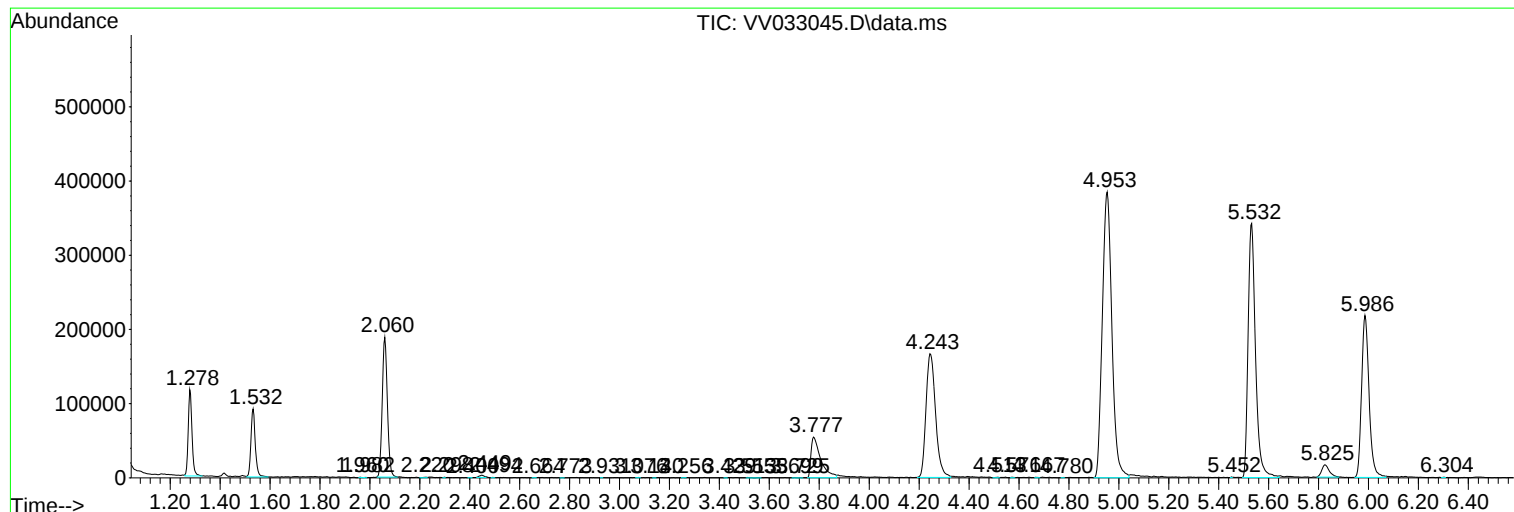

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033045.D
Acq On : 21 Nov 2023 11:55
Operator : SY/MD
Sample : 05436-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033045.D
Acq On : 21 Nov 2023 11:55
Operator : SY/MD
Sample : 05436-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc