

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033046.D
 Acq On : 21 Nov 2023 12:35
 Operator : SY/MD
 Sample : VIBLK254
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK254

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M

Title : VOC Analysis

Signal : TIC: VV033046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	114318	122662	11.14%	1.432%
2	1.532	146	153	172	rVB	90881	109647	9.96%	1.280%
3	1.963	283	287	290	rBV2	485	435	0.04%	0.005%
4	2.060	305	317	336	rBV	173349	256004	23.26%	2.988%
5	2.172	349	352	355	rBV	347	245	0.02%	0.003%
6	2.185	355	356	359	rVV	594	300	0.03%	0.004%
7	2.220	365	367	368	rBV	535	183	0.02%	0.002%
8	2.307	392	394	397	rBV3	654	293	0.03%	0.003%
9	2.420	425	429	431	rBV	662	444	0.04%	0.005%
10	2.445	431	437	448	rVB5	4345	7293	0.66%	0.085%
11	2.516	453	459	460	rBV2	363	329	0.03%	0.004%
12	2.648	498	500	504	rBV	279	202	0.02%	0.002%
13	2.677	507	509	514	rVB3	275	186	0.02%	0.002%
14	2.722	521	523	525	rBV	380	181	0.02%	0.002%
15	2.767	535	537	539	rBV	237	168	0.02%	0.002%
16	2.838	555	559	560	rBV2	332	234	0.02%	0.003%
17	2.934	584	589	591	rBV	325	288	0.03%	0.003%
18	2.963	595	598	600	rBV2	512	331	0.03%	0.004%
19	3.066	628	630	632	rVB2	394	156	0.01%	0.002%
20	3.208	672	674	677	rVB2	339	160	0.01%	0.002%
21	3.227	678	680	681	rBV2	366	194	0.02%	0.002%
22	3.301	700	703	705	rBV	269	211	0.02%	0.002%
23	3.384	727	729	732	rVB2	294	164	0.01%	0.002%
24	3.407	733	736	738	rBV	250	164	0.01%	0.002%
25	3.455	749	751	752	rBV	329	177	0.02%	0.002%
26	3.577	787	789	791	rVB	439	172	0.02%	0.002%
27	3.590	792	793	796	rBV	363	196	0.02%	0.002%
28	3.616	799	801	803	rBV	397	209	0.02%	0.002%
29	3.722	831	834	839	rVB	244	234	0.02%	0.003%
30	3.748	839	842	843	rBV	423	262	0.02%	0.003%
31	3.777	843	851	884	rBV	61032	166252	15.10%	1.940%
32	4.246	980	997	1021	rBV2	175124	446481	40.56%	5.211%
33	4.674	1128	1130	1133	rBV3	450	220	0.02%	0.003%
34	4.767	1156	1159	1161	rVB	446	202	0.02%	0.002%
35	4.786	1162	1165	1168	rBV2	425	290	0.03%	0.003%
36	4.851	1181	1185	1187	rBV	516	322	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112123\
 Data File : VW033046.D
 Acq On : 21 Nov 2023 12:35
 Operator : SY/MD
 Sample : VIBLK254
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK254

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	4.953	1200	1217	1252	rBV2	372956	1010983	91.84%	11.799%
38	5.532	1385	1397	1430	rBV	397712	823268	74.79%	9.608%
39	5.825	1479	1488	1504	rVB4	14864	31181	2.83%	0.364%
40	5.986	1525	1538	1561	rBV	218302	453726	41.22%	5.296%
41	6.275	1625	1628	1630	rBV2	437	279	0.03%	0.003%
42	6.400	1661	1667	1669	rBV3	441	418	0.04%	0.005%
43	6.500	1696	1698	1700	rBV	395	246	0.02%	0.003%
44	6.526	1704	1706	1708	rBV	395	222	0.02%	0.003%
45	6.667	1747	1750	1753	rVB	248	190	0.02%	0.002%
46	6.847	1803	1806	1807	rBV	254	166	0.02%	0.002%
47	6.912	1815	1826	1848	rBV	125482	233704	21.23%	2.728%
48	7.194	1913	1914	1917	rBV	265	170	0.02%	0.002%
49	7.243	1917	1929	1953	rBV	430116	766306	69.61%	8.944%
50	7.551	2015	2025	2049	rBV	93851	168232	15.28%	1.963%
51	7.828	2109	2111	2113	rBV2	270	144	0.01%	0.002%
52	8.021	2162	2171	2201	rBV	217945	407528	37.02%	4.756%
53	8.310	2259	2261	2265	rBV	394	193	0.02%	0.002%
54	8.452	2301	2305	2310	rBV	576	499	0.05%	0.006%
55	8.503	2318	2321	2322	rBV2	527	277	0.03%	0.003%
56	8.715	2385	2387	2391	rVB3	359	226	0.02%	0.003%
57	8.783	2396	2408	2432	rBV	636277	1043336	94.78%	12.177%
58	9.323	2570	2576	2579	rBV2	409	430	0.04%	0.005%
59	9.365	2587	2589	2591	rVB	434	166	0.02%	0.002%
60	9.490	2626	2628	2630	rBV	289	168	0.02%	0.002%
61	9.513	2632	2635	2640	rBV2	367	329	0.03%	0.004%
62	9.558	2645	2649	2652	rBV	363	287	0.03%	0.003%
63	9.632	2669	2672	2675	rBV	314	274	0.02%	0.003%
64	9.677	2681	2686	2687	rBV2	477	292	0.03%	0.003%
65	9.741	2702	2706	2709	rBV	258	230	0.02%	0.003%
66	9.876	2746	2748	2752	rVB2	516	307	0.03%	0.004%
67	9.905	2753	2757	2760	rBV	462	315	0.03%	0.004%
68	10.011	2786	2790	2792	rVV2	310	202	0.02%	0.002%
69	10.088	2810	2814	2817	rBV	362	256	0.02%	0.003%
70	10.153	2822	2834	2862	rBV	309154	488794	44.40%	5.705%
71	10.284	2872	2875	2877	rBV2	409	234	0.02%	0.003%
72	10.323	2882	2887	2891	rBV3	629	567	0.05%	0.007%
73	10.455	2923	2928	2929	rBV	414	313	0.03%	0.004%
74	10.882	3059	3061	3064	rBV	413	236	0.02%	0.003%
75	10.921	3071	3073	3077	rBV	275	232	0.02%	0.003%
76	11.005	3095	3099	3102	rBV	422	339	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112123\
 Data File : VV033046.D
 Acq On : 21 Nov 2023 12:35
 Operator : SY/MD
 Sample : VIBLK254
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK254

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	11.075	3117	3121	3123	rBV	282	190	0.02%	0.002%
78	11.185	3143	3155	3186	rBV	717354	1100846	100.00%	12.848%
79	11.352	3205	3207	3209	rBV2	378	219	0.02%	0.003%
80	11.419	3226	3228	3232	rBV2	581	449	0.04%	0.005%
81	11.561	3260	3272	3294	rBV	580358	909546	82.62%	10.615%
82	11.780	3337	3340	3341	rVB2	400	162	0.01%	0.002%
83	11.792	3341	3344	3347	rBV2	287	261	0.02%	0.003%
84	11.992	3404	3406	3409	rBV2	382	228	0.02%	0.003%
85	12.178	3461	3464	3467	rBV2	519	385	0.03%	0.004%
86	12.378	3523	3526	3529	rBV2	337	243	0.02%	0.003%
87	12.587	3589	3591	3593	rBV2	428	231	0.02%	0.003%
88	12.628	3600	3604	3605	rBV	283	176	0.02%	0.002%
89	12.706	3626	3628	3634	rVB2	348	261	0.02%	0.003%
90	12.786	3650	3653	3656	rBV2	307	258	0.02%	0.003%
91	12.902	3686	3689	3693	rBV2	484	455	0.04%	0.005%
92	12.943	3699	3702	3705	rBV	426	313	0.03%	0.004%
93	12.963	3706	3708	3713	rVV3	596	354	0.03%	0.004%
94	12.998	3716	3719	3721	rBV	285	160	0.01%	0.002%
95	13.027	3725	3728	3730	rBV	391	231	0.02%	0.003%
96	13.451	3853	3860	3861	rBV3	1013	970	0.09%	0.011%
97	13.574	3896	3898	3900	rBV2	622	346	0.03%	0.004%
98	13.622	3910	3913	3920	rVB3	676	528	0.05%	0.006%
99	13.734	3946	3948	3951	rBV	395	199	0.02%	0.002%
100	14.107	4062	4064	4068	rBV3	734	361	0.03%	0.004%




Sum of corrected areas: 8568128

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033046.D
Acq On : 21 Nov 2023 12:35
Operator : SY/MD
Sample : VIBLK254
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK254

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

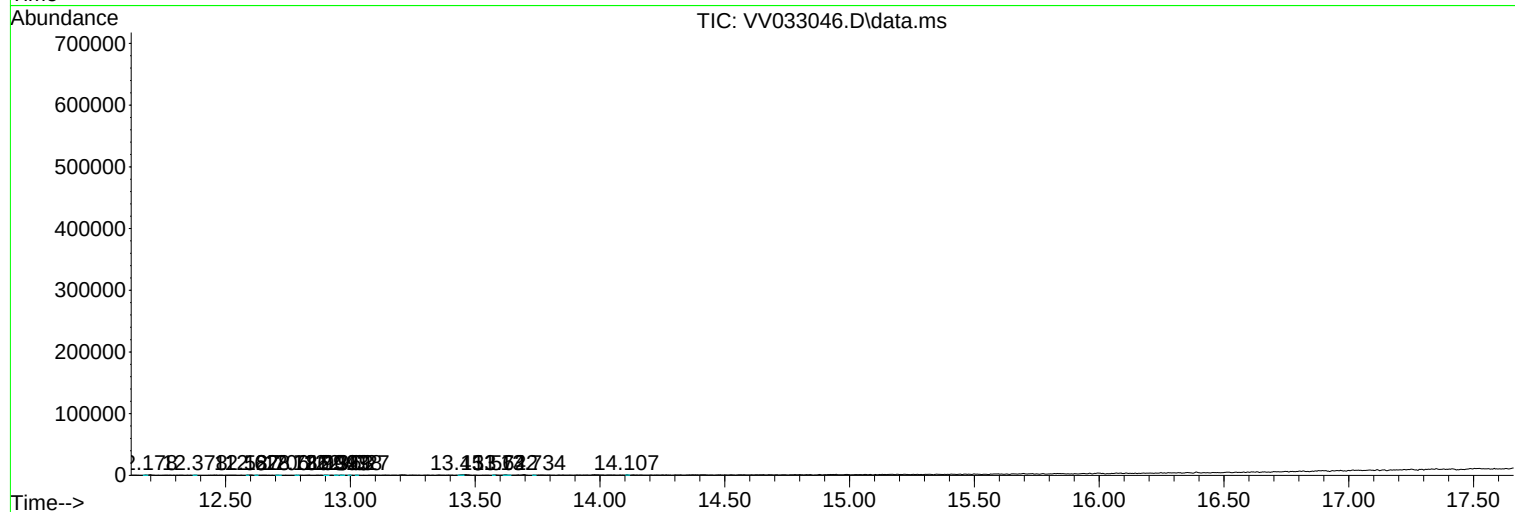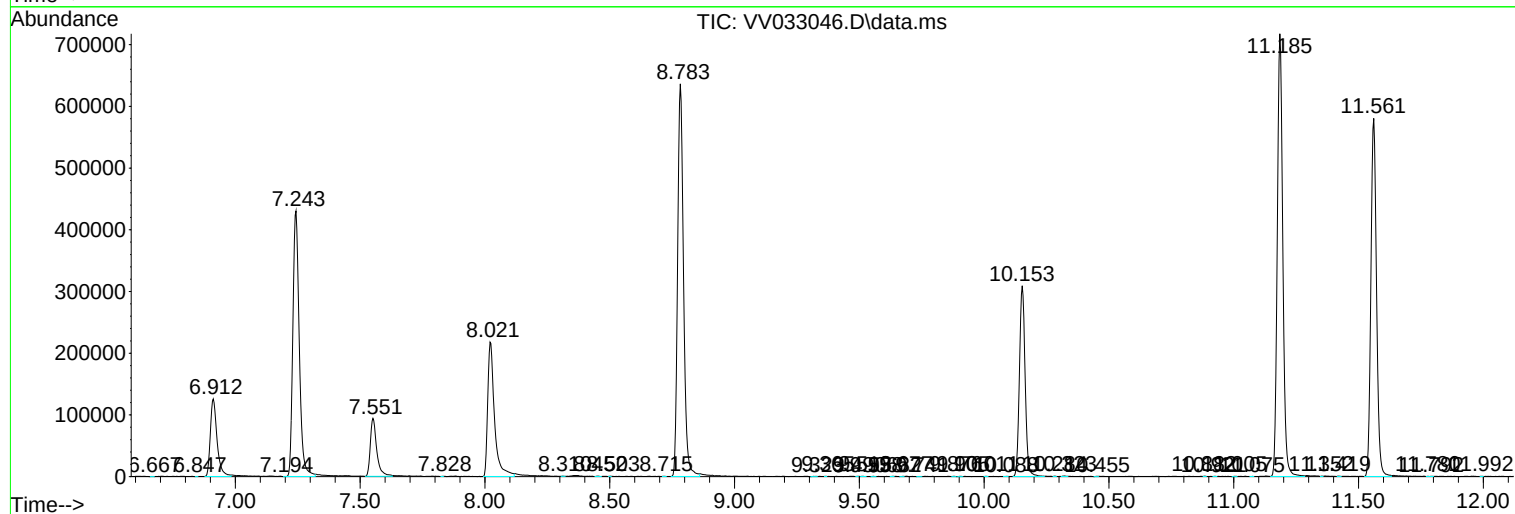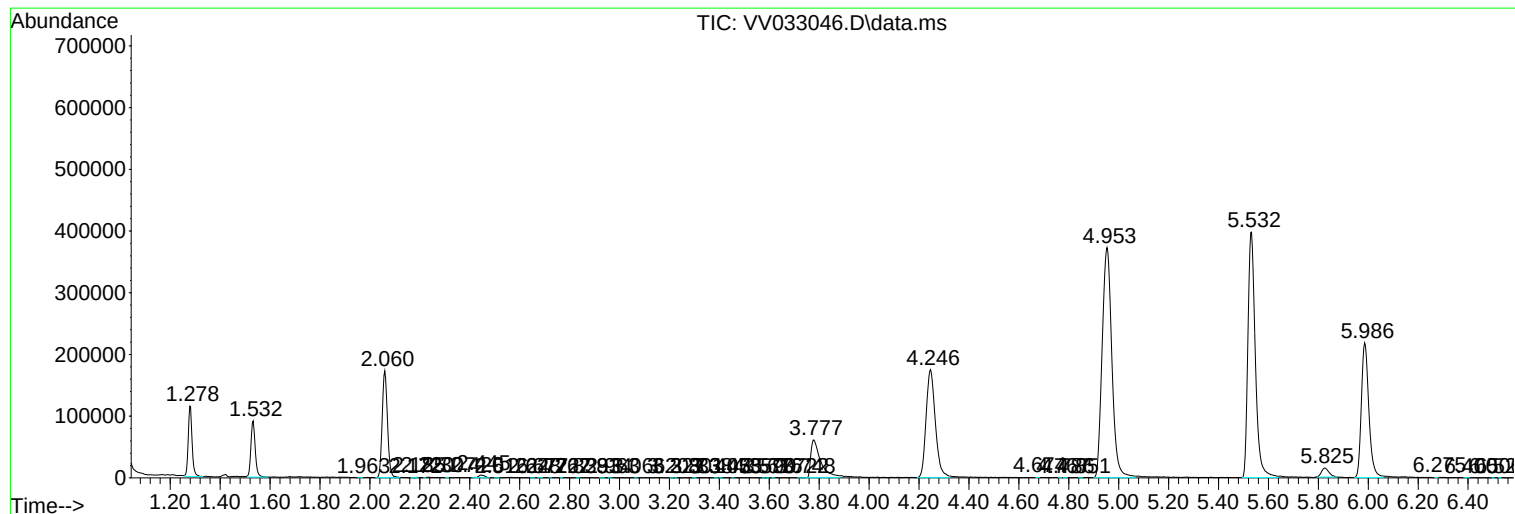

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033046.D
Acq On : 21 Nov 2023 12:35
Operator : SY/MD
Sample : VIBLK254
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK254

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033046.D
Acq On : 21 Nov 2023 12:35
Operator : SY/MD
Sample : VIBLK254
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK254

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------