

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033047.D
 Acq On : 21 Nov 2023 13:50
 Operator : SY/MD
 Sample : 05438-02ME
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1G3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	137637	170451	12.10%	1.579%
2	2.043	302	312	328	rBV	221287	323767	22.98%	3.000%
3	2.220	365	367	369	rBV	509	280	0.02%	0.003%
4	2.294	388	390	392	rBV2	384	219	0.02%	0.002%
5	2.362	409	411	412	rBV2	421	206	0.01%	0.002%
6	2.552	459	470	483	rBV3	4629	9721	0.69%	0.090%
7	2.674	506	508	512	rVB3	612	348	0.02%	0.003%
8	2.876	569	571	574	rBV2	409	223	0.02%	0.002%
9	2.896	574	577	580	rVV3	314	200	0.01%	0.002%
10	2.966	594	599	602	rBV3	548	530	0.04%	0.005%
11	3.031	615	619	620	rBV	330	215	0.02%	0.002%
12	3.050	623	625	628	rBV	403	237	0.02%	0.002%
13	3.172	659	663	666	rBV2	308	255	0.02%	0.002%
14	3.227	677	680	682	rBV	345	221	0.02%	0.002%
15	3.384	725	729	731	rVB2	359	247	0.02%	0.002%
16	3.416	736	739	741	rBV2	538	283	0.02%	0.003%
17	3.458	750	752	755	rBV2	490	297	0.02%	0.003%
18	3.651	808	812	813	rBV	404	297	0.02%	0.003%
19	3.719	830	833	836	rBV2	306	231	0.02%	0.002%
20	3.786	845	854	885	rBV2	55451	181120	12.86%	1.678%
21	4.243	981	996	1024	rBV	218511	561460	39.85%	5.202%
22	4.497	1073	1075	1079	rVB4	446	296	0.02%	0.003%
23	4.513	1079	1080	1083	rBV	333	193	0.01%	0.002%
24	4.812	1170	1173	1176	rVV	330	262	0.02%	0.002%
25	4.847	1181	1184	1186	rBV2	446	197	0.01%	0.002%
26	4.947	1198	1215	1253	rBV2	503179	1313219	93.21%	12.168%
27	5.236	1302	1305	1307	rBV2	447	337	0.02%	0.003%
28	5.529	1381	1396	1423	rBV	475540	989022	70.20%	9.164%
29	5.828	1477	1489	1505	rBV4	15690	36486	2.59%	0.338%
30	5.985	1525	1538	1567	rBV	277515	588771	41.79%	5.456%
31	6.207	1606	1607	1611	rBV2	683	563	0.04%	0.005%
32	6.420	1671	1673	1674	rBV	432	219	0.02%	0.002%
33	6.516	1699	1703	1705	rBV2	452	328	0.02%	0.003%
34	6.590	1721	1726	1728	rBV3	840	701	0.05%	0.006%
35	6.629	1736	1738	1740	rBV2	509	290	0.02%	0.003%
36	6.821	1796	1798	1800	rBV	358	234	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112123\
 Data File : VW033047.D
 Acq On : 21 Nov 2023 13:50
 Operator : SY/MD
 Sample : 05438-02ME
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1G3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	6.850	1803	1807	1810	rBV3	313	226	0.02%	0.002%
38	6.908	1815	1825	1852	rBV	165250	324334	23.02%	3.005%
39	7.137	1893	1896	1898	rBV2	685	436	0.03%	0.004%
40	7.239	1917	1928	1951	rBV	570484	1019231	72.34%	9.444%
41	7.551	2015	2025	2049	rBV2	115064	224056	15.90%	2.076%
42	7.802	2100	2103	2108	rBV3	506	400	0.03%	0.004%
43	7.863	2120	2122	2125	rBV3	378	248	0.02%	0.002%
44	7.911	2134	2137	2140	rBV2	503	241	0.02%	0.002%
45	7.927	2140	2142	2145	rVB2	588	263	0.02%	0.002%
46	7.944	2145	2147	2150	rBV	281	194	0.01%	0.002%
47	8.040	2165	2177	2215	rBV	191134	484139	34.36%	4.486%
48	8.645	2362	2365	2366	rBV	420	234	0.02%	0.002%
49	8.786	2396	2409	2435	rBV	728513	1276425	90.60%	11.827%
50	9.069	2495	2497	2499	rBV2	518	245	0.02%	0.002%
51	9.198	2533	2537	2539	rBV	380	267	0.02%	0.002%
52	9.220	2541	2544	2546	rBV	380	238	0.02%	0.002%
53	9.464	2615	2620	2622	rBV2	313	251	0.02%	0.002%
54	9.545	2643	2645	2648	rVB	342	201	0.01%	0.002%
55	9.567	2648	2652	2655	rBV	336	281	0.02%	0.003%
56	9.657	2677	2680	2681	rBV2	356	196	0.01%	0.002%
57	9.706	2693	2695	2697	rBV2	328	240	0.02%	0.002%
58	9.879	2747	2749	2752	rVB2	378	194	0.01%	0.002%
59	9.992	2782	2784	2788	rBV	325	193	0.01%	0.002%
60	10.017	2788	2792	2793	rVB	439	230	0.02%	0.002%
61	10.027	2793	2795	2799	rBV2	282	281	0.02%	0.003%
62	10.159	2823	2836	2854	rBV	381002	627535	44.54%	5.815%
63	10.384	2903	2906	2910	rVB2	460	336	0.02%	0.003%
64	10.648	2985	2988	2991	rVB2	339	206	0.01%	0.002%
65	10.667	2991	2994	2997	rBV	389	259	0.02%	0.002%
66	10.712	3005	3008	3009	rBV	488	297	0.02%	0.003%
67	10.863	3052	3055	3058	rVB2	559	333	0.02%	0.003%
68	10.882	3058	3061	3064	rBV2	353	251	0.02%	0.002%
69	10.898	3064	3066	3068	rVV2	441	222	0.02%	0.002%
70	10.911	3068	3070	3074	rVB	349	217	0.02%	0.002%
71	11.188	3144	3156	3181	rBV	924302	1408896	100.00%	13.055%
72	11.423	3227	3229	3234	rVB2	638	376	0.03%	0.003%
73	11.445	3234	3236	3240	rVB2	425	197	0.01%	0.002%
74	11.468	3240	3243	3247	rBV3	481	336	0.02%	0.003%
75	11.564	3260	3273	3295	rBV	790734	1226632	87.06%	11.366%
76	11.722	3320	3322	3327	rBV5	501	466	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112123\
 Data File : VW033047.D
 Acq On : 21 Nov 2023 13:50
 Operator : SY/MD
 Sample : 05438-02ME
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1G3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	11.943	3389	3391	3393	rBV2	553	321	0.02%	0.003%
78	11.982	3401	3403	3406	rVB2	458	199	0.01%	0.002%
79	12.014	3410	3413	3417	rBV	436	357	0.03%	0.003%
80	12.178	3460	3464	3465	rBV	596	375	0.03%	0.003%
81	12.197	3465	3470	3481	rVB4	1447	2021	0.14%	0.019%
82	12.249	3484	3486	3488	rBV4	521	225	0.02%	0.002%
83	12.310	3502	3505	3511	rVB	379	230	0.02%	0.002%
84	12.406	3532	3535	3537	rBV	340	244	0.02%	0.002%
85	12.593	3589	3593	3598	rBV2	645	581	0.04%	0.005%
86	12.635	3602	3606	3610	rBV	544	414	0.03%	0.004%
87	12.673	3617	3618	3622	rBV	494	270	0.02%	0.003%
88	12.744	3636	3640	3642	rBV2	410	371	0.03%	0.003%
89	12.795	3654	3656	3658	rVV2	416	202	0.01%	0.002%
90	12.879	3679	3682	3686	rVV2	423	301	0.02%	0.003%
91	13.107	3749	3753	3756	rBV4	546	437	0.03%	0.004%
92	13.162	3768	3770	3776	rVB3	499	416	0.03%	0.004%
93	13.332	3821	3823	3824	rBV	486	255	0.02%	0.002%
94	13.416	3847	3849	3851	rBV3	699	399	0.03%	0.004%
95	13.561	3891	3894	3896	rBV	594	380	0.03%	0.004%
96	13.638	3911	3918	3921	rBV4	902	1060	0.08%	0.010%
97	13.654	3921	3923	3925	rBV3	400	221	0.02%	0.002%
98	13.728	3944	3946	3947	rBV	874	335	0.02%	0.003%
99	13.808	3969	3971	3974	rBV	676	280	0.02%	0.003%
100	14.091	4056	4059	4061	rBV3	869	617	0.04%	0.006%




Sum of corrected areas: 10792240

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033047.D
Acq On : 21 Nov 2023 13:50
Operator : SY/MD
Sample : 05438-02ME
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1G3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

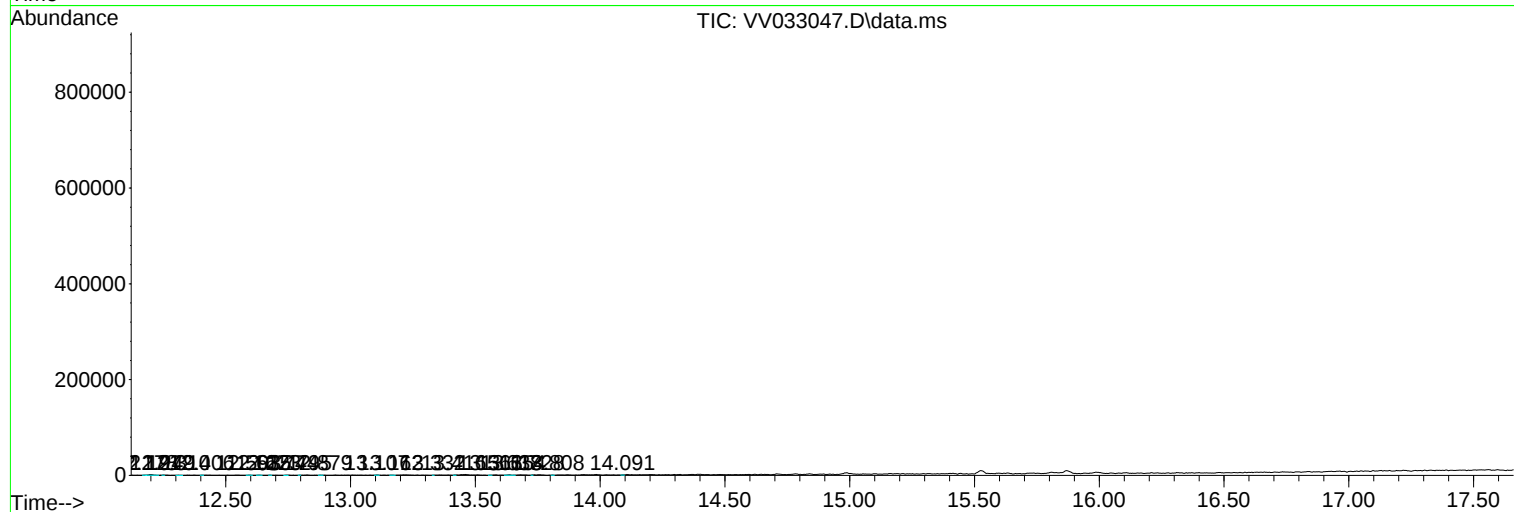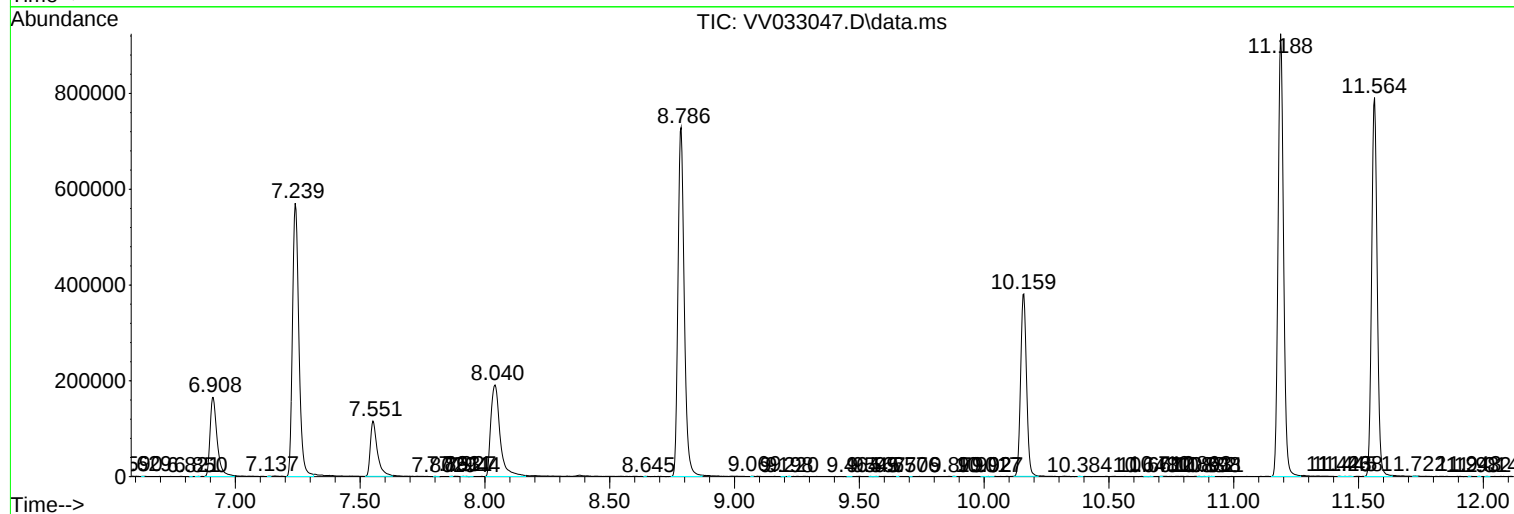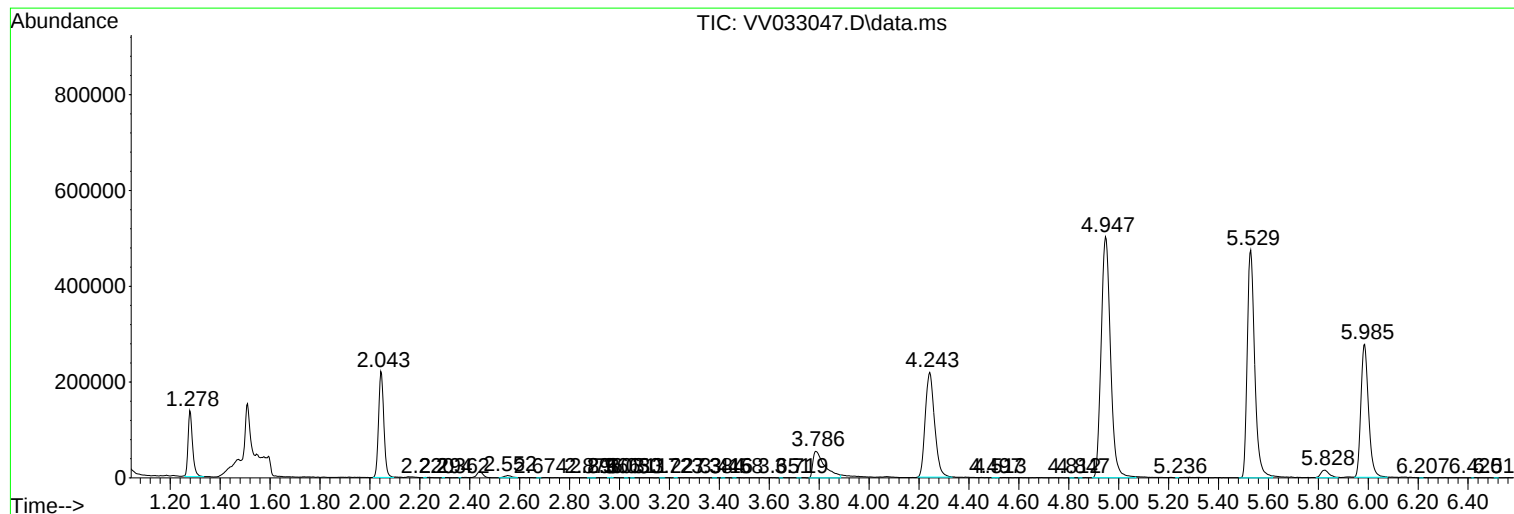

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033047.D
Acq On : 21 Nov 2023 13:50
Operator : SY/MD
Sample : 05438-02ME
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1G3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033047.D
Acq On : 21 Nov 2023 13:50
Operator : SY/MD
Sample : 05438-02ME
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1G3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc