

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033048.D
 Acq On : 21 Nov 2023 14:13
 Operator : SY/MD
 Sample : 05438-03ME
 Misc : 5.07G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1G4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	88	rVB	122769	154295	11.67%	1.459%
2	2.043	301	312	330	rBV	211123	309549	23.41%	2.928%
3	2.445	426	437	451	rVB3	10968	20995	1.59%	0.199%
4	2.555	459	471	486	rBV	5747	12549	0.95%	0.119%
5	2.957	593	596	604	rBV3	1100	1049	0.08%	0.010%
6	3.063	624	629	632	rBV	379	422	0.03%	0.004%
7	3.117	642	646	648	rBV2	245	195	0.01%	0.002%
8	3.166	660	661	667	rVB	464	222	0.02%	0.002%
9	3.217	674	677	680	rVB2	404	236	0.02%	0.002%
10	3.236	680	683	686	rVB2	442	310	0.02%	0.003%
11	3.259	687	690	693	rBV	462	366	0.03%	0.003%
12	3.281	693	697	700	rBV	421	400	0.03%	0.004%
13	3.310	702	706	708	rBV	363	191	0.01%	0.002%
14	3.449	745	749	752	rVB2	426	363	0.03%	0.003%
15	3.494	758	763	768	rBV3	532	508	0.04%	0.005%
16	3.542	772	778	781	rBV2	346	344	0.03%	0.003%
17	3.574	785	788	793	rVB	386	283	0.02%	0.003%
18	3.674	816	819	820	rBV	466	240	0.02%	0.002%
19	3.712	828	831	835	rBV2	360	282	0.02%	0.003%
20	3.793	845	856	887	rBV2	59747	202129	15.29%	1.912%
21	4.246	978	997	1034	rBV	208619	560874	42.42%	5.305%
22	4.490	1070	1073	1076	rBV3	633	446	0.03%	0.004%
23	4.571	1095	1098	1102	rBV3	541	481	0.04%	0.005%
24	4.735	1144	1149	1151	rBV2	305	312	0.02%	0.003%
25	4.789	1163	1166	1169	rVB	297	173	0.01%	0.002%
26	4.953	1200	1217	1250	rBV2	490070	1274900	96.42%	12.059%
27	5.368	1344	1346	1350	rVB	591	285	0.02%	0.003%
28	5.394	1350	1354	1356	rBV2	594	412	0.03%	0.004%
29	5.465	1371	1376	1378	rBV2	483	406	0.03%	0.004%
30	5.532	1384	1397	1433	rBV	444146	936288	70.81%	8.856%
31	5.825	1478	1488	1504	rBV2	14652	33174	2.51%	0.314%
32	5.985	1526	1538	1566	rBV	270613	577642	43.69%	5.464%
33	6.397	1661	1666	1669	rBV2	500	527	0.04%	0.005%
34	6.474	1685	1690	1695	rBV2	353	310	0.02%	0.003%
35	6.731	1765	1770	1773	rVV2	372	349	0.03%	0.003%
36	6.812	1792	1795	1801	rBV2	328	397	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112123\
 Data File : VW033048.D
 Acq On : 21 Nov 2023 14:13
 Operator : SY/MD
 Sample : 05438-03ME
 Misc : 5.07G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1G4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	6.860	1808	1810	1814	rVB	468	302	0.02%	0.003%
38	6.911	1814	1826	1857	rBV	160131	319325	24.15%	3.020%
39	7.063	1870	1873	1874	rBV	577	311	0.02%	0.003%
40	7.104	1883	1886	1891	rBV3	300	334	0.03%	0.003%
41	7.243	1918	1929	1953	rBV	558159	1000178	75.64%	9.460%
42	7.493	2005	2007	2008	rBV2	390	175	0.01%	0.002%
43	7.554	2016	2026	2055	rBV	110964	220271	16.66%	2.083%
44	7.751	2084	2087	2090	rBV3	704	511	0.04%	0.005%
45	7.834	2109	2113	2116	rBV3	536	328	0.02%	0.003%
46	7.857	2117	2120	2122	rBV3	411	231	0.02%	0.002%
47	7.870	2122	2124	2125	rBV	446	175	0.01%	0.002%
48	7.972	2153	2156	2158	rBV	307	197	0.01%	0.002%
49	8.046	2165	2179	2213	rBV2	198737	540191	40.85%	5.109%
50	8.477	2310	2313	2316	rBV	395	283	0.02%	0.003%
51	8.554	2332	2337	2341	rBV2	538	503	0.04%	0.005%
52	8.654	2363	2368	2370	rBV4	623	462	0.03%	0.004%
53	8.664	2370	2371	2375	rVV3	367	192	0.01%	0.002%
54	8.722	2386	2389	2391	rBV	378	253	0.02%	0.002%
55	8.786	2397	2409	2439	rBV	681830	1207498	91.32%	11.421%
56	9.043	2486	2489	2490	rBV	433	265	0.02%	0.003%
57	9.085	2500	2502	2507	rBV3	310	188	0.01%	0.002%
58	9.156	2519	2524	2526	rBV2	492	360	0.03%	0.003%
59	9.236	2546	2549	2553	rBV2	362	315	0.02%	0.003%
60	9.294	2565	2567	2569	rBV2	287	181	0.01%	0.002%
61	9.361	2583	2588	2591	rBV2	323	298	0.02%	0.003%
62	9.448	2613	2615	2619	rVB	448	236	0.02%	0.002%
63	9.519	2635	2637	2639	rBV	492	244	0.02%	0.002%
64	9.847	2737	2739	2744	rVV	281	234	0.02%	0.002%
65	10.059	2802	2805	2807	rBV	559	349	0.03%	0.003%
66	10.114	2820	2822	2823	rBV	390	179	0.01%	0.002%
67	10.159	2824	2836	2860	rVV	391893	655401	49.57%	6.199%
68	10.410	2910	2914	2920	rBV	476	530	0.04%	0.005%
69	10.487	2936	2938	2941	rVV2	382	210	0.02%	0.002%
70	10.612	2974	2977	2980	rBV	319	208	0.02%	0.002%
71	10.664	2991	2993	2997	rBV	327	197	0.01%	0.002%
72	10.718	3005	3010	3013	rBV2	261	303	0.02%	0.003%
73	10.847	3044	3050	3053	rBV2	297	294	0.02%	0.003%
74	10.950	3079	3082	3086	rVB	411	228	0.02%	0.002%
75	11.014	3100	3102	3107	rVB2	324	190	0.01%	0.002%
76	11.066	3115	3118	3119	rBV	350	179	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033048.D
 Acq On : 21 Nov 2023 14:13
 Operator : SY/MD
 Sample : 05438-03ME
 Misc : 5.07G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1G4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	11.136	3135	3140	3142	rBV2	603	652	0.05%	0.006%
78	11.188	3144	3156	3178	rBV	841169	1322288	100.00%	12.507%
79	11.564	3261	3273	3292	rBV	774891	1197214	90.54%	11.324%
80	11.879	3369	3371	3375	rBV2	469	359	0.03%	0.003%
81	11.972	3396	3400	3401	rBV2	272	182	0.01%	0.002%
82	12.017	3412	3414	3419	rVB3	615	362	0.03%	0.003%
83	12.107	3440	3442	3446	rBV3	375	212	0.02%	0.002%
84	12.197	3461	3470	3477	rBV6	1313	2265	0.17%	0.021%
85	12.252	3481	3487	3492	rBV2	570	546	0.04%	0.005%
86	12.374	3523	3525	3529	rBV	293	194	0.01%	0.002%
87	12.512	3565	3568	3571	rBV	457	279	0.02%	0.003%
88	12.664	3613	3615	3617	rBV	553	296	0.02%	0.003%
89	12.805	3656	3659	3660	rBV2	476	266	0.02%	0.003%
90	12.840	3668	3670	3673	rBV2	328	176	0.01%	0.002%
91	12.857	3673	3675	3678	rVB2	472	217	0.02%	0.002%
92	12.924	3692	3696	3699	rBV	417	342	0.03%	0.003%
93	12.947	3699	3703	3704	rBV	329	241	0.02%	0.002%
94	12.982	3712	3714	3716	rBV2	453	224	0.02%	0.002%
95	13.104	3750	3752	3755	rVB2	469	176	0.01%	0.002%
96	13.168	3769	3772	3775	rBV	243	225	0.02%	0.002%
97	13.246	3794	3796	3801	rVB2	523	369	0.03%	0.003%
98	13.413	3845	3848	3850	rBV	500	392	0.03%	0.004%
99	13.831	3976	3978	3984	rVB3	495	291	0.02%	0.003%
100	14.056	4046	4048	4053	rVB	503	330	0.02%	0.003%




Sum of corrected areas: 10572311

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033048.D
Acq On : 21 Nov 2023 14:13
Operator : SY/MD
Sample : 05438-03ME
Misc : 5.07G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1G4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

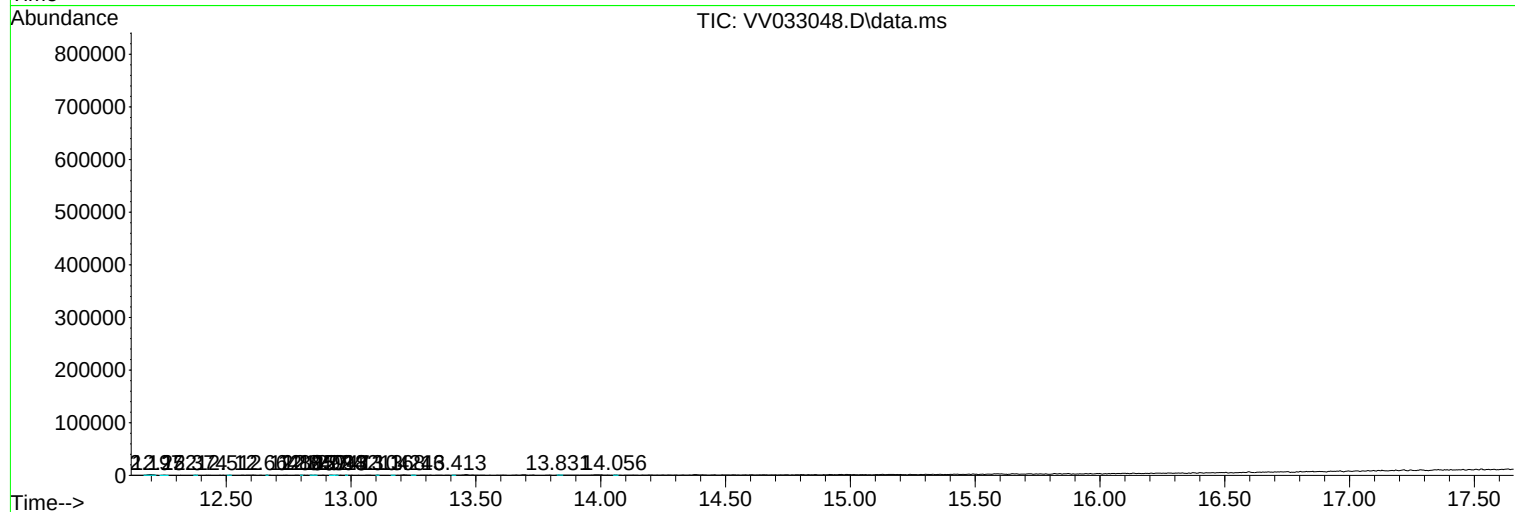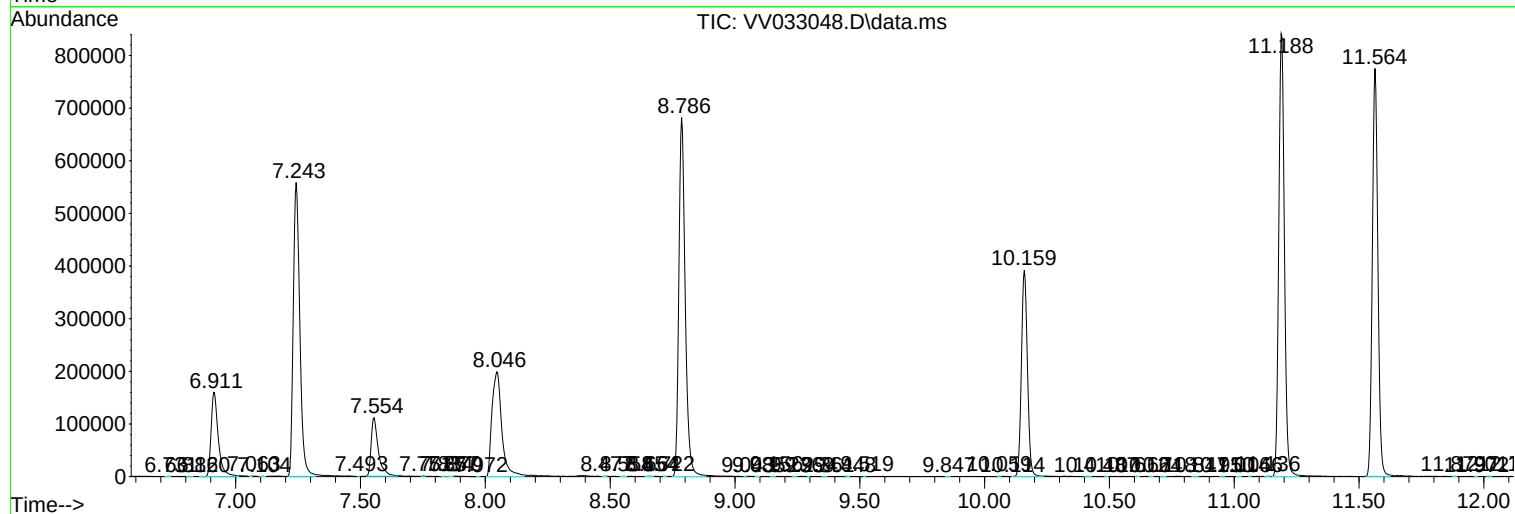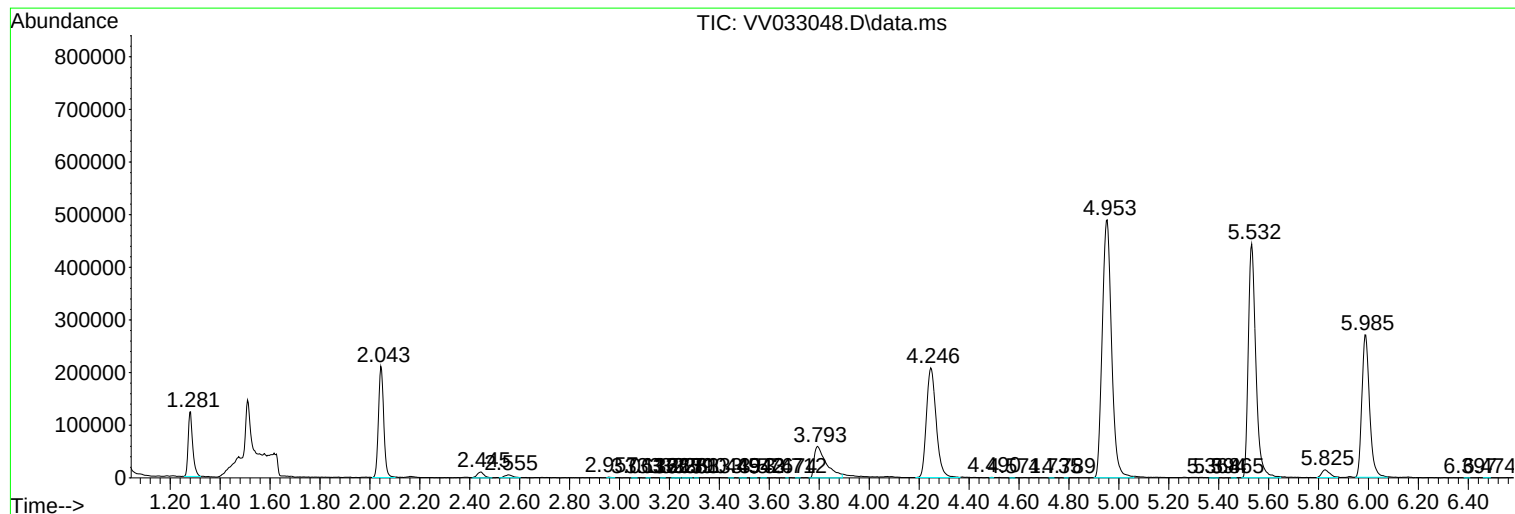

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033048.D
Acq On : 21 Nov 2023 14:13
Operator : SY/MD
Sample : 05438-03ME
Misc : 5.07G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1G4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033048.D
Acq On : 21 Nov 2023 14:13
Operator : SY/MD
Sample : 05438-03ME
Misc : 5.07G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1G4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc