

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112123\
 Data File : VW033049.D
 Acq On : 21 Nov 2023 14:36
 Operator : SY/MD
 Sample : 05438-04ME
 Misc : 5.06G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1G5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VW033049.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	85424	109787	9.54%	1.396%
2	2.047	302	313	329	rBV	146776	215809	18.74%	2.744%
3	2.336	401	403	405	rBV	404	216	0.02%	0.003%
4	2.378	409	416	423	rBV6	1243	2224	0.19%	0.028%
5	2.442	427	436	448	rVB4	11043	19050	1.65%	0.242%
6	2.558	460	472	487	rBV2	7372	14452	1.26%	0.184%
7	2.793	542	545	548	rBV	445	405	0.04%	0.005%
8	2.822	552	554	556	rBB2	265	139	0.01%	0.002%
9	2.841	557	560	561	rBV	263	151	0.01%	0.002%
10	2.864	565	567	569	rBV	230	139	0.01%	0.002%
11	2.896	575	577	579	rBV	211	111	0.01%	0.001%
12	2.995	606	608	615	rVB3	370	317	0.03%	0.004%
13	3.089	635	637	639	rBV	243	93	0.01%	0.001%
14	3.166	659	661	666	rVB2	518	346	0.03%	0.004%
15	3.198	667	671	676	rBV	499	505	0.04%	0.006%
16	3.256	687	689	691	rBV	240	158	0.01%	0.002%
17	3.278	695	696	697	rBV	236	82	0.01%	0.001%
18	3.372	723	725	726	rBV	251	102	0.01%	0.001%
19	3.397	731	733	734	rBV	269	129	0.01%	0.002%
20	3.481	755	759	763	rVV2	275	325	0.03%	0.004%
21	3.516	767	770	772	rBV2	167	139	0.01%	0.002%
22	3.564	783	785	787	rBV	224	108	0.01%	0.001%
23	3.622	801	803	805	rBV	244	122	0.01%	0.002%
24	3.638	805	808	810	rVV2	158	100	0.01%	0.001%
25	3.651	810	812	814	rVB	131	50	0.00%	0.001%
26	3.664	814	816	818	rBV	361	196	0.02%	0.002%
27	3.716	831	832	834	rBV	242	88	0.01%	0.001%
28	3.728	834	836	837	rBV	210	86	0.01%	0.001%
29	3.764	844	847	848	rBV	230	106	0.01%	0.001%
30	3.796	848	857	886	rBV	39838	131511	11.42%	1.672%
31	4.246	981	997	1026	rBV	144039	382796	33.25%	4.867%
32	4.468	1064	1066	1070	rVB3	436	265	0.02%	0.003%
33	4.490	1070	1073	1074	rBV2	418	256	0.02%	0.003%
34	4.529	1083	1085	1087	rBV2	384	174	0.02%	0.002%
35	4.571	1097	1098	1100	rVB2	291	71	0.01%	0.001%
36	4.597	1100	1106	1107	rBV2	481	447	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112123\
 Data File : VW033049.D
 Acq On : 21 Nov 2023 14:36
 Operator : SY/MD
 Sample : 05438-04ME
 Misc : 5.06G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1G5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	4.632	1114	1117	1121	rVB3	290	259	0.02%	0.003%
38	4.738	1148	1150	1152	rBV	162	51	0.00%	0.001%
39	4.767	1155	1159	1160	rBV	204	135	0.01%	0.002%
40	4.825	1173	1177	1179	rBV	310	227	0.02%	0.003%
41	4.896	1197	1199	1201	rBV2	246	141	0.01%	0.002%
42	4.953	1201	1217	1247	rBV2	334456	870156	75.57%	11.063%
43	5.227	1301	1302	1306	rBV	363	291	0.03%	0.004%
44	5.439	1366	1368	1369	rBV	177	62	0.01%	0.001%
45	5.468	1375	1377	1378	rBV	303	95	0.01%	0.001%
46	5.532	1385	1397	1425	rBV	373535	789157	68.54%	10.033%
47	5.828	1479	1489	1503	rBV3	10252	22860	1.99%	0.291%
48	5.989	1528	1539	1566	rVB	181890	387230	33.63%	4.923%
49	6.137	1582	1585	1586	rBV3	594	256	0.02%	0.003%
50	6.188	1599	1601	1602	rBV3	302	85	0.01%	0.001%
51	6.198	1602	1604	1607	rVB	501	231	0.02%	0.003%
52	6.233	1614	1615	1616	rBV	391	149	0.01%	0.002%
53	6.262	1622	1624	1625	rBV	227	91	0.01%	0.001%
54	6.326	1641	1644	1647	rBV	420	281	0.02%	0.004%
55	6.378	1658	1660	1661	rBV	230	77	0.01%	0.001%
56	6.455	1682	1684	1685	rBV	191	57	0.00%	0.001%
57	6.494	1694	1696	1700	rVB	247	187	0.02%	0.002%
58	6.513	1700	1702	1705	rBV	308	191	0.02%	0.002%
59	6.532	1706	1708	1711	rVB2	491	247	0.02%	0.003%
60	6.564	1712	1718	1719	rBV2	408	339	0.03%	0.004%
61	6.629	1735	1738	1740	rBV2	433	338	0.03%	0.004%
62	6.722	1764	1767	1774	rVB2	517	354	0.03%	0.005%
63	6.767	1779	1781	1783	rVV2	176	73	0.01%	0.001%
64	6.796	1788	1790	1794	rVB2	273	170	0.01%	0.002%
65	6.815	1794	1796	1797	rBV2	210	60	0.01%	0.001%
66	6.850	1802	1807	1809	rBV	405	341	0.03%	0.004%
67	6.867	1810	1812	1816	rVB	321	121	0.01%	0.002%
68	6.915	1816	1827	1849	rBV	107356	216069	18.77%	2.747%
69	7.133	1893	1895	1896	rBV	295	138	0.01%	0.002%
70	7.140	1896	1897	1900	rVV2	454	276	0.02%	0.004%
71	7.243	1918	1929	1960	rBV	375538	685796	59.56%	8.719%
72	7.555	2017	2026	2061	rBV	76848	155510	13.51%	1.977%
73	7.728	2077	2080	2083	rVB3	417	299	0.03%	0.004%
74	7.751	2083	2087	2091	rVB3	627	598	0.05%	0.008%
75	7.770	2091	2093	2094	rBV	552	237	0.02%	0.003%
76	7.867	2119	2123	2125	rBV2	902	705	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
 Data File : VV033049.D
 Acq On : 21 Nov 2023 14:36
 Operator : SY/MD
 Sample : 05438-04ME
 Misc : 5.06G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1G5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	7.963	2152	2153	2154	rBV2	286	94	0.01%	0.001%
78	8.047	2166	2179	2203	rBV2	131937	343766	29.86%	4.371%
79	8.539	2330	2332	2336	rBV	362	274	0.02%	0.003%
80	8.580	2344	2345	2346	rBV	231	76	0.01%	0.001%
81	8.651	2364	2367	2370	rBV4	969	695	0.06%	0.009%
82	8.690	2378	2379	2381	rBV	243	98	0.01%	0.001%
83	8.731	2386	2392	2393	rBV2	711	571	0.05%	0.007%
84	8.786	2397	2409	2432	rBV	570516	1013883	88.06%	12.891%
85	9.082	2497	2501	2503	rBV	724	458	0.04%	0.006%
86	9.124	2513	2514	2516	rBV2	466	143	0.01%	0.002%
87	9.143	2518	2520	2523	rBV2	424	247	0.02%	0.003%
88	9.178	2529	2531	2533	rBV	501	239	0.02%	0.003%
89	9.223	2543	2545	2546	rBV	211	55	0.00%	0.001%
90	9.346	2579	2583	2584	rBV	674	444	0.04%	0.006%
91	9.381	2588	2594	2595	rBV3	918	863	0.07%	0.011%
92	9.567	2649	2652	2659	rVB5	1185	1071	0.09%	0.014%
93	9.612	2659	2666	2669	rBV4	2088	2555	0.22%	0.032%
94	9.911	2751	2759	2767	rBV8	3487	5735	0.50%	0.073%
95	9.956	2767	2773	2785	rVB7	4378	7858	0.68%	0.100%
96	10.092	2813	2815	2816	rBV	426	207	0.02%	0.003%
97	10.159	2825	2836	2853	rVB	276173	467382	40.59%	5.942%
98	11.188	3146	3156	3177	rBV	743940	1151387	100.00%	14.639%
99	11.564	3262	3273	3291	rBV	530885	842655	73.19%	10.714%
100	12.310	3496	3505	3510	rBV	5440	9490	0.82%	0.121%




Sum of corrected areas: 7865241

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033049.D
Acq On : 21 Nov 2023 14:36
Operator : SY/MD
Sample : 05438-04ME
Misc : 5.06G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1G5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

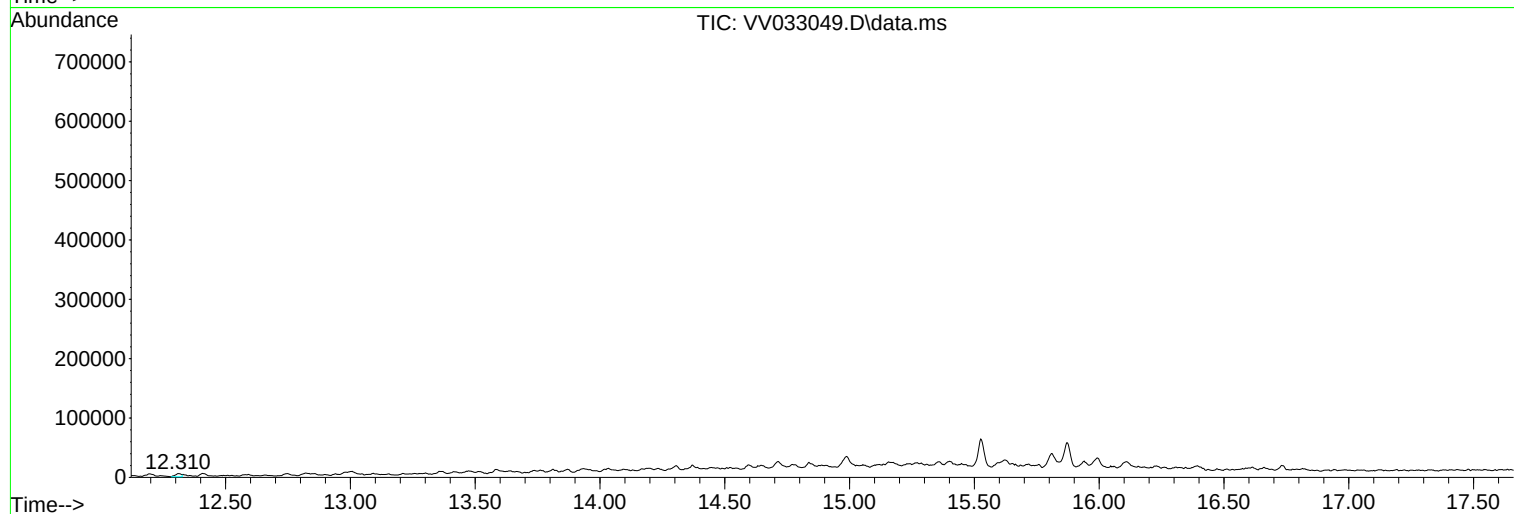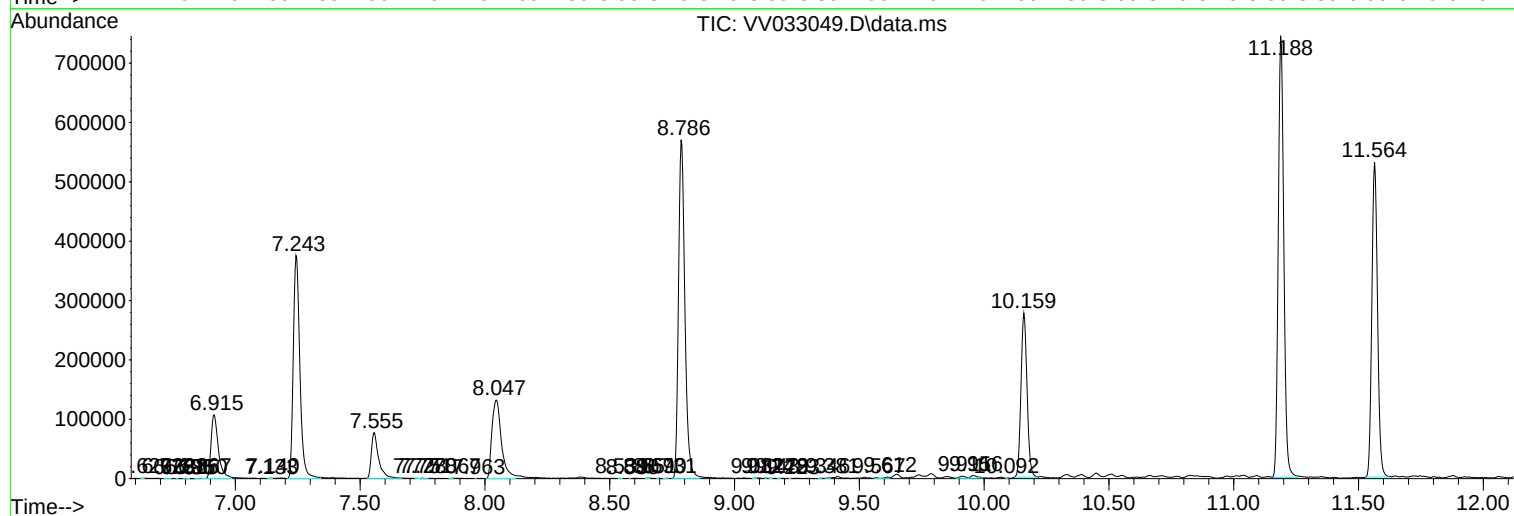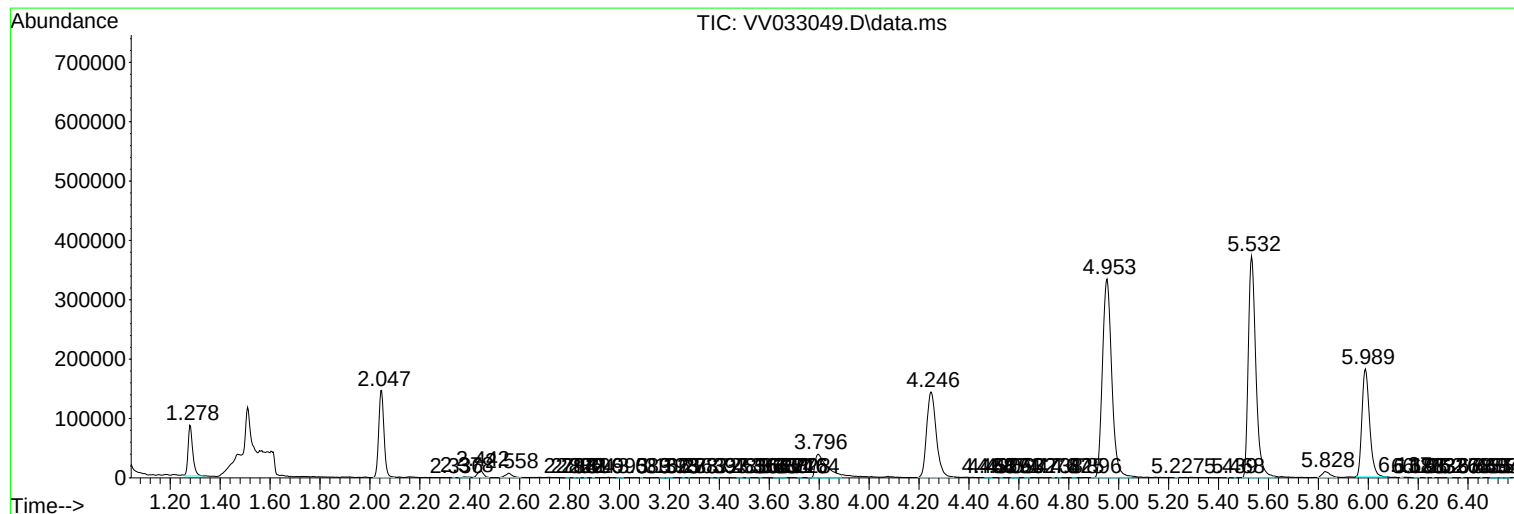

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033049.D
Acq On : 21 Nov 2023 14:36
Operator : SY/MD
Sample : 05438-04ME
Misc : 5.06G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1G5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033049.D
Acq On : 21 Nov 2023 14:36
Operator : SY/MD
Sample : 05438-04ME
Misc : 5.06G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1G5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------