


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112123\
Data File : VV033039.D
Acq On : 21 Nov 2023 08:16
Operator : SY/MD
Sample : BFB235
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB235

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Title : VOC Analysis
Last Update : Wed Nov 22 03:48:12 2023

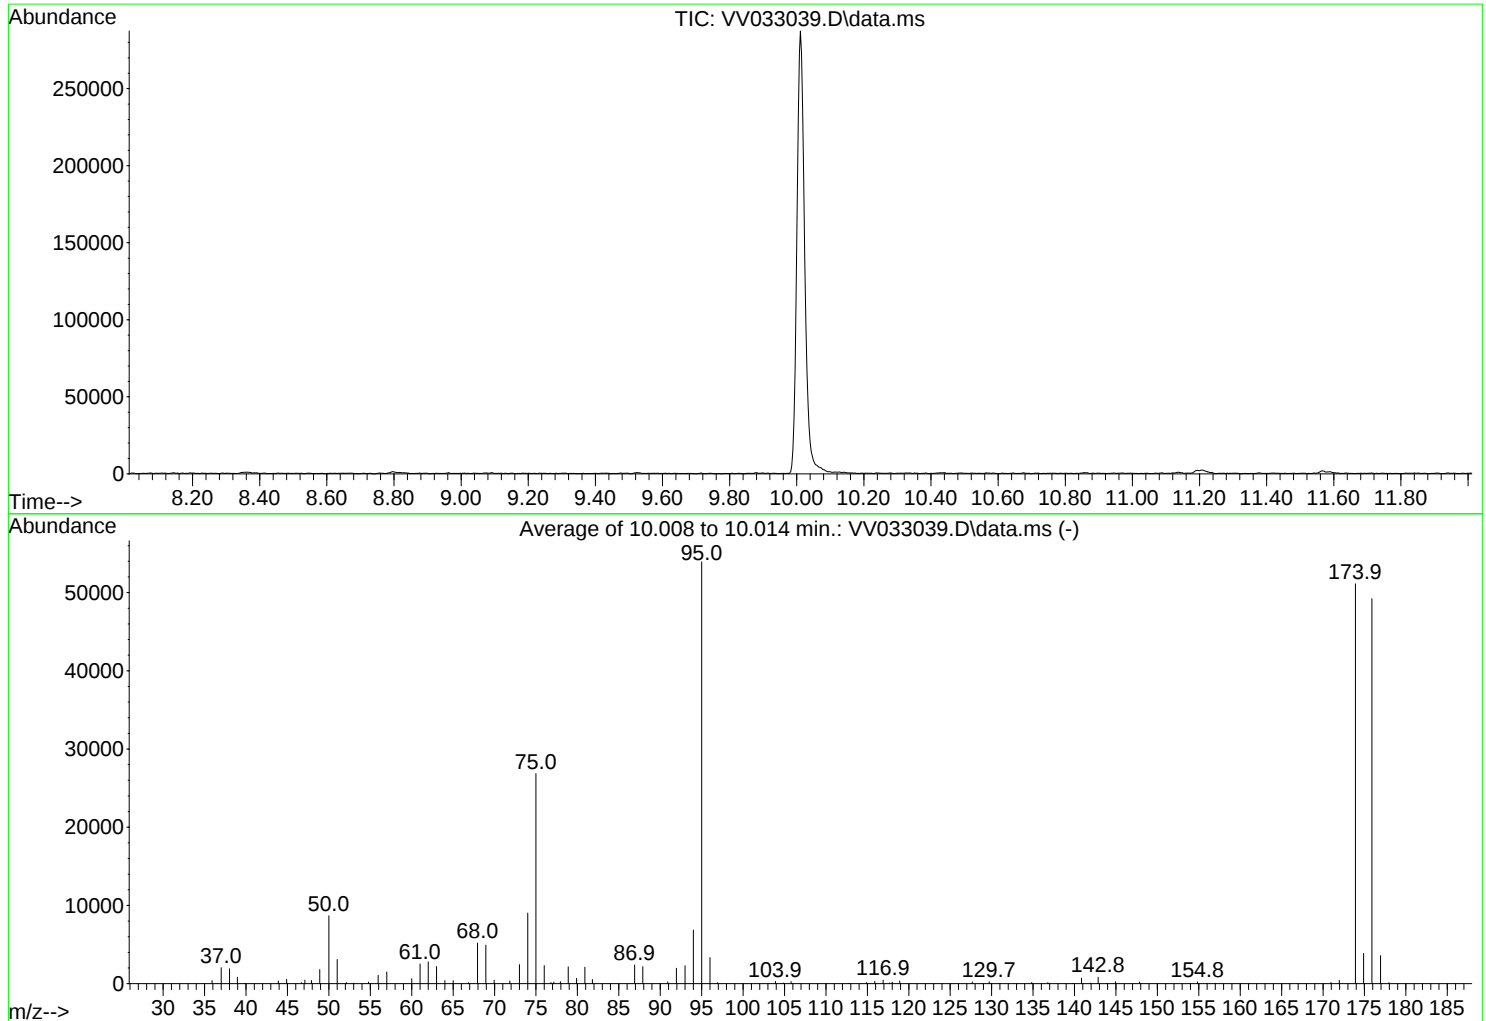

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	8676	PASS
75	95	30	80	49.8	26872	PASS
95	95	100	100	100.0	53931	PASS
96	95	5	9	6.2	3339	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.8	51131	PASS
175	174	5	9	7.5	3860	PASS
176	174	95	105	96.3	49224	PASS
177	176	5	10	7.3	3590	PASS

m/z	Abundance
39.80	142.0
43.80	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
35.90	397.0
37.00	2035.0
38.00	1921.0
39.00	718.0
39.90	197.0
43.90	512.0
44.90	580.0
46.70	400.0
47.10	406.0
47.90	445.0
48.90	1740.0
50.00	8633.0
51.00	3128.0
52.10	125.0
54.80	146.0
55.90	989.0
57.00	1445.0
60.00	601.0
61.00	2447.0
62.00	2642.0
63.00	2117.0
64.00	442.0
65.00	350.0
66.80	104.0
67.90	5345.0
69.00	5187.0
70.00	398.0
71.90	347.0
73.00	2434.0
74.00	9132.0
75.00	26800.0
76.00	2160.0
76.80	226.0
77.10	236.0
77.90	246.0
78.90	2013.0
79.90	689.0
80.90	2093.0
81.80	518.0
86.90	2186.0
87.90	2105.0
90.90	225.0
91.90	1912.0
93.00	2194.0
94.00	6611.0
95.00	53176.0
96.00	3388.0
96.90	106.0
104.00	292.0
105.80	303.0
112.70	100.0
115.00	125.0
116.00	254.0
117.00	439.0
117.70	267.0
118.90	358.0
127.70	199.0
129.70	273.0
134.80	133.0
136.90	152.0
139.80	101.0
140.90	753.0
142.90	806.0
143.90	114.0
145.00	203.0
147.80	210.0
154.80	243.0
157.00	100.0
170.90	174.0
171.90	408.0
173.90	50224.0
174.90	3766.0
175.90	47416.0
177.00	3500.0
178.00	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
35.90	383.0
37.00	2140.0
38.00	1944.0
38.90	864.0
39.90	177.0
44.00	545.0
44.90	582.0
47.10	469.0
47.90	456.0
48.90	1816.0
50.00	8880.0
51.00	3281.0
52.10	154.0
54.80	194.0
55.90	1137.0
57.00	1558.0
60.00	676.0
61.00	2575.0
62.00	2861.0
63.00	2286.0
64.00	427.0
65.00	404.0
66.90	125.0
67.90	5414.0
69.00	4990.0
70.00	465.0
71.80	378.0
73.00	2501.0
74.00	9363.0
75.00	27808.0
76.00	2461.0
76.80	192.0
77.20	208.0
78.00	247.0
78.90	2216.0
79.90	723.0
80.90	2206.0
81.80	577.0
86.90	2429.0
87.90	2227.0
90.90	229.0
92.00	2056.0
93.00	2345.0
94.00	7066.0
95.00	55728.0
96.00	3409.0
96.90	133.0
103.90	288.0
104.80	110.0
105.80	262.0
114.80	132.0
115.90	300.0
116.90	474.0
118.00	275.0
118.90	368.0
127.70	223.0
129.70	241.0
134.80	169.0
136.80	126.0
140.90	738.0
141.90	111.0
142.90	835.0
144.90	280.0
147.90	228.0
154.90	245.0
171.00	158.0
171.90	453.0
173.90	53080.0
174.90	4015.0
175.90	51112.0
177.00	3722.0
178.00	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
35.90	379.0
37.00	1984.0
38.00	1872.0
38.90	905.0
39.90	149.0
44.00	463.0
44.90	479.0
47.10	464.0
47.90	345.0
48.90	1819.0
50.00	8514.0
51.00	2845.0
52.10	171.0
53.00	181.0
54.80	250.0
56.00	1075.0
57.00	1508.0
60.00	623.0
61.00	2527.0
62.00	2852.0
63.00	2187.0
64.00	309.0
65.00	386.0
66.90	165.0
68.00	4842.0
68.90	4646.0
69.90	479.0
71.90	314.0
73.00	2359.0
74.00	8552.0
75.00	26008.0
76.00	2318.0
77.20	196.0
78.00	245.0
78.90	2205.0
79.90	644.0
80.90	2043.0
81.80	515.0
86.90	2555.0
87.90	2193.0
90.90	233.0
92.00	1952.0
93.00	2313.0
94.00	6854.0
95.00	52888.0
96.00	3220.0
96.90	157.0
103.80	259.0
104.90	127.0
105.80	241.0
114.90	160.0
115.80	305.0
116.80	465.0
118.00	306.0
118.90	313.0
127.60	237.0
129.70	216.0
131.00	107.0
134.90	195.0
136.70	160.0
140.80	656.0
141.90	142.0
142.80	815.0
144.90	281.0
147.90	196.0
154.90	211.0
171.00	129.0
172.00	452.0
173.90	50088.0
174.90	3799.0
175.90	49144.0
176.90	3549.0
177.90	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235