
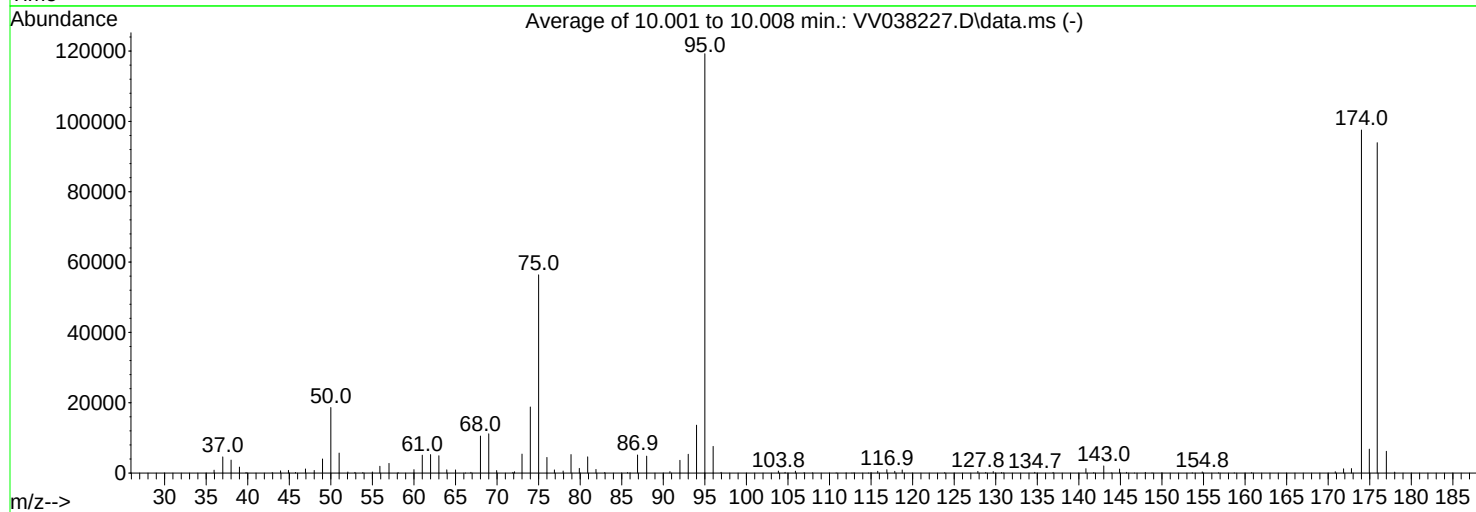


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112124\
Data File : VV038227.D
Acq On : 21 Nov 2024 07:53
Operator : SY/MD
Sample : BFB289
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB289

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Nov 25 00:21:44 2024

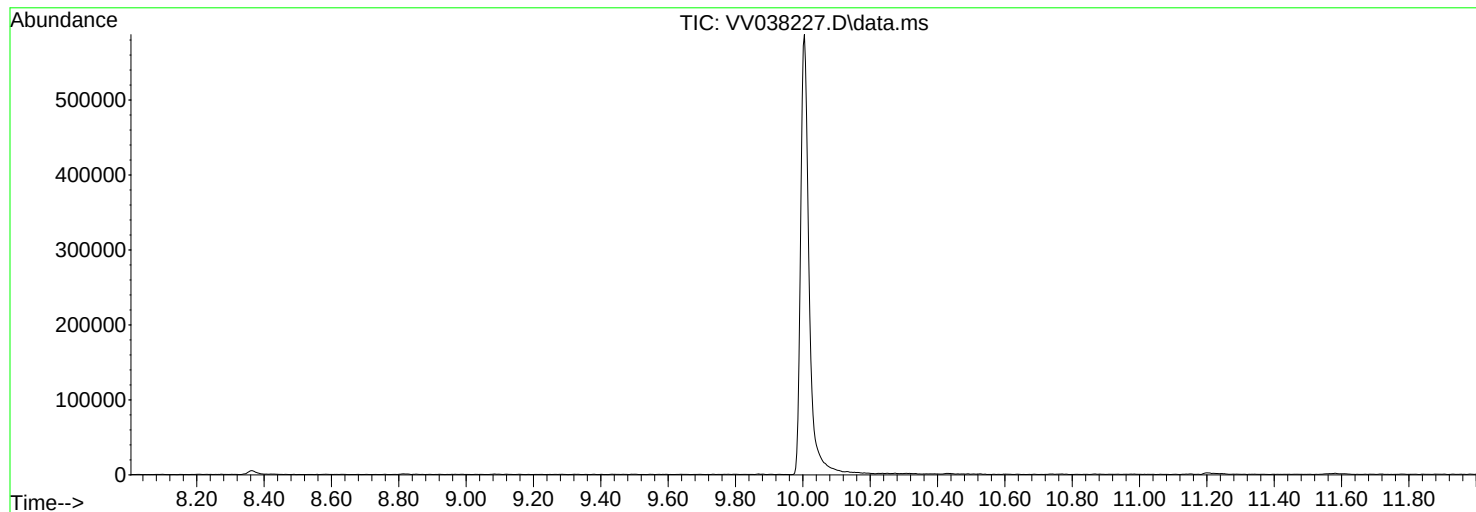

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	18640	PASS
75	95	30	80	47.3	56368	PASS
95	95	100	100	100.0	119243	PASS
96	95	5	9	6.4	7592	PASS
173	174	0.00	2	1.3	1280	PASS
174	95	50	120	81.8	97552	PASS
175	174	5	9	7.0	6814	PASS
176	174	95	105	96.3	93944	PASS
177	176	5	10	6.6	6192	PASS

m/z	Abundance
39.80	147.0
43.90	270.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

m/z	Abundance
36.00	823.0
37.00	4771.0
38.00	3762.0
39.00	1740.0
39.80	312.0
43.10	107.0
44.00	953.0
44.90	842.0
45.70	114.0
47.00	1176.0
48.00	790.0
49.00	4126.0
50.00	18752.0
51.00	5910.0
52.00	374.0
52.90	160.0
53.90	126.0
55.00	329.0
55.90	2031.0
57.00	2774.0
60.00	1045.0
61.00	5105.0
62.00	5328.0
63.00	5110.0
64.00	886.0
65.00	774.0
66.20	102.0
66.80	214.0
68.00	11064.0
69.00	11616.0
69.90	845.0
71.90	612.0
73.00	5284.0
74.00	19136.0
75.00	57360.0
76.00	4637.0
76.90	1007.0
78.00	562.0
78.90	5465.0
79.90	1276.0
80.90	4635.0
81.90	1011.0
82.90	126.0
85.70	118.0
86.00	109.0
86.90	5356.0
88.00	4863.0
90.80	348.0
92.00	3649.0
93.00	5410.0
94.00	13768.0
95.00	120576.0
96.00	7989.0
96.90	210.0
103.80	522.0
104.60	237.0
105.80	520.0
110.80	112.0
112.00	100.0
112.70	108.0
115.00	148.0
115.80	548.0
116.90	971.0
117.90	481.0
118.70	901.0
123.80	105.0
127.90	449.0
128.80	216.0
129.70	363.0
130.70	313.0
134.70	223.0
136.90	224.0
140.90	1329.0
141.70	131.0
143.00	1967.0
143.90	111.0
144.90	1156.0
145.70	200.0
146.70	103.0
148.00	198.0
148.80	128.0
150.00	118.0
153.70	135.0
154.90	281.0
156.80	146.0
158.70	107.0
160.80	141.0
170.90	359.0
171.90	1232.0
172.80	1278.0
174.00	95200.0
174.90	6741.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

175.90	92704.0
177.00	6233.0
178.00	349.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

m/z	Abundance
35.90	841.0
37.00	4767.0
38.00	3790.0
39.00	1728.0
39.80	334.0
42.90	150.0
44.00	921.0
44.90	791.0
45.80	200.0
47.00	1178.0
48.00	816.0
49.00	4038.0
50.00	19280.0
51.00	5853.0
52.10	314.0
52.90	205.0
53.80	157.0
55.00	354.0
55.90	2023.0
57.00	2859.0
58.10	166.0
60.00	980.0
61.00	5206.0
62.00	5409.0
63.00	5077.0
63.90	983.0
65.00	939.0
66.90	227.0
68.00	10820.0
69.00	11470.0
69.90	726.0
72.10	586.0
73.00	5580.0
74.00	19432.0
75.00	57600.0
76.00	4533.0
76.90	926.0
77.90	614.0
78.90	5443.0
79.90	1381.0
80.90	4727.0
81.90	1063.0
82.90	159.0
85.70	159.0
86.90	5341.0
88.00	5078.0
90.80	417.0
92.00	3750.0
93.00	5548.0
94.00	14151.0
95.00	123024.0
96.00	7760.0
97.00	224.0
103.80	584.0
104.60	211.0
105.90	572.0
107.00	165.0
108.00	104.0
110.80	102.0
113.00	111.0
115.00	139.0
115.80	544.0
116.90	975.0
117.90	493.0
118.80	890.0
123.80	128.0
127.90	506.0
128.80	206.0
129.70	468.0
130.70	199.0
134.70	231.0
136.90	204.0
140.80	1261.0
141.80	150.0
143.00	2103.0
143.90	110.0
144.90	1193.0
145.70	213.0
148.00	213.0
148.80	123.0
153.60	132.0
154.80	372.0
156.80	111.0
158.70	104.0
160.80	181.0
170.80	409.0
171.90	1271.0
172.80	1313.0
174.00	100712.0
175.00	7063.0
175.90	96616.0
177.00	6405.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

178.00

275.0

Instrument :

MSVOA_V

ClientSampleId :

BFB289

m/z	Abundance
35.90	845.0
37.00	4263.0
38.00	3541.0
39.00	1646.0
39.90	350.0
42.90	140.0
44.00	861.0
44.90	676.0
45.80	222.0
46.90	1162.0
48.00	637.0
49.00	3885.0
50.00	17888.0
51.00	5330.0
52.00	244.0
52.90	242.0
53.80	197.0
55.00	284.0
55.90	1751.0
57.00	2667.0
58.10	227.0
60.00	928.0
61.00	4987.0
62.00	5046.0
63.00	4605.0
63.90	937.0
65.00	987.0
66.90	225.0
68.00	9757.0
69.00	10424.0
70.00	561.0
72.10	578.0
73.00	5358.0
74.00	17816.0
75.00	54144.0
76.00	4173.0
76.90	772.0
77.90	576.0
78.90	4909.0
79.90	1372.0
80.90	4490.0
81.90	1042.0
83.00	177.0
85.70	158.0
86.90	4760.0
88.00	4512.0
90.80	449.0
92.00	3487.0
93.00	5101.0
94.00	12954.0
95.00	114128.0
96.00	7028.0
97.00	224.0
103.90	610.0
104.70	188.0
106.00	542.0
106.90	206.0
107.90	108.0
112.90	114.0
114.70	102.0
115.80	453.0
116.90	946.0
117.80	537.0
118.80	867.0
123.90	111.0
127.80	483.0
128.80	143.0
129.70	466.0
130.90	172.0
134.70	186.0
136.90	173.0
140.90	1194.0
141.90	156.0
143.00	2030.0
144.90	1086.0
145.80	232.0
148.00	185.0
154.80	380.0
160.80	170.0
170.80	438.0
171.80	1154.0
172.80	1250.0
174.00	96744.0
175.00	6639.0
175.90	92512.0
177.00	5938.0
178.00	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289