
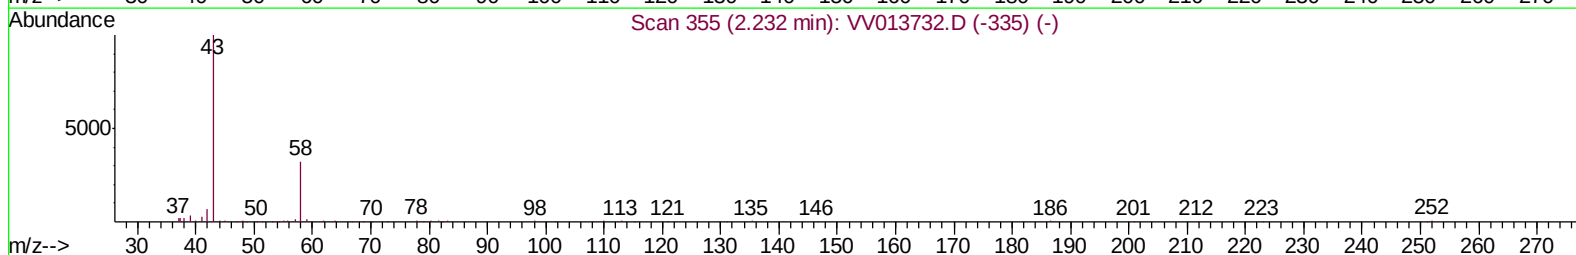
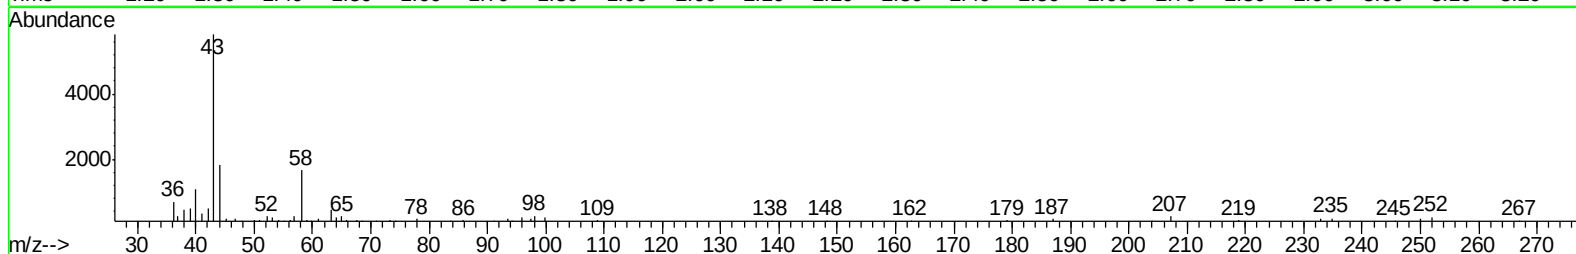


Data File : VV013749.D
Acq On : 22 Nov 2019 21:24
Operator : SY/MD
Sample : K5941-18DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Nov 23 01:41:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Nov 23 01:35:18 2019
Response via : Initial Calibration

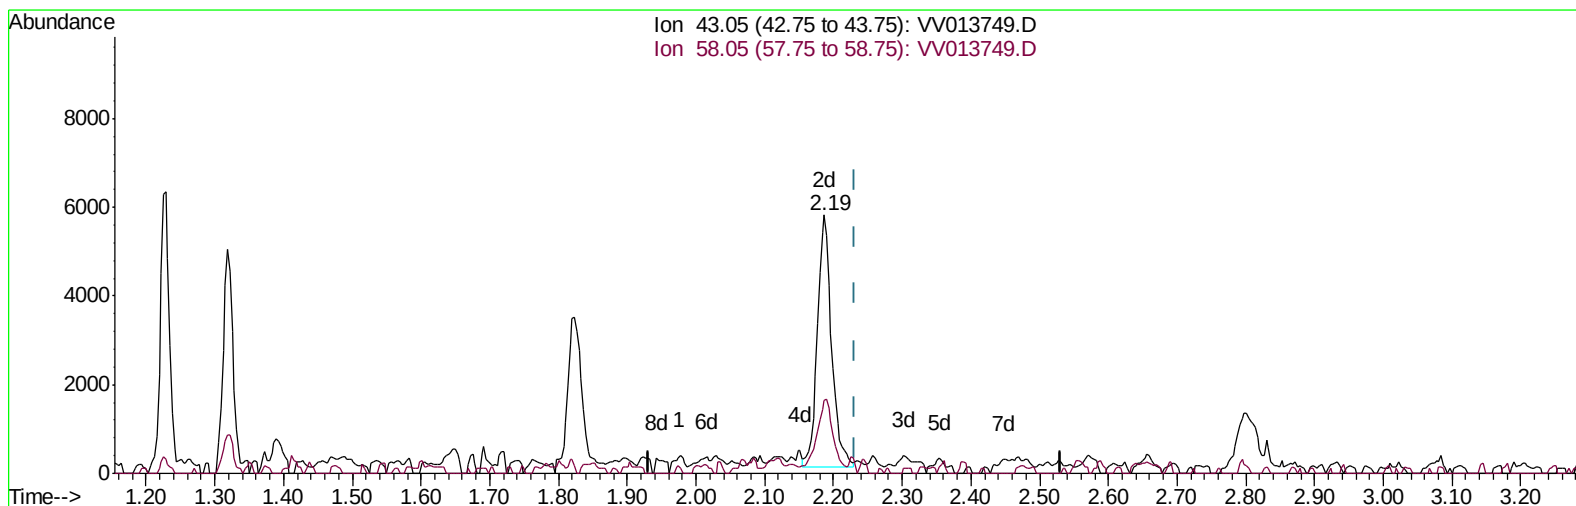

TIC: VV013749.D

(13) Acetone (T)

2.187min (-0.045) 2.79ug/L m

response 8110

Ion	Exp%	Act%
43.05	100	100
58.05	13.60	1.06
0.00	0.00	0.00
0.00	0.00	0.00