


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV112219\
 Data File : VV013724.D
 Acq On : 22 Nov 2019 08:26
 Operator : SY/MD
 Sample : BFB37
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB37

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Nov 26 04:36:55 2019

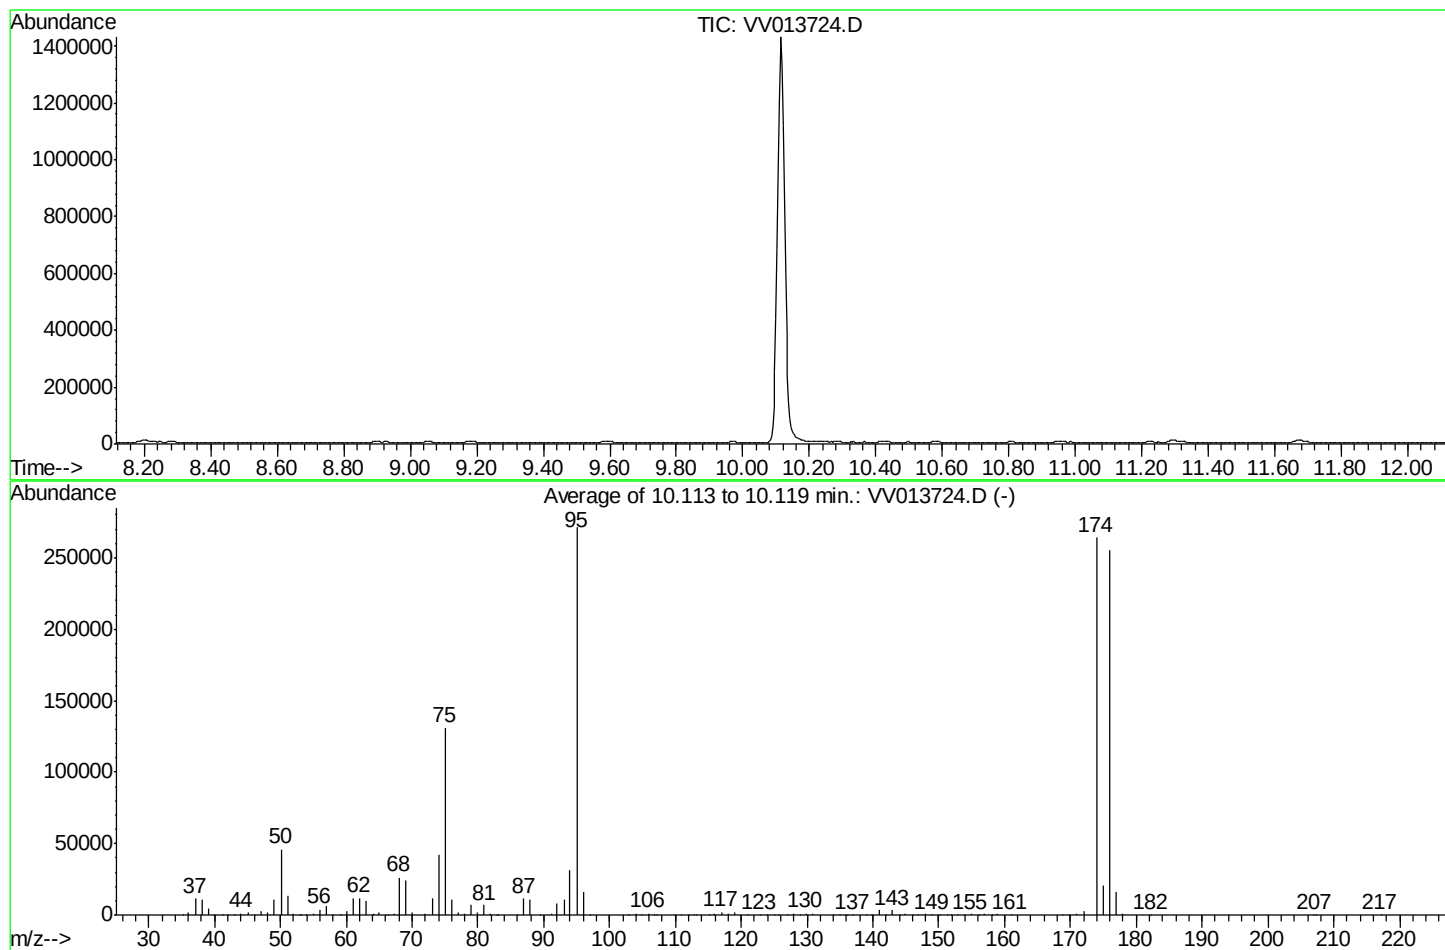

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	46000	PASS
75	95	30	80	48.4	131274	PASS
95	95	100	100	100.0	271338	PASS
96	95	5	9	6.1	16458	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	97.3	264021	PASS
175	174	5	9	7.7	20226	PASS
176	174	95	101	96.6	255018	PASS
177	176	5	9	6.5	16550	PASS

m/z	Abundance
35.10	145.0
36.10	2269.0
37.10	12002.0
38.10	11214.0
39.10	4077.0
39.90	1063.0
41.20	147.0
42.00	176.0
43.00	260.0
44.10	2017.0
45.10	2089.0
46.00	370.0
47.10	3373.0
48.00	1710.0
49.00	10700.0
50.10	47904.0
51.10	14638.0
52.00	572.0
52.90	297.0
53.90	218.0
55.00	802.0
56.00	3524.0
57.00	6446.0
58.00	323.0
59.00	109.0
60.00	2434.0
61.10	11910.0
62.00	12497.0
63.10	10378.0
64.10	1452.0
65.00	2001.0
66.20	243.0
67.20	950.0
68.00	26520.0
69.10	25640.0
70.10	2014.0
72.00	1222.0
73.10	12270.0
74.10	42960.0
75.10	135552.0
76.10	11583.0
77.00	1480.0
78.00	1478.0
79.00	7493.0
79.90	1780.0
80.90	7192.0
81.90	1490.0
82.80	178.0
85.90	509.0
87.00	12118.0
87.90	10663.0
89.50	107.0
91.10	938.0
92.00	8024.0
93.00	10957.0
94.00	31416.0
95.00	274240.0
96.10	16944.0
97.00	422.0
102.80	143.0
104.00	1013.0
104.80	415.0
105.90	1177.0
107.10	292.0
109.90	135.0
110.80	257.0
112.80	167.0
113.30	152.0
115.00	347.0
116.00	835.0
117.00	1958.0
117.90	1123.0
118.90	1651.0
122.80	183.0
123.90	154.0
124.90	117.0
125.70	133.0
126.90	166.0
127.90	918.0
128.90	373.0
129.80	1019.0
130.80	582.0
133.90	166.0
134.90	376.0
135.60	178.0
136.10	109.0
137.00	427.0
139.00	135.0
139.80	335.0
140.90	3098.0
141.90	495.0
142.90	3376.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

144.00	482.0
144.90	1282.0
146.10	531.0
146.80	326.0
147.90	778.0
149.00	173.0
150.00	310.0
151.30	110.0
151.90	225.0
152.90	324.0
153.80	258.0
155.00	743.0
156.20	158.0
157.00	728.0
158.90	486.0
160.90	311.0
168.80	194.0
169.80	114.0
170.90	519.0
172.00	3249.0
174.00	259840.0
175.00	20168.0
176.00	250304.0
177.00	17064.0
178.00	501.0
207.20	108.0
217.10	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
35.20	126.0
36.10	2222.0
37.10	11893.0
38.10	11038.0
39.10	4521.0
39.90	1188.0
41.30	172.0
42.00	190.0
43.10	211.0
44.00	1921.0
45.10	2121.0
46.00	325.0
47.00	3303.0
48.00	1537.0
49.10	10885.0
50.10	47400.0
51.10	14255.0
52.00	605.0
53.10	233.0
53.90	212.0
55.10	700.0
56.00	3745.0
57.00	6492.0
57.90	334.0
59.10	117.0
60.00	2421.0
61.00	12508.0
62.00	12575.0
63.10	10501.0
64.10	1322.0
65.00	1793.0
66.30	201.0
67.20	969.0
68.10	27392.0
69.00	25296.0
70.10	1939.0
72.00	1180.0
73.10	12628.0
74.10	44016.0
75.00	135808.0
76.10	11416.0
77.00	1586.0
78.00	1351.0
79.00	7174.0
79.90	1828.0
80.90	7359.0
81.90	1453.0
83.10	204.0
85.90	501.0
87.00	11919.0
87.90	11589.0
91.10	1003.0
92.00	8600.0
93.10	11200.0
94.00	32232.0
95.00	279552.0
96.10	16960.0
97.00	410.0
102.80	132.0
104.00	1111.0
104.90	464.0
105.90	1287.0
106.70	323.0
109.90	105.0
110.90	221.0
111.90	121.0
112.70	144.0
113.30	168.0
115.00	319.0
116.00	832.0
117.00	1873.0
118.00	1207.0
119.00	1669.0
122.80	179.0
123.90	162.0
125.00	136.0
125.70	191.0
126.90	146.0
127.80	923.0
128.90	401.0
129.80	1151.0
130.80	612.0
133.90	141.0
134.90	438.0
135.70	188.0
137.00	428.0
139.00	195.0
139.80	258.0
140.90	3341.0
141.90	408.0
143.00	3440.0
144.00	423.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

144.90	1392.0
146.10	459.0
146.90	312.0
147.90	804.0
148.90	185.0
150.00	251.0
151.90	181.0
152.90	414.0
153.80	178.0
155.00	694.0
156.20	145.0
156.90	645.0
158.90	606.0
161.00	310.0
168.80	122.0
170.90	524.0
172.00	3211.0
174.00	272896.0
175.00	20800.0
176.00	264064.0
177.00	17192.0
178.00	569.0
207.20	105.0
217.10	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
36.00	2081.0
37.10	10661.0
38.10	9991.0
39.10	4425.0
39.90	1173.0
41.30	240.0
42.00	153.0
43.10	239.0
44.00	1717.0
45.00	1874.0
47.00	3077.0
48.00	1271.0
49.10	9981.0
50.10	42696.0
51.10	12826.0
52.00	607.0
53.10	220.0
53.90	219.0
55.20	551.0
56.00	3517.0
57.00	5758.0
57.90	272.0
59.10	124.0
60.00	2153.0
61.00	11617.0
62.00	11294.0
63.00	9438.0
64.10	1053.0
65.00	1525.0
65.90	174.0
66.20	179.0
67.20	753.0
68.10	24672.0
69.00	22800.0
70.00	1931.0
72.00	1164.0
73.00	11419.0
74.10	40512.0
75.00	122464.0
76.00	10095.0
77.00	1459.0
78.10	1163.0
79.00	6253.0
80.00	1663.0
80.90	6843.0
82.00	1178.0
83.10	216.0
85.90	429.0
87.00	10727.0
87.90	11232.0
91.10	1024.0
92.00	7969.0
93.10	10392.0
94.00	29896.0
95.00	260224.0
96.10	15472.0
97.00	441.0
102.80	109.0
104.00	1046.0
104.90	450.0
105.90	1270.0
106.70	329.0
111.00	213.0
112.00	139.0
112.70	127.0
113.20	152.0
115.00	260.0
115.90	775.0
117.00	1734.0
118.00	1141.0
119.00	1622.0
120.90	112.0
122.90	190.0
123.70	170.0
124.90	137.0
125.70	228.0
127.80	798.0
129.00	397.0
129.80	1099.0
130.90	531.0
134.90	527.0
135.70	170.0
136.90	393.0
139.00	212.0
139.80	170.0
140.90	3268.0
141.90	350.0
142.90	3357.0
144.00	353.0
144.90	1354.0
146.10	400.0
146.80	300.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

147.90	683.0
148.90	227.0
150.10	208.0
151.90	183.0
152.90	398.0
153.90	159.0
154.80	682.0
156.00	135.0
156.90	586.0
158.10	121.0
158.90	559.0
161.00	318.0
170.90	519.0
172.00	2889.0
174.00	259328.0
175.00	19712.0
176.00	250688.0
177.00	15394.0
178.00	530.0
182.20	151.0
206.90	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
36.60	122.0
37.70	130.0
38.50	105.0
39.30	102.0
40.00	883.0
41.00	155.0
41.90	104.0
43.90	782.0
47.20	162.0
48.80	119.0
49.80	215.0
51.20	107.0
52.60	131.0
53.20	102.0
53.90	110.0
67.90	114.0
71.20	106.0
73.60	140.0
76.80	108.0
115.20	118.0
141.80	149.0
161.40	110.0
166.90	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37