

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112221\
 Data File : VW023659.D
 Acq On : 22 Nov 2021 14:09
 Operator : SY/MD
 Sample : VW1122WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 23 02:10:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM112221.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 23 02:04:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.615	114	11904	0.500	ug/L	-0.02
5) Chlorobenzene-d5	8.863	117	11451	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.244	152	5989	0.500	ug/L	-0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	5349	0.442	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	88.000%
4) 1,2-Dichloroethane-d4	5.042	65	4740	0.577	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	116.000%
7) 1,2-Dichloropropane-d6	6.068	67	5814	0.585	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	116.000%
8) Toluene-d8	7.317	98	14797	0.575	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	116.000%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	3494	0.578	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	116.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.409	75	11	0.012	ug/L	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112221\
Data File : VW023659.D
Acq On : 22 Nov 2021 14:09
Operator : SY/MD
Sample : VW1122WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 23 02:10:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM112221.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 23 02:04:29 2021
Response via : Initial Calibration

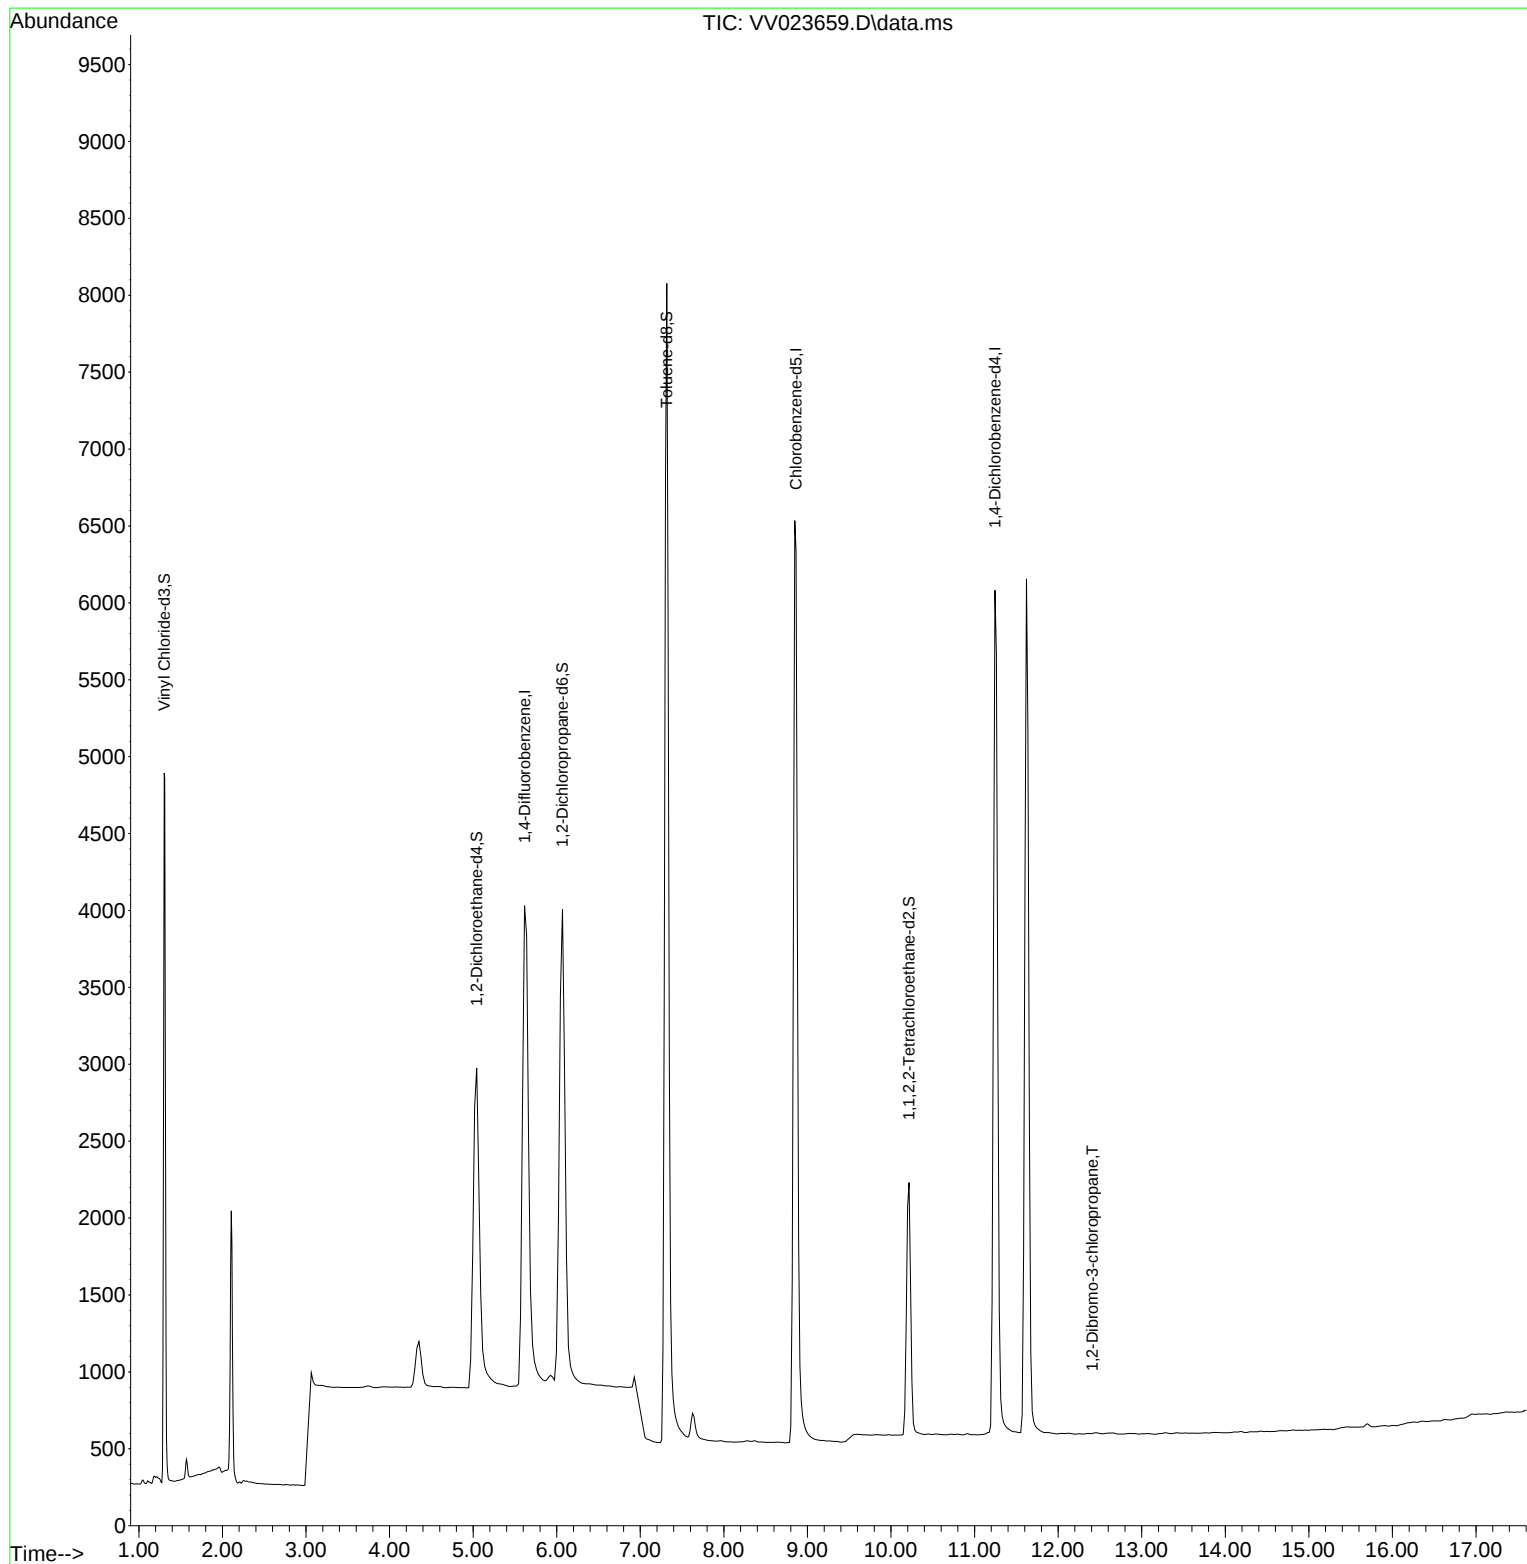

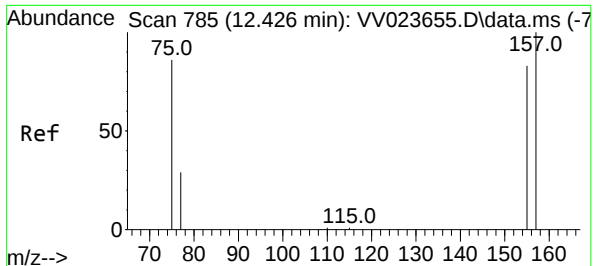

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.012 ug/L
 RT: 12.409 min Scan# 784
 Delta R.T. -0.017 min
 Lab File: VV023659.D
 Acq: 22 Nov 2021 14:09

Instrument :
 MSVOA_V
 ClientSampleId :

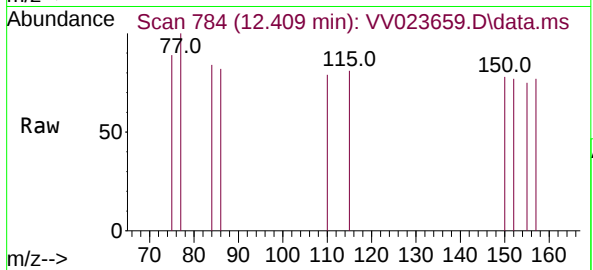

Tgt Ion: 75	Resp:	11	
Ion Ratio	Lower	Upper	
75 100			
157	86.2	85.7	128.5
155	84.6	74.3	111.5

