

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112223\
 Data File : VW033053.D
 Acq On : 22 Nov 2023 10:53
 Operator : SY/MD
 Sample : VW1122MBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 23 05:51:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 22 03:48:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	297070	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	299812	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	159919	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	59098	38.049	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.100%
7) Chloroethane-d5	1.532	69	49622	41.540	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	83.080%
11) 1,1-Dichloroethene-d2	2.060	65	26486	41.674	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.340%
21) 2-Butanone-d5	3.780	46	93137	94.246	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.250%
24) Chloroform-d	4.249	84	173330	45.281	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.560%
26) 1,2-Dichloroethane-d4	4.941	65	113213	47.413	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.820%
32) Benzene-d6	4.960	84	321035	45.981	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.960%
36) 1,2-Dichloropropane-d6	5.989	67	94241	47.600	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.200%
41) Toluene-d8	7.243	98	296687	44.515	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.020%
43) trans-1,3-Dichloroprop...	7.551	79	51204	44.301	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.600%
47) 2-Hexanone-d5	8.024	63	76594	93.490	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.490%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	130625	43.344	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.680%
66) 1,2-Dichlorobenzene-d4	11.561	152	143959	50.481	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.960%
Target Compounds						
39) cis-1,3-Dichloropropene	6.912	75	3571	1.013	ug/L	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033053.D
Acq On : 22 Nov 2023 10:53
Operator : SY/MD
Sample : VW1122MBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 23 05:51:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 22 03:48:12 2023
Response via : Initial Calibration

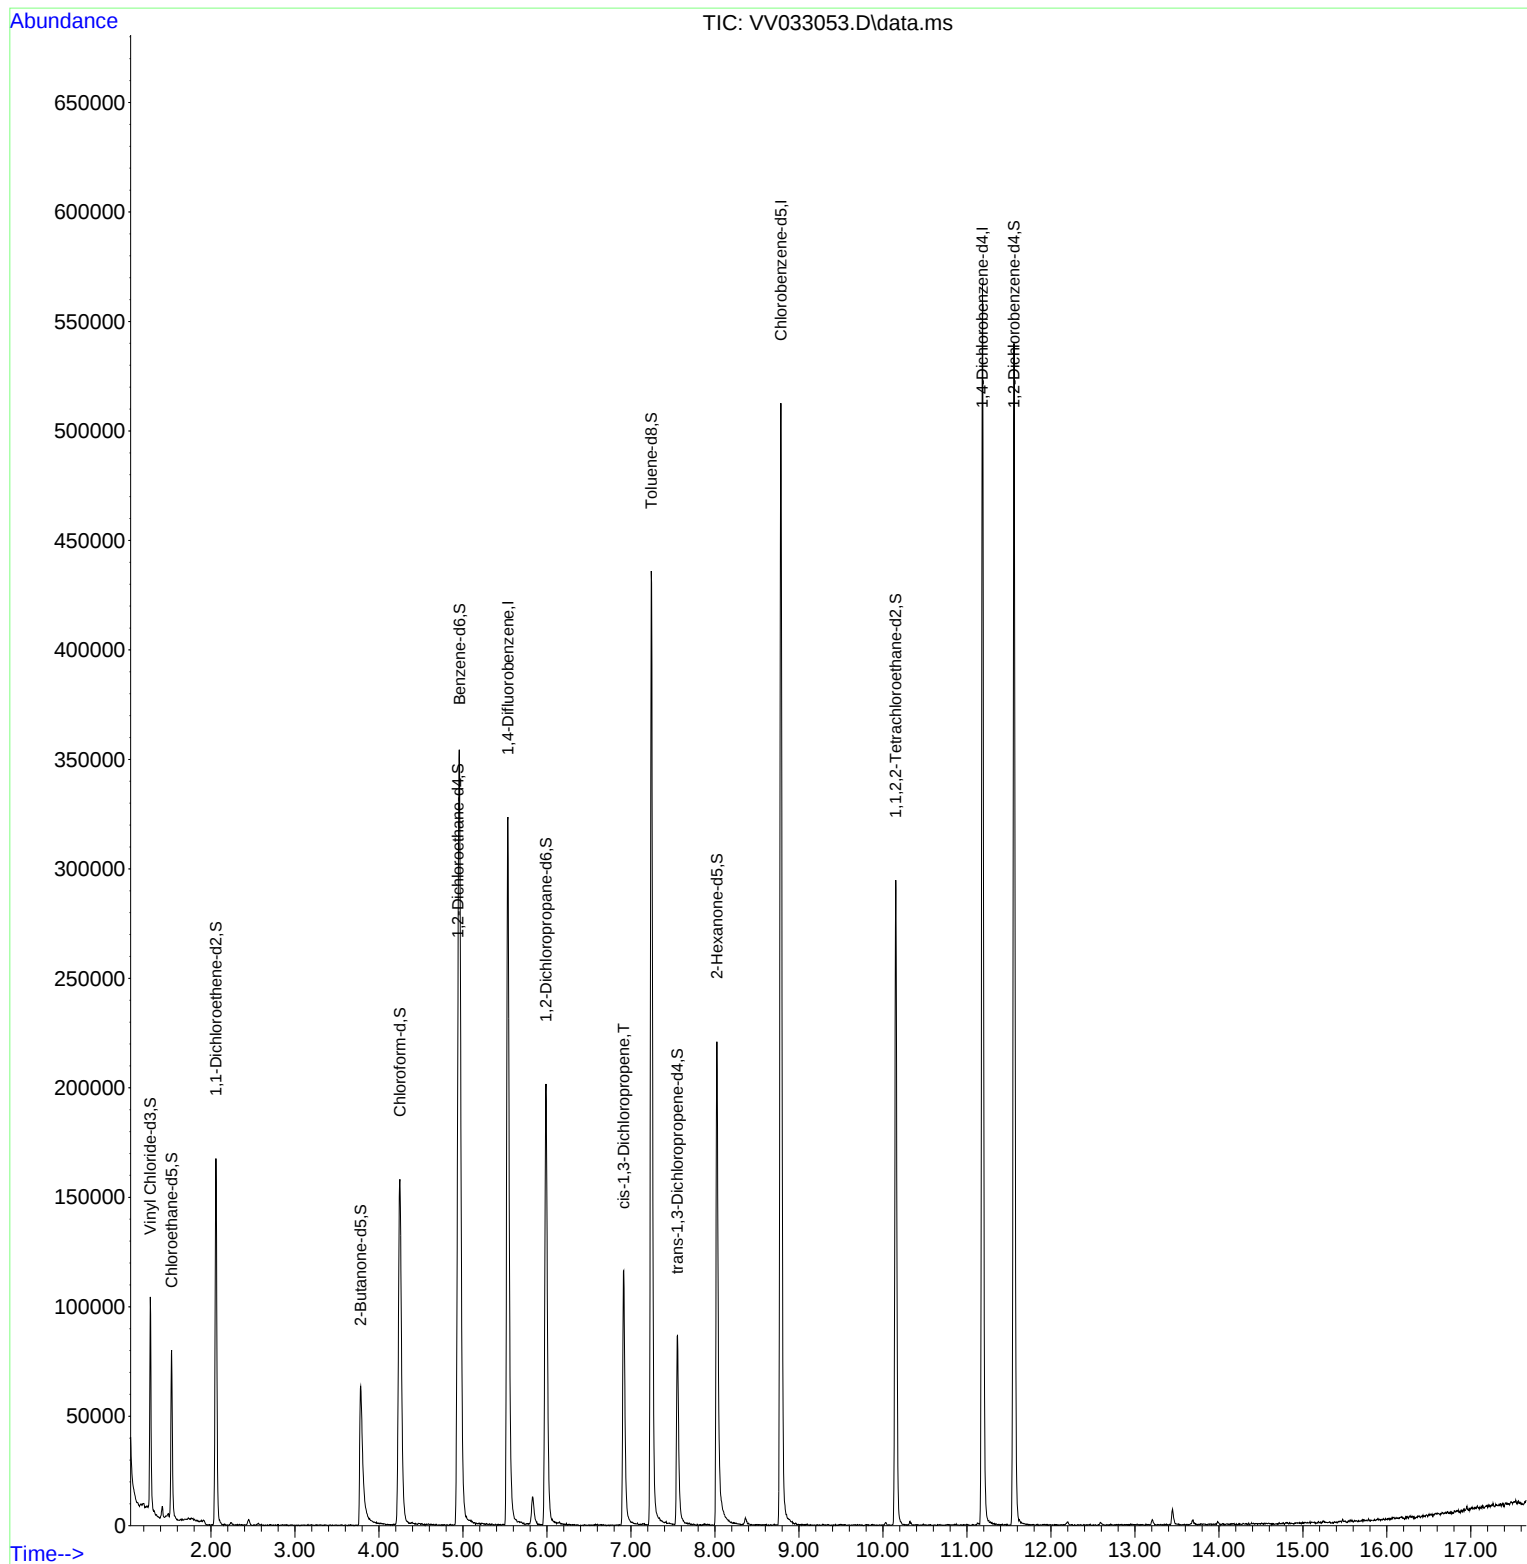

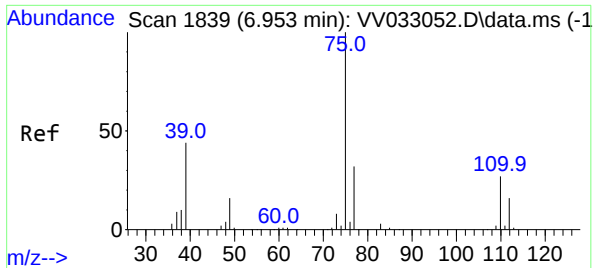

#39
 cis-1,3-Dichloropropene
 Concen: 1.013 ug/L
 RT: 6.912 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VV033053.D
 Acq: 22 Nov 2023 10:53

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion:	75	Resp:	3571
Ion Ratio	Lower	Upper	
75	100		
77	39.5	21.9	40.7

