

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
 Data File : VV033053.D
 Acq On : 22 Nov 2023 10:53
 Operator : SY/MD
 Sample : VV1122MBL01
 Misc : 5.00g/5mL/100uL/5.00ML/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rVB	97658	102807	10.95%	1.336%
2	1.532	146	153	173	rVB	77598	97821	10.42%	1.271%
3	1.966	286	288	293	rBV2	325	208	0.02%	0.003%
4	2.008	298	301	304	rBV2	218	162	0.02%	0.002%
5	2.060	306	317	329	rBV	167291	242274	25.81%	3.148%
6	2.233	365	371	372	rBV2	1069	747	0.08%	0.010%
7	2.339	402	404	408	rVB	339	185	0.02%	0.002%
8	2.394	419	421	423	rBV	354	226	0.02%	0.003%
9	2.449	431	438	449	rVB4	2592	4277	0.46%	0.056%
10	2.513	454	458	462	rBV2	393	298	0.03%	0.004%
11	2.699	513	516	518	rBV	378	260	0.03%	0.003%
12	2.915	582	583	586	rVB	376	166	0.02%	0.002%
13	2.944	587	592	593	rBV	385	301	0.03%	0.004%
14	2.995	604	608	611	rBV2	224	173	0.02%	0.002%
15	3.015	611	614	617	rVB	216	169	0.02%	0.002%
16	3.047	622	624	628	rVB	324	192	0.02%	0.002%
17	3.072	629	632	634	rBV	378	225	0.02%	0.003%
18	3.156	657	658	662	rVB	369	155	0.02%	0.002%
19	3.243	681	685	686	rBV	271	177	0.02%	0.002%
20	3.397	730	733	736	rBV2	161	163	0.02%	0.002%
21	3.416	737	739	745	rVB	347	296	0.03%	0.004%
22	3.600	791	796	799	rBV2	267	249	0.03%	0.003%
23	3.638	804	808	810	rBV	354	249	0.03%	0.003%
24	3.690	821	824	827	rVB	321	252	0.03%	0.003%
25	3.722	831	834	836	rBV	348	217	0.02%	0.003%
26	3.783	842	853	885	rBV	63445	170035	18.12%	2.210%
27	4.143	963	965	966	rBV	302	149	0.02%	0.002%
28	4.175	970	975	977	rBV2	553	481	0.05%	0.006%
29	4.191	977	980	981	rBV	403	229	0.02%	0.003%
30	4.249	983	998	1024	rVV	157313	402823	42.92%	5.235%
31	4.436	1054	1056	1063	rBV3	523	356	0.04%	0.005%
32	4.471	1063	1067	1068	rBV3	510	350	0.04%	0.005%
33	4.619	1111	1113	1117	rBV2	395	252	0.03%	0.003%
34	4.680	1129	1132	1137	rBV3	464	296	0.03%	0.004%
35	4.744	1148	1152	1154	rVB3	308	243	0.03%	0.003%
36	4.780	1160	1163	1169	rBV3	434	419	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
 Data File : VV033053.D
 Acq On : 22 Nov 2023 10:53
 Operator : SY/MD
 Sample : VV1122MBL01
 Misc : 5.00g/5mL/100uL/5.00ML/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	4.809	1170	1172	1176	rVB2	368	248	0.03%	0.003%
38	4.847	1180	1184	1189	rBV3	536	496	0.05%	0.006%
39	4.957	1201	1218	1243	rBV2	354035	938547	100.00%	12.197%
40	5.156	1278	1280	1284	rBV2	635	503	0.05%	0.007%
41	5.535	1386	1398	1429	rBV	323347	665645	70.92%	8.650%
42	5.989	1526	1539	1562	rBV	201399	421782	44.94%	5.481%
43	6.449	1678	1682	1685	rBV2	401	325	0.03%	0.004%
44	6.494	1693	1696	1700	rBV2	243	201	0.02%	0.003%
45	6.526	1702	1706	1708	rBV2	299	220	0.02%	0.003%
46	6.577	1720	1722	1725	rBV2	575	364	0.04%	0.005%
47	6.632	1732	1739	1741	rBV3	322	385	0.04%	0.005%
48	6.719	1763	1766	1767	rBV3	266	151	0.02%	0.002%
49	6.860	1808	1810	1812	rBV2	419	220	0.02%	0.003%
50	6.915	1816	1827	1852	rBV	116116	218836	23.32%	2.844%
51	7.243	1918	1929	1956	rBV	435649	771728	82.23%	10.029%
52	7.555	2016	2026	2053	rBV2	86221	155855	16.61%	2.025%
53	7.789	2096	2099	2101	rBV	589	288	0.03%	0.004%
54	7.857	2117	2120	2121	rBV	334	162	0.02%	0.002%
55	7.966	2149	2154	2155	rBV2	264	182	0.02%	0.002%
56	8.024	2161	2172	2214	rBV	220842	411980	43.90%	5.354%
57	8.612	2353	2355	2356	rBV2	422	162	0.02%	0.002%
58	8.786	2397	2409	2428	rBV	512337	847633	90.31%	11.015%
59	9.014	2478	2480	2481	rBV	388	195	0.02%	0.003%
60	9.088	2501	2503	2504	rBV	298	160	0.02%	0.002%
61	9.169	2525	2528	2531	rBV	258	207	0.02%	0.003%
62	9.217	2540	2543	2545	rBV	398	286	0.03%	0.004%
63	9.419	2603	2606	2608	rBV	266	197	0.02%	0.003%
64	9.481	2621	2625	2626	rBV2	394	222	0.02%	0.003%
65	9.632	2669	2672	2674	rBV	264	201	0.02%	0.003%
66	9.696	2689	2692	2695	rBV	430	294	0.03%	0.004%
67	9.796	2714	2723	2726	rBV3	575	705	0.08%	0.009%
68	10.034	2790	2797	2803	rBV5	1315	1848	0.20%	0.024%
69	10.153	2823	2834	2852	rBV	294436	470319	50.11%	6.112%
70	10.268	2868	2870	2874	rVB	284	206	0.02%	0.003%
71	10.416	2914	2916	2921	rBV	287	215	0.02%	0.003%
72	11.130	3133	3138	3141	rBV4	975	1006	0.11%	0.013%
73	11.185	3145	3155	3176	rBV	566703	891240	94.96%	11.582%
74	11.561	3260	3272	3290	rBV	539697	838164	89.30%	10.892%
75	11.828	3353	3355	3356	rBV	431	222	0.02%	0.003%
76	11.963	3395	3397	3399	rVB2	478	206	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
 Data File : VV033053.D
 Acq On : 22 Nov 2023 10:53
 Operator : SY/MD
 Sample : VV1122MBL01
 Misc : 5.00g/5mL/100uL/5.00ML/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	11.982	3399	3403	3404	rBV	331	242	0.03%	0.003%
78	12.056	3423	3426	3428	rBV2	335	209	0.02%	0.003%
79	12.098	3436	3439	3441	rBV2	280	174	0.02%	0.002%
80	12.281	3493	3496	3499	rBV2	318	168	0.02%	0.002%
81	12.316	3505	3507	3509	rBV	314	167	0.02%	0.002%
82	12.394	3528	3531	3533	rVB	468	288	0.03%	0.004%
83	12.468	3552	3554	3558	rVB	539	305	0.03%	0.004%
84	12.657	3610	3613	3616	rBV	371	232	0.02%	0.003%
85	12.680	3616	3620	3623	rVB	384	256	0.03%	0.003%
86	12.712	3627	3630	3634	rBV	603	525	0.06%	0.007%
87	12.779	3647	3651	3652	rBV	375	224	0.02%	0.003%
88	12.824	3661	3665	3666	rBV	252	181	0.02%	0.002%
89	13.066	3736	3740	3742	rBV	362	255	0.03%	0.003%
90	13.133	3758	3761	3762	rBV	563	223	0.02%	0.003%
91	13.207	3778	3784	3793	rVB7	2440	3683	0.39%	0.048%
92	13.358	3829	3831	3834	rBV	397	190	0.02%	0.002%
93	13.448	3851	3859	3869	rBV	7206	11424	1.22%	0.148%
94	13.693	3929	3935	3939	rVB5	1834	1978	0.21%	0.026%
95	13.985	4022	4026	4036	rVB5	1591	2331	0.25%	0.030%
96	14.146	4073	4076	4078	rBV2	620	363	0.04%	0.005%
97	14.207	4092	4095	4099	rBV2	573	328	0.03%	0.004%
98	14.355	4139	4141	4145	rVB4	852	500	0.05%	0.006%
99	14.377	4145	4148	4150	rBV3	539	422	0.04%	0.005%
100	14.844	4290	4293	4297	rBV2	721	574	0.06%	0.007%




Sum of corrected areas: 7694930

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033053.D
Acq On : 22 Nov 2023 10:53
Operator : SY/MD
Sample : VV1122MBL01
Misc : 5.00g/5mL/100uL/5.00ML/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

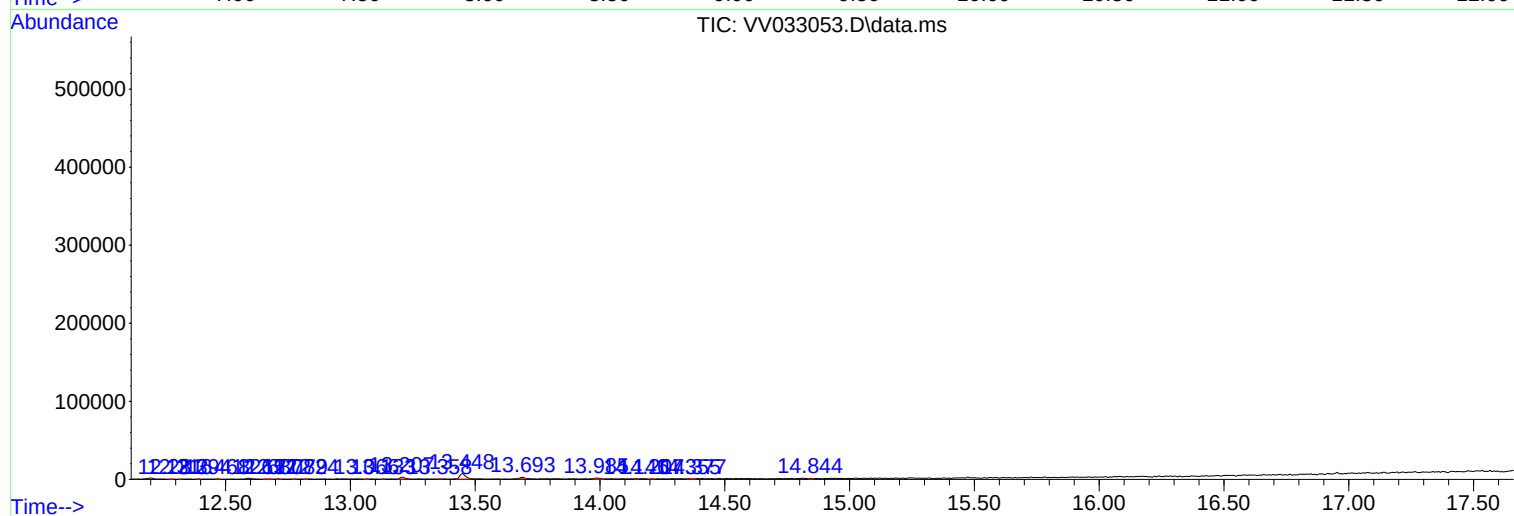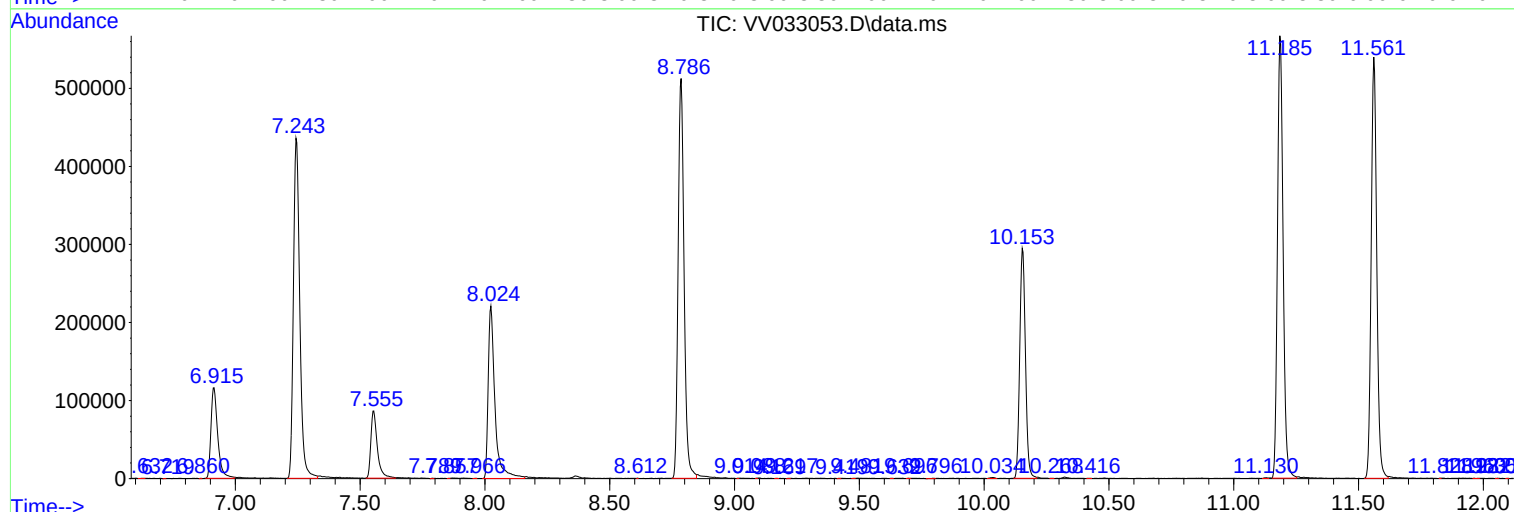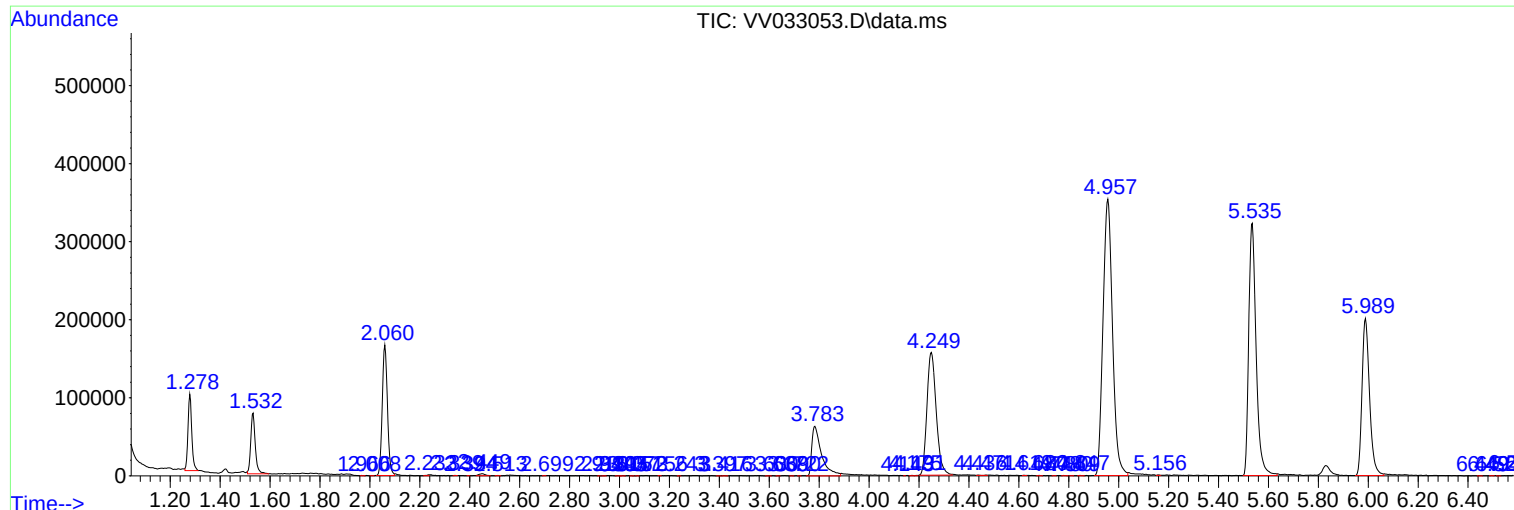

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033053.D
Acq On : 22 Nov 2023 10:53
Operator : SY/MD
Sample : VV1122MBL01
Misc : 5.00g/5mL/100uL/5.00ML/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033053.D
Acq On : 22 Nov 2023 10:53
Operator : SY/MD
Sample : VV1122MBL01
Misc : 5.00g/5mL/100uL/5.00ML/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK227

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------