

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
 Data File : VV033055.D
 Acq On : 22 Nov 2023 12:27
 Operator : SY/MD
 Sample : 05437-07ME
 Misc : 4.26G/5mL/100uL/5.00ML/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1E6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	84195	112313	9.97%	1.346%
2	1.963	285	287	289	rBV3	565	318	0.03%	0.004%
3	2.037	300	310	326	rVB	158959	230252	20.44%	2.759%
4	2.439	425	435	447	rVB5	5293	9633	0.86%	0.115%
5	2.555	458	471	484	rBV3	7548	17849	1.58%	0.214%
6	2.806	546	549	555	rVB2	280	247	0.02%	0.003%
7	3.072	628	632	633	rBV	404	267	0.02%	0.003%
8	3.185	664	667	672	rBV	332	316	0.03%	0.004%
9	3.243	683	685	690	rVB2	304	287	0.03%	0.003%
10	3.294	697	701	704	rBV	439	355	0.03%	0.004%
11	3.368	720	724	727	rBV2	239	231	0.02%	0.003%
12	3.410	734	737	738	rBV	326	166	0.01%	0.002%
13	3.436	743	745	749	rBV	230	181	0.02%	0.002%
14	3.458	749	752	757	rVB2	464	402	0.04%	0.005%
15	3.503	764	766	770	rBV	362	264	0.02%	0.003%
16	3.606	793	798	801	rVB4	610	453	0.04%	0.005%
17	3.629	802	805	806	rBV	296	189	0.02%	0.002%
18	3.709	826	830	834	rVB2	276	240	0.02%	0.003%
19	3.760	844	846	848	rBV2	340	163	0.01%	0.002%
20	3.796	848	857	888	rBV2	42170	150997	13.41%	1.810%
21	4.185	976	978	979	rBV	465	189	0.02%	0.002%
22	4.243	982	996	1022	rVV2	155587	414987	36.85%	4.973%
23	4.516	1077	1081	1083	rBV2	380	350	0.03%	0.004%
24	4.564	1092	1096	1098	rBV3	400	374	0.03%	0.004%
25	4.667	1125	1128	1131	rVV	417	265	0.02%	0.003%
26	4.686	1131	1134	1137	rVB	248	189	0.02%	0.002%
27	4.706	1137	1140	1143	rBV	188	171	0.02%	0.002%
28	4.815	1171	1174	1177	rVB2	379	214	0.02%	0.003%
29	4.950	1199	1216	1249	rBV2	374972	964103	85.60%	11.554%
30	5.185	1287	1289	1294	rVB3	563	238	0.02%	0.003%
31	5.227	1300	1302	1305	rBV2	814	406	0.04%	0.005%
32	5.256	1305	1311	1313	rBV3	646	597	0.05%	0.007%
33	5.368	1343	1346	1349	rBV2	344	232	0.02%	0.003%
34	5.423	1361	1363	1365	rBV2	376	181	0.02%	0.002%
35	5.477	1372	1380	1382	rBV3	468	579	0.05%	0.007%
36	5.529	1384	1396	1423	rBV	369527	796675	70.74%	9.548%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112223\
 Data File : VW033055.D
 Acq On : 22 Nov 2023 12:27
 Operator : SY/MD
 Sample : 05437-07ME
 Misc : 4.26G/5mL/100uL/5.00ML/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1E6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	5.828	1477	1489	1509	rBV4	44599	106190	9.43%	1.273%
38	5.985	1526	1538	1565	rBV	198366	427310	37.94%	5.121%
39	6.214	1607	1609	1612	rBV	469	190	0.02%	0.002%
40	6.313	1636	1640	1642	rBV2	425	293	0.03%	0.004%
41	6.387	1661	1663	1666	rBV2	286	169	0.02%	0.002%
42	6.558	1709	1716	1718	rBV4	417	525	0.05%	0.006%
43	6.571	1718	1720	1723	rVV2	288	159	0.01%	0.002%
44	6.664	1747	1749	1753	rBV2	462	343	0.03%	0.004%
45	6.683	1753	1755	1758	rVB2	305	160	0.01%	0.002%
46	6.735	1768	1771	1772	rBV	428	186	0.02%	0.002%
47	6.870	1809	1813	1816	rBV	393	304	0.03%	0.004%
48	6.911	1816	1826	1859	rVV	120508	240813	21.38%	2.886%
49	7.243	1917	1929	1957	rBV	414797	750945	66.68%	9.000%
50	7.519	2012	2015	2016	rBV	342	189	0.02%	0.002%
51	7.555	2016	2026	2058	rVV2	82780	168442	14.96%	2.019%
52	7.847	2113	2117	2119	rBV2	545	368	0.03%	0.004%
53	7.979	2156	2158	2163	rBV2	468	247	0.02%	0.003%
54	8.046	2166	2179	2205	rBV2	137765	397213	35.27%	4.760%
55	8.506	2318	2322	2325	rBV	504	449	0.04%	0.005%
56	8.619	2354	2357	2359	rBV	325	189	0.02%	0.002%
57	8.744	2392	2396	2397	rBV	320	239	0.02%	0.003%
58	8.786	2398	2409	2439	rVV	574708	1026495	91.14%	12.302%
59	9.255	2552	2555	2559	rBV2	175	173	0.02%	0.002%
60	9.336	2577	2580	2581	rBV2	449	187	0.02%	0.002%
61	9.371	2588	2591	2592	rBV	338	198	0.02%	0.002%
62	9.426	2606	2608	2613	rBV2	523	341	0.03%	0.004%
63	9.445	2613	2614	2618	rVV2	309	157	0.01%	0.002%
64	9.493	2625	2629	2632	rBV3	457	346	0.03%	0.004%
65	9.654	2676	2679	2680	rBV	390	216	0.02%	0.003%
66	9.690	2684	2690	2692	rBV2	361	280	0.02%	0.003%
67	9.706	2692	2695	2697	rBV	489	321	0.03%	0.004%
68	9.754	2707	2710	2713	rVB2	253	164	0.01%	0.002%
69	10.037	2795	2798	2802	rBV2	356	240	0.02%	0.003%
70	10.159	2824	2836	2857	rBV	277163	476057	42.27%	5.705%
71	10.416	2914	2916	2922	rVB2	506	355	0.03%	0.004%
72	10.509	2943	2945	2947	rVB2	284	160	0.01%	0.002%
73	10.529	2947	2951	2953	rBV2	542	443	0.04%	0.005%
74	10.616	2976	2978	2983	rVB2	244	160	0.01%	0.002%
75	10.654	2987	2990	2992	rBV	436	269	0.02%	0.003%
76	10.709	3001	3007	3012	rBV3	498	571	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
 Data File : VV033055.D
 Acq On : 22 Nov 2023 12:27
 Operator : SY/MD
 Sample : 05437-07ME
 Misc : 4.26G/5mL/100uL/5.00ML/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY1E6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	10.754	3018	3021	3022	rBV2	232	152	0.01%	0.002%
78	10.857	3051	3053	3056	rBV2	408	220	0.02%	0.003%
79	10.927	3072	3075	3077	rBV	437	167	0.01%	0.002%
80	10.966	3085	3087	3091	rBV2	460	203	0.02%	0.002%
81	11.008	3097	3100	3107	rBV2	314	294	0.03%	0.004%
82	11.111	3130	3132	3136	rBV	480	296	0.03%	0.004%
83	11.140	3136	3141	3145	rBV2	504	483	0.04%	0.006%
84	11.191	3145	3157	3179	rBV	718382	1126275	100.00%	13.498%
85	11.503	3251	3254	3255	rBV	423	204	0.02%	0.002%
86	11.564	3261	3273	3297	rBV	571411	903319	80.20%	10.826%
87	11.841	3357	3359	3361	rBV2	408	185	0.02%	0.002%
88	11.857	3361	3364	3367	rVB2	376	273	0.02%	0.003%
89	11.895	3374	3376	3379	rBV2	419	262	0.02%	0.003%
90	11.982	3400	3403	3406	rBV	368	245	0.02%	0.003%
91	12.078	3429	3433	3435	rBV	215	209	0.02%	0.003%
92	12.651	3608	3611	3613	rBV	271	189	0.02%	0.002%
93	12.718	3629	3632	3636	rBV3	515	365	0.03%	0.004%
94	12.815	3659	3662	3663	rBV2	571	293	0.03%	0.004%
95	12.950	3700	3704	3707	rBV3	585	466	0.04%	0.006%
96	13.165	3767	3771	3773	rBV2	337	257	0.02%	0.003%
97	13.213	3781	3786	3787	rBV2	1313	868	0.08%	0.010%
98	13.660	3924	3925	3926	rBV2	459	157	0.01%	0.002%
99	13.689	3929	3934	3936	rBV2	902	813	0.07%	0.010%
100	13.976	4020	4023	4029	rBV2	825	881	0.08%	0.011%




Sum of corrected areas: 8344005

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033055.D
Acq On : 22 Nov 2023 12:27
Operator : SY/MD
Sample : 05437-07ME
Misc : 4.26G/5mL/100uL/5.00ML/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1E6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

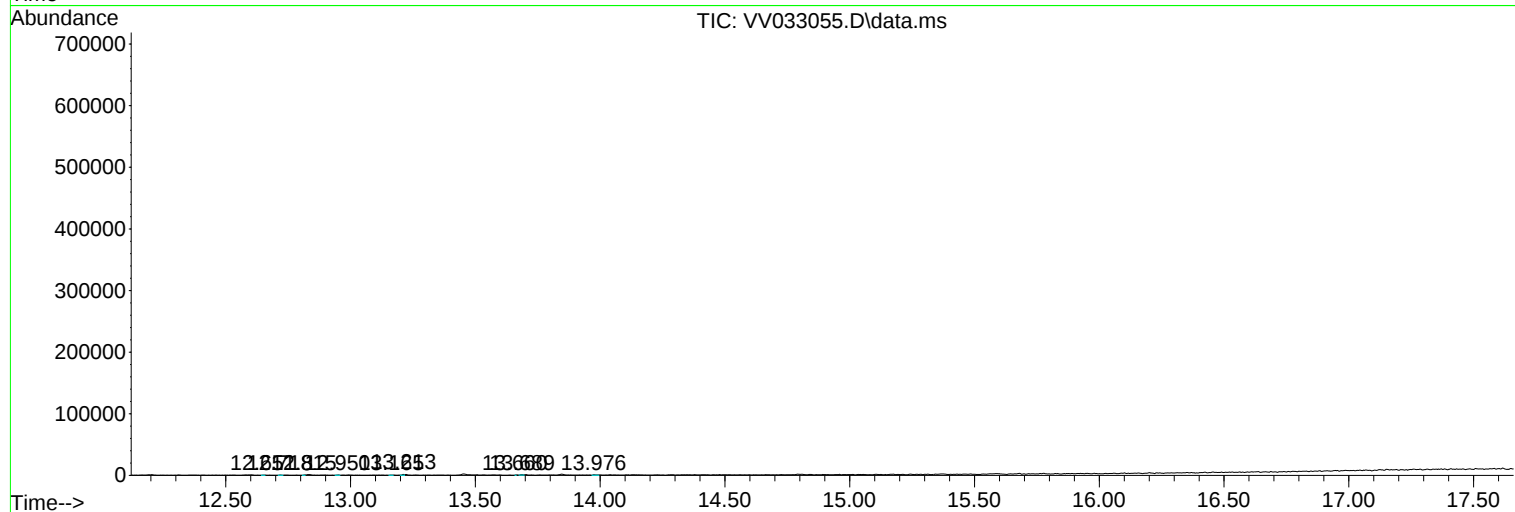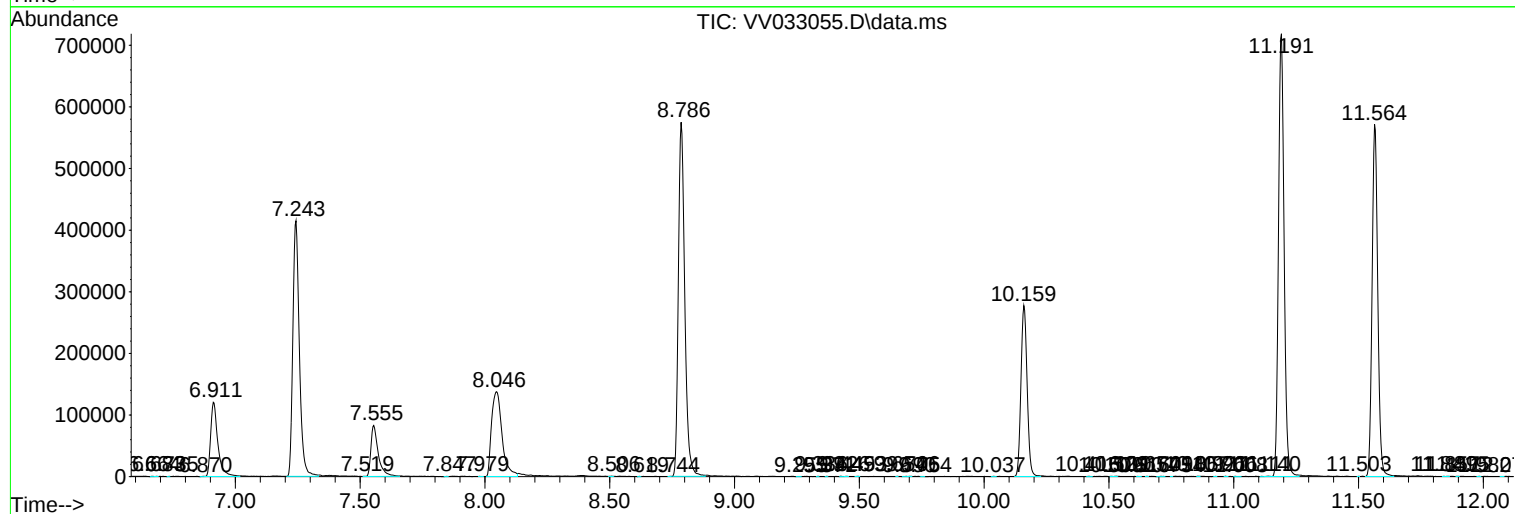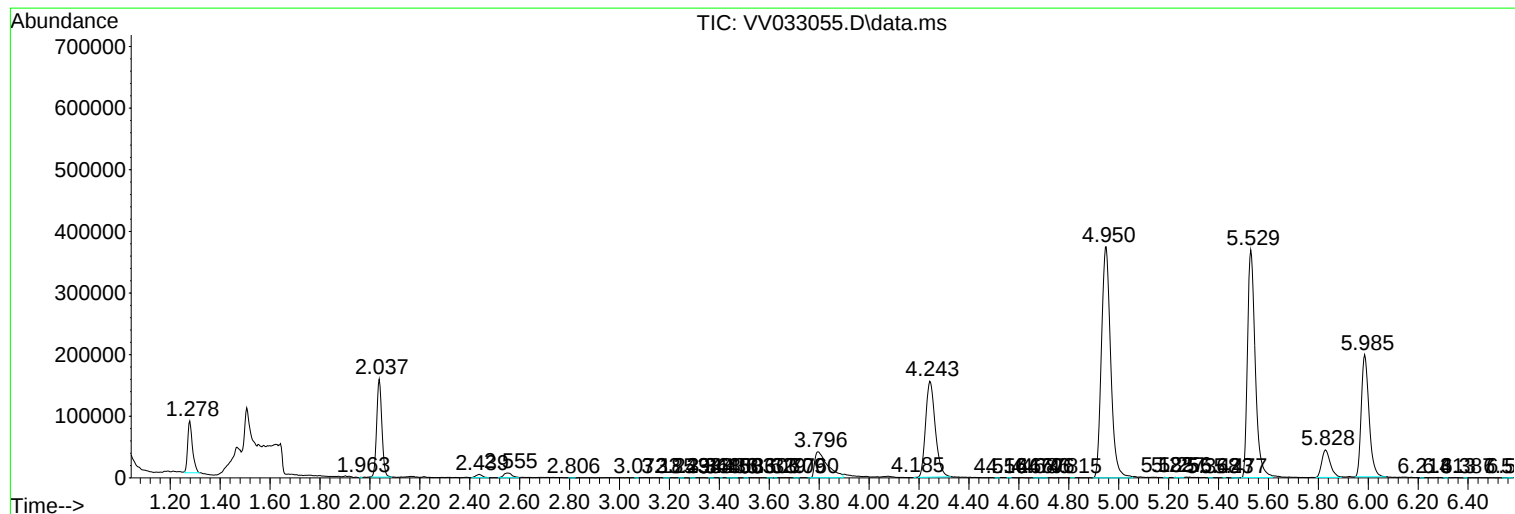

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033055.D
Acq On : 22 Nov 2023 12:27
Operator : SY/MD
Sample : 05437-07ME
Misc : 4.26G/5mL/100uL/5.00ML/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1E6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033055.D
Acq On : 22 Nov 2023 12:27
Operator : SY/MD
Sample : 05437-07ME
Misc : 4.26G/5mL/100uL/5.00ML/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY1E6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc