

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
 Data File : VV033059.D
 Acq On : 22 Nov 2023 14:57
 Operator : SY/MD
 Sample : VIBLK255
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK255

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M

Title : VOC Analysis

Signal : TIC: VV033059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	89	rVB	82946	88332	9.76%	1.169%
2	1.532	147	153	168	rVB	74435	87843	9.70%	1.162%
3	2.015	301	303	305	rBV	337	181	0.02%	0.002%
4	2.060	306	317	340	rVB	139915	206701	22.84%	2.735%
5	2.169	345	351	352	rBV3	904	786	0.09%	0.010%
6	2.355	407	409	411	rVB	520	176	0.02%	0.002%
7	2.394	417	421	422	rBV	540	354	0.04%	0.005%
8	2.449	430	438	449	rVB3	3334	5651	0.62%	0.075%
9	2.494	449	452	453	rBV2	439	272	0.03%	0.004%
10	2.545	466	468	469	rBV2	528	203	0.02%	0.003%
11	2.635	492	496	498	rBV	475	364	0.04%	0.005%
12	2.664	502	505	507	rVB2	348	195	0.02%	0.003%
13	2.693	507	514	516	rBV4	1323	1466	0.16%	0.019%
14	2.831	551	557	561	rBV	424	501	0.06%	0.007%
15	2.947	589	593	597	rVB2	231	225	0.02%	0.003%
16	2.982	601	604	610	rBV2	361	359	0.04%	0.005%
17	3.085	632	636	640	rBB2	653	452	0.05%	0.006%
18	3.111	640	644	646	rBB	256	151	0.02%	0.002%
19	3.143	650	654	659	rBV	439	409	0.05%	0.005%
20	3.230	676	681	683	rBB	196	182	0.02%	0.002%
21	3.252	683	688	691	rBB2	400	346	0.04%	0.005%
22	3.272	691	694	695	rBV	317	198	0.02%	0.003%
23	3.310	704	706	709	rBV	253	191	0.02%	0.003%
24	3.436	742	745	749	rBV2	201	167	0.02%	0.002%
25	3.458	749	752	753	rBV	247	169	0.02%	0.002%
26	3.503	763	766	767	rBV	313	171	0.02%	0.002%
27	3.523	770	772	777	rVB2	291	259	0.03%	0.003%
28	3.548	778	780	786	rBB	405	474	0.05%	0.006%
29	3.580	786	790	794	rBV	336	318	0.04%	0.004%
30	3.619	798	802	803	rBV2	370	240	0.03%	0.003%
31	3.690	820	824	826	rBV2	289	223	0.02%	0.003%
32	3.783	844	853	884	rBV2	60920	165182	18.25%	2.186%
33	4.249	983	998	1027	rBV	151846	389952	43.08%	5.160%
34	4.487	1070	1072	1075	rBV2	471	305	0.03%	0.004%
35	4.510	1075	1079	1082	rVV4	498	381	0.04%	0.005%
36	4.561	1093	1095	1097	rBV2	389	203	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112223\
 Data File : VW033059.D
 Acq On : 22 Nov 2023 14:57
 Operator : SY/MD
 Sample : VIBLK255
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK255

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	4.738	1147	1150	1151	rBV	504	294	0.03%	0.004%
38	4.831	1175	1179	1184	rBV	320	342	0.04%	0.005%
39	4.957	1201	1218	1247	rBV2	341157	905173	100.00%	11.976%
40	5.426	1362	1364	1369	rBV3	520	470	0.05%	0.006%
41	5.535	1386	1398	1422	rBV	323311	657561	72.64%	8.700%
42	5.831	1481	1490	1505	rVB8	10568	22278	2.46%	0.295%
43	5.931	1518	1521	1522	rBV3	479	240	0.03%	0.003%
44	5.989	1526	1539	1562	rBV	194179	401629	44.37%	5.314%
45	6.297	1629	1635	1637	rBV3	459	409	0.05%	0.005%
46	6.442	1677	1680	1682	rBV2	534	334	0.04%	0.004%
47	6.519	1700	1704	1710	rVB2	376	440	0.05%	0.006%
48	6.551	1711	1714	1719	rBV2	338	347	0.04%	0.005%
49	6.583	1719	1724	1727	rBV2	804	807	0.09%	0.011%
50	6.667	1748	1750	1754	rBV	599	389	0.04%	0.005%
51	6.857	1807	1809	1812	rBV	322	186	0.02%	0.002%
52	6.915	1816	1827	1852	rBV	114539	216767	23.95%	2.868%
53	7.204	1915	1917	1918	rBV2	502	220	0.02%	0.003%
54	7.246	1918	1930	1954	rVV	393343	699814	77.31%	9.259%
55	7.555	2016	2026	2048	rBV	84683	151891	16.78%	2.010%
56	7.744	2082	2085	2086	rVB	359	160	0.02%	0.002%
57	7.770	2086	2093	2098	rBV4	616	649	0.07%	0.009%
58	7.857	2118	2120	2121	rBV	404	158	0.02%	0.002%
59	7.870	2122	2124	2128	rVV	385	283	0.03%	0.004%
60	7.973	2151	2156	2159	rBV	300	301	0.03%	0.004%
61	8.024	2163	2172	2201	rBV	212584	388342	42.90%	5.138%
62	8.362	2269	2277	2280	rBV6	2654	3756	0.41%	0.050%
63	8.513	2321	2324	2326	rBV2	244	174	0.02%	0.002%
64	8.558	2337	2338	2340	rBV	499	176	0.02%	0.002%
65	8.577	2342	2344	2347	rVB	428	169	0.02%	0.002%
66	8.603	2349	2352	2355	rBV2	382	296	0.03%	0.004%
67	8.786	2398	2409	2440	rBV	527829	855339	94.49%	11.317%
68	9.374	2589	2592	2595	rBV	312	277	0.03%	0.004%
69	9.616	2664	2667	2669	rBV2	248	189	0.02%	0.003%
70	9.789	2717	2721	2725	rBV	219	226	0.02%	0.003%
71	9.818	2727	2730	2733	rVV2	309	202	0.02%	0.003%
72	10.021	2789	2793	2795	rBV2	291	207	0.02%	0.003%
73	10.152	2823	2834	2861	rBV	292140	471566	52.10%	6.239%
74	10.316	2882	2885	2886	rBV3	601	420	0.05%	0.006%
75	10.397	2909	2910	2917	rVB2	284	168	0.02%	0.002%
76	10.458	2925	2929	2930	rBV	231	159	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
 Data File : VV033059.D
 Acq On : 22 Nov 2023 14:57
 Operator : SY/MD
 Sample : VIBLK255
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK255

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	10.480	2931	2936	2942	rBV4	1810	2241	0.25%	0.030%
78	10.532	2949	2952	2954	rBV2	359	260	0.03%	0.003%
79	10.664	2989	2993	2998	rBV2	520	433	0.05%	0.006%
80	10.792	3030	3033	3036	rBV2	339	239	0.03%	0.003%
81	10.860	3048	3054	3065	rVB4	2056	2880	0.32%	0.038%
82	11.095	3121	3127	3130	rBV2	241	295	0.03%	0.004%
83	11.130	3130	3138	3145	rBV2	3687	5882	0.65%	0.078%
84	11.185	3145	3155	3185	rVV	574649	905107	99.99%	11.976%
85	11.471	3241	3244	3248	rBV	269	221	0.02%	0.003%
86	11.561	3261	3272	3292	rBV	498976	795888	87.93%	10.530%
87	12.342	3512	3515	3518	rBV2	280	179	0.02%	0.002%
88	12.371	3518	3524	3527	rBV4	1525	1610	0.18%	0.021%
89	12.590	3582	3592	3603	rBV3	6612	10776	1.19%	0.143%
90	12.770	3643	3648	3651	rBV3	369	356	0.04%	0.005%
91	13.027	3725	3728	3733	rVB2	519	407	0.04%	0.005%
92	13.056	3733	3737	3739	rBV3	535	395	0.04%	0.005%
93	13.207	3774	3784	3795	rBV2	11161	18043	1.99%	0.239%
94	13.400	3842	3844	3847	rBV3	300	197	0.02%	0.003%
95	13.445	3850	3858	3869	rBV	31092	49476	5.47%	0.655%
96	13.631	3914	3916	3918	rBV	280	185	0.02%	0.002%
97	13.686	3924	3933	3945	rBV3	16071	25250	2.79%	0.334%
98	13.799	3964	3968	3969	rBV	716	451	0.05%	0.006%
99	13.834	3976	3979	3982	rBV2	497	397	0.04%	0.005%
100	14.512	4188	4190	4192	rBV2	583	381	0.04%	0.005%




Sum of corrected areas: 7557939

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033059.D
Acq On : 22 Nov 2023 14:57
Operator : SY/MD
Sample : VIBLK255
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK255

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

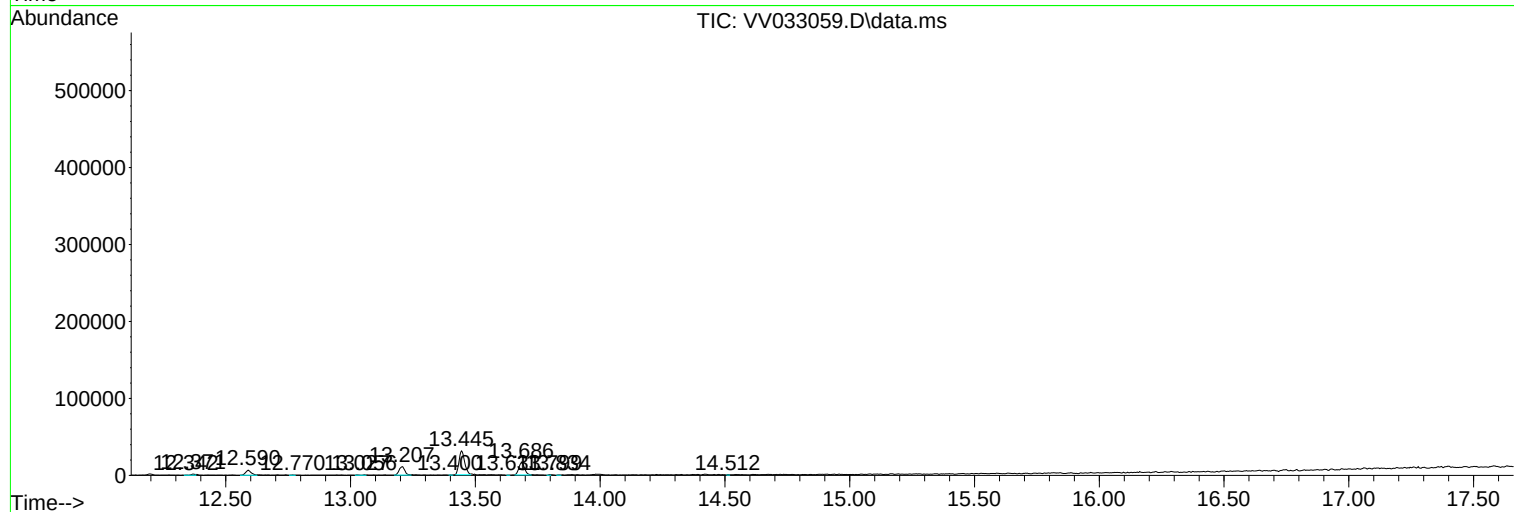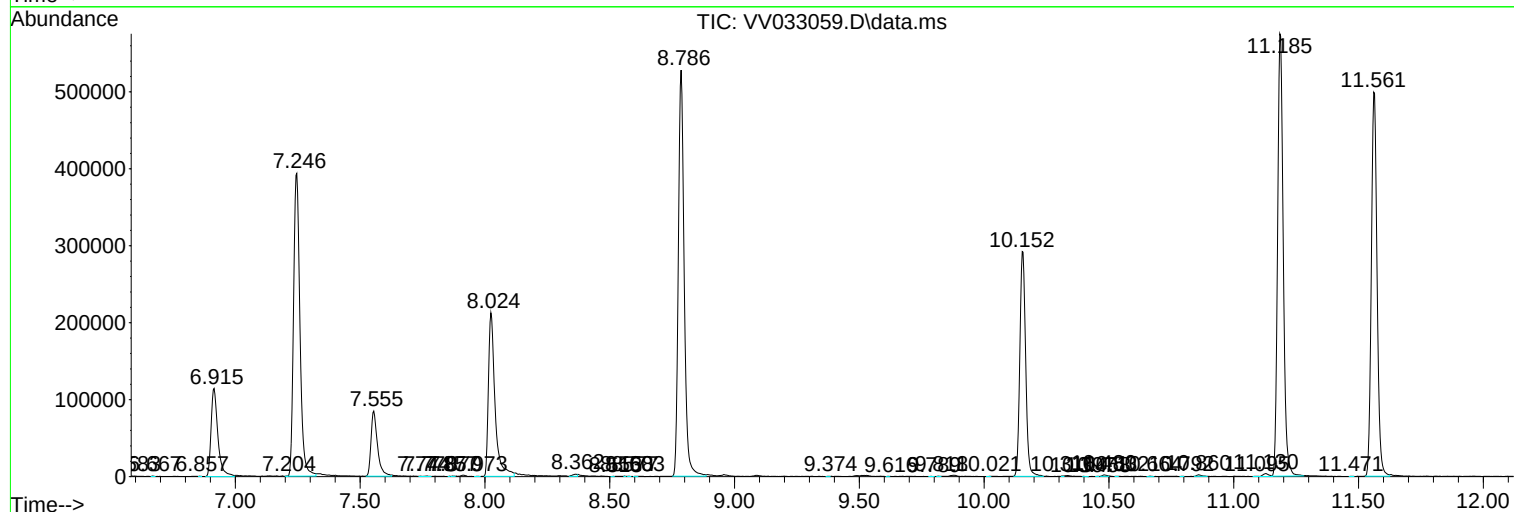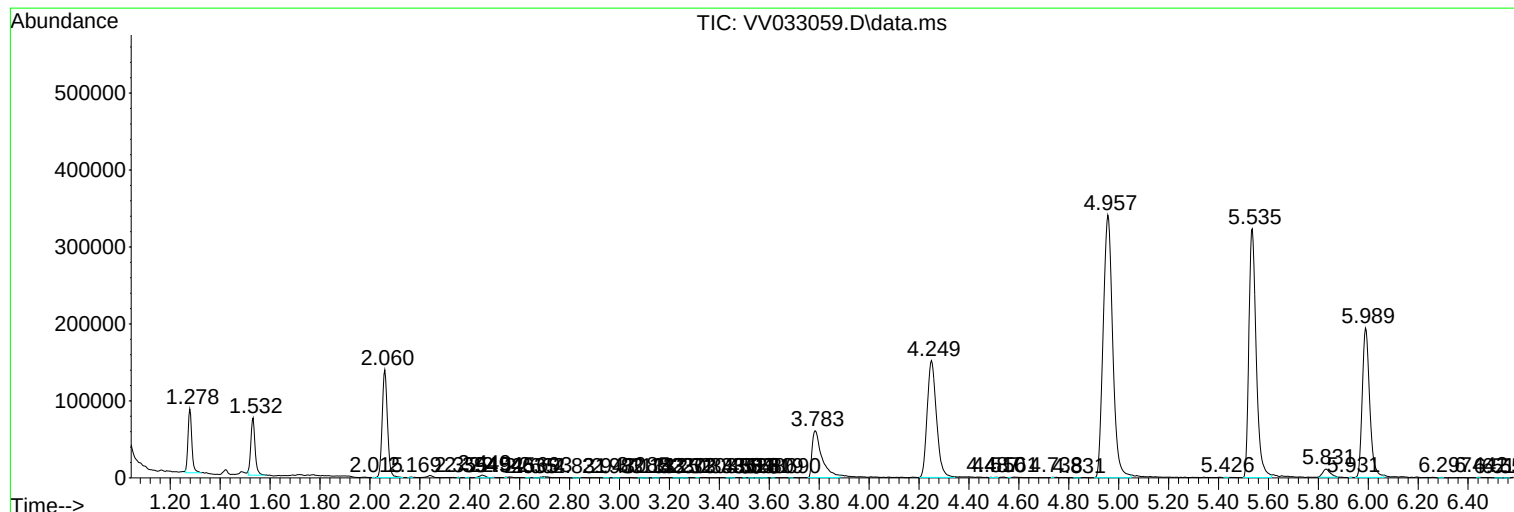

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033059.D
Acq On : 22 Nov 2023 14:57
Operator : SY/MD
Sample : VIBLK255
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK255

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033059.D
Acq On : 22 Nov 2023 14:57
Operator : SY/MD
Sample : VIBLK255
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK255

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------