

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
 Data File : VV033060.D
 Acq On : 22 Nov 2023 15:29
 Operator : SY/MD
 Sample : VIBLK256
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

Signal : TIC: VV033060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	104353	107927	10.47%	1.366%
2	1.532	146	153	168	rVB	80853	94407	9.16%	1.195%
3	2.015	300	303	306	rBV2	338	240	0.02%	0.003%
4	2.060	306	317	338	rVV	156685	229726	22.29%	2.907%
5	2.236	367	372	378	rBV3	1718	2328	0.23%	0.029%
6	2.317	393	397	398	rBV2	364	232	0.02%	0.003%
7	2.343	403	405	407	rVV3	559	259	0.03%	0.003%
8	2.449	432	438	448	rBV6	2138	3194	0.31%	0.040%
9	2.529	459	463	465	rBV	413	346	0.03%	0.004%
10	2.545	465	468	470	rBV3	576	400	0.04%	0.005%
11	2.699	512	516	518	rVV3	739	552	0.05%	0.007%
12	2.725	522	524	527	rVB	386	187	0.02%	0.002%
13	2.789	542	544	546	rBV	391	208	0.02%	0.003%
14	2.950	590	594	597	rVB	228	171	0.02%	0.002%
15	3.040	618	622	625	rVB2	302	221	0.02%	0.003%
16	3.156	649	658	659	rBV	450	534	0.05%	0.007%
17	3.204	668	673	676	rBV2	312	347	0.03%	0.004%
18	3.224	676	679	681	rBV2	224	169	0.02%	0.002%
19	3.288	697	699	704	rBV2	267	225	0.02%	0.003%
20	3.317	706	708	713	rVB2	355	265	0.03%	0.003%
21	3.548	778	780	783	rVB2	299	177	0.02%	0.002%
22	3.568	783	786	787	rBV	366	193	0.02%	0.002%
23	3.577	787	789	792	rVB2	362	188	0.02%	0.002%
24	3.609	797	799	801	rBV2	271	169	0.02%	0.002%
25	3.687	818	823	825	rBV3	425	412	0.04%	0.005%
26	3.780	843	852	886	rBV	61159	167088	16.22%	2.115%
27	4.249	983	998	1021	rBV	154809	394089	38.25%	4.988%
28	4.606	1106	1109	1115	rVB3	635	539	0.05%	0.007%
29	4.677	1128	1131	1134	rBV2	210	187	0.02%	0.002%
30	4.703	1137	1139	1142	rVB	607	248	0.02%	0.003%
31	4.751	1151	1154	1158	rVB	319	225	0.02%	0.003%
32	4.822	1173	1176	1178	rVV	422	246	0.02%	0.003%
33	4.851	1182	1185	1189	rBV2	393	293	0.03%	0.004%
34	4.892	1192	1198	1200	rBV2	314	271	0.03%	0.003%
35	4.953	1201	1217	1247	rBV2	337763	911641	88.47%	11.538%
36	5.294	1322	1323	1327	rVB3	621	406	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112223\
 Data File : VW033060.D
 Acq On : 22 Nov 2023 15:29
 Operator : SY/MD
 Sample : VIBLK256
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

37	5.391	1351	1353	1359	rVB2	468	258	0.03%	0.003%
38	5.416	1359	1361	1362	rBV	406	197	0.02%	0.002%
39	5.532	1386	1397	1424	rBV	366772	746979	72.49%	9.454%
40	5.828	1477	1489	1508	rVB4	14393	32477	3.15%	0.411%
41	5.937	1520	1523	1524	rBV2	391	227	0.02%	0.003%
42	5.989	1526	1539	1567	rVV2	197874	410601	39.85%	5.197%
43	6.281	1628	1630	1633	rBV2	414	217	0.02%	0.003%
44	6.304	1635	1637	1641	rVB2	419	196	0.02%	0.002%
45	6.368	1652	1657	1659	rBV2	529	496	0.05%	0.006%
46	6.500	1695	1698	1700	rBV2	260	194	0.02%	0.002%
47	6.584	1721	1724	1725	rBV2	403	198	0.02%	0.003%
48	6.654	1744	1746	1750	rVB2	463	275	0.03%	0.003%
49	6.686	1750	1756	1760	rBV3	644	764	0.07%	0.010%
50	6.912	1815	1826	1852	rBV	114944	215769	20.94%	2.731%
51	7.133	1891	1895	1899	rBV3	766	620	0.06%	0.008%
52	7.243	1918	1929	1948	rBV	401954	695422	67.49%	8.801%
53	7.513	2010	2013	2016	rBV2	472	357	0.03%	0.005%
54	7.555	2016	2026	2048	rBV	84287	153080	14.86%	1.937%
55	7.866	2120	2123	2126	rBV2	434	323	0.03%	0.004%
56	8.024	2162	2172	2201	rBV	211932	393551	38.19%	4.981%
57	8.535	2328	2331	2333	rBV2	373	173	0.02%	0.002%
58	8.625	2357	2359	2362	rBV	380	250	0.02%	0.003%
59	8.786	2397	2409	2443	rBV	575420	953387	92.53%	12.066%
60	9.339	2579	2581	2584	rVB	359	179	0.02%	0.002%
61	9.374	2588	2592	2593	rBV	294	195	0.02%	0.002%
62	9.397	2596	2599	2601	rBV2	351	254	0.02%	0.003%
63	9.577	2653	2655	2657	rBV	302	189	0.02%	0.002%
64	9.863	2740	2744	2745	rBV2	589	339	0.03%	0.004%
65	9.905	2754	2757	2759	rBV	377	203	0.02%	0.003%
66	10.005	2784	2788	2789	rBV	314	203	0.02%	0.003%
67	10.053	2800	2803	2808	rBV	350	274	0.03%	0.003%
68	10.153	2823	2834	2856	rBV	291916	466231	45.25%	5.901%
69	10.268	2868	2870	2873	rBV2	581	320	0.03%	0.004%
70	10.336	2888	2891	2893	rBV	452	274	0.03%	0.003%
71	10.400	2908	2911	2913	rVB2	365	188	0.02%	0.002%
72	10.690	2999	3001	3006	rVB	514	368	0.04%	0.005%
73	10.786	3027	3031	3034	rVB2	410	327	0.03%	0.004%
74	10.850	3048	3051	3052	rBV	315	183	0.02%	0.002%
75	11.188	3144	3156	3180	rBV	667235	1030395	100.00%	13.041%
76	11.439	3231	3234	3236	rBV2	525	296	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
 Data File : VV033060.D
 Acq On : 22 Nov 2023 15:29
 Operator : SY/MD
 Sample : VIBLK256
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
 Title : VOC Analysis

77	11.561	3261	3272	3294	rBV	532468	845144	82.02%	10.696%
78	12.053	3422	3425	3427	rBV2	288	194	0.02%	0.002%
79	12.172	3458	3462	3463	rBV2	389	261	0.03%	0.003%
80	12.268	3491	3492	3498	rVB2	265	172	0.02%	0.002%
81	12.300	3498	3502	3504	rBV	285	256	0.02%	0.003%
82	12.406	3532	3535	3538	rBV	386	273	0.03%	0.003%
83	12.516	3567	3569	3572	rVB	425	176	0.02%	0.002%
84	12.593	3587	3593	3601	rVV4	1664	2611	0.25%	0.033%
85	12.657	3611	3613	3616	rBV2	332	222	0.02%	0.003%
86	12.841	3666	3670	3673	rBV2	248	244	0.02%	0.003%
87	12.895	3685	3687	3691	rVB2	502	347	0.03%	0.004%
88	12.969	3709	3710	3714	rVB	375	206	0.02%	0.003%
89	12.988	3714	3716	3718	rBV2	326	168	0.02%	0.002%
90	13.053	3732	3736	3738	rBV2	458	379	0.04%	0.005%
91	13.207	3778	3784	3793	rBV4	3524	4906	0.48%	0.062%
92	13.281	3805	3807	3809	rBV	391	218	0.02%	0.003%
93	13.355	3828	3830	3834	rVB2	466	253	0.02%	0.003%
94	13.448	3852	3859	3871	rBB	7781	12434	1.21%	0.157%
95	13.529	3881	3884	3886	rBV2	597	369	0.04%	0.005%
96	13.564	3892	3895	3898	rBV2	579	425	0.04%	0.005%
97	13.686	3926	3933	3948	rVB8	3876	6615	0.64%	0.084%
98	13.837	3979	3980	3983	rBV2	278	162	0.02%	0.002%
99	13.914	4001	4004	4005	rBV2	405	175	0.02%	0.002%
100	14.204	4091	4094	4096	rBV3	350	257	0.02%	0.003%




Sum of corrected areas: 7901206

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033060.D
Acq On : 22 Nov 2023 15:29
Operator : SY/MD
Sample : VIBLK256
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK256

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

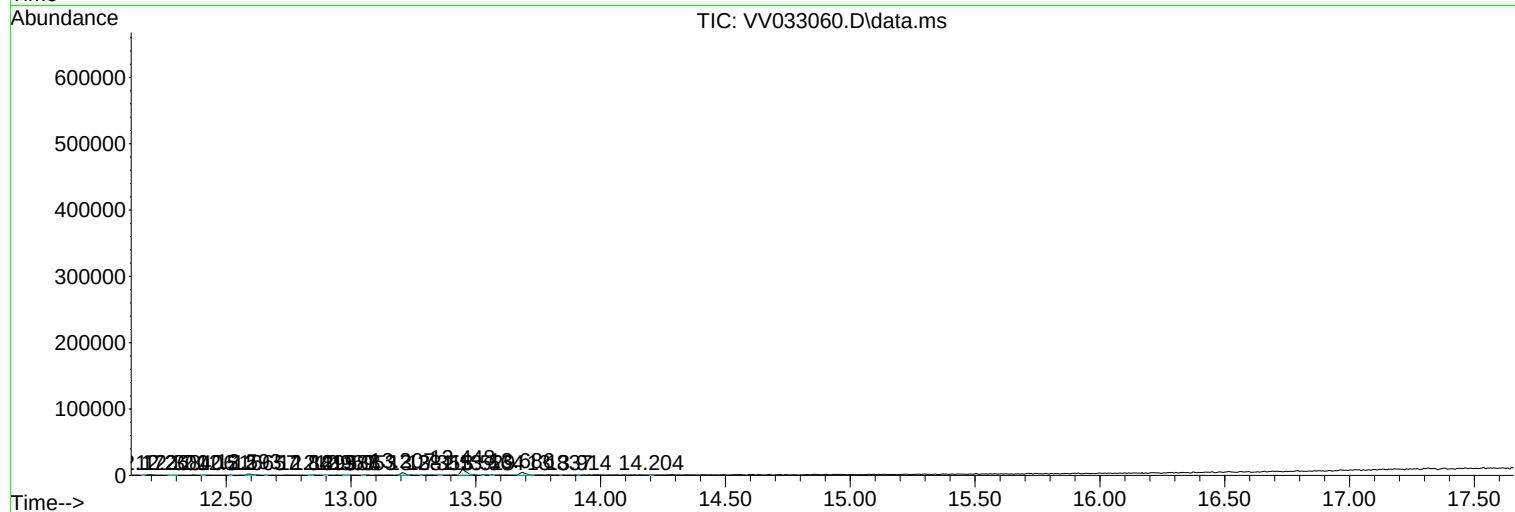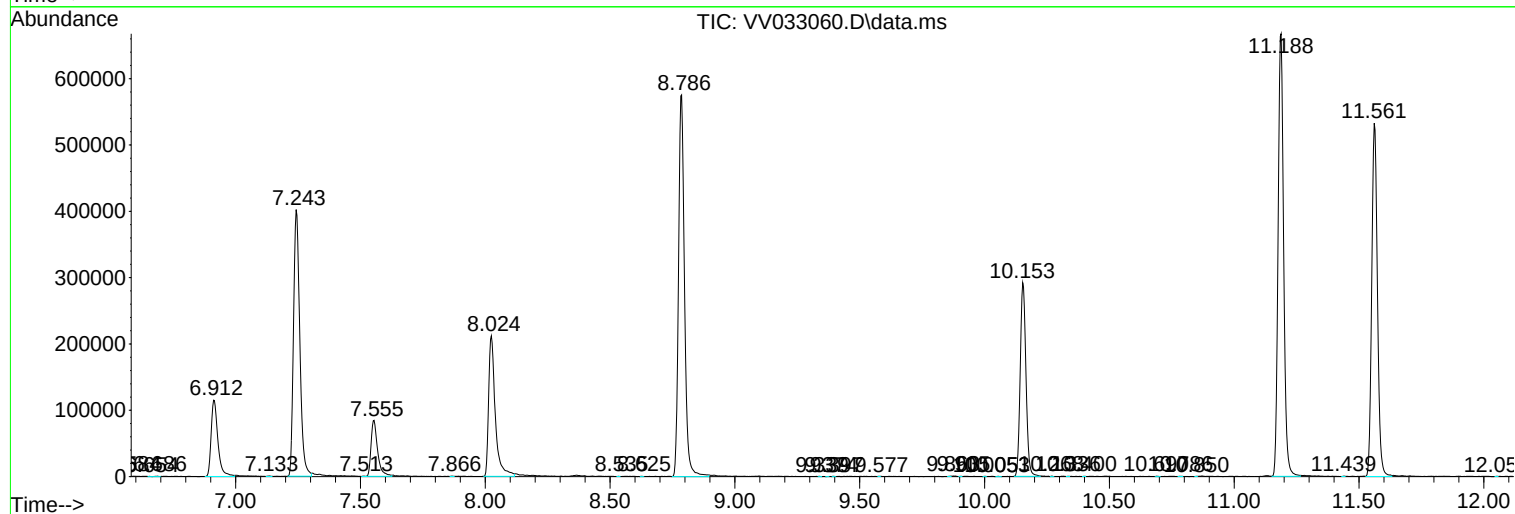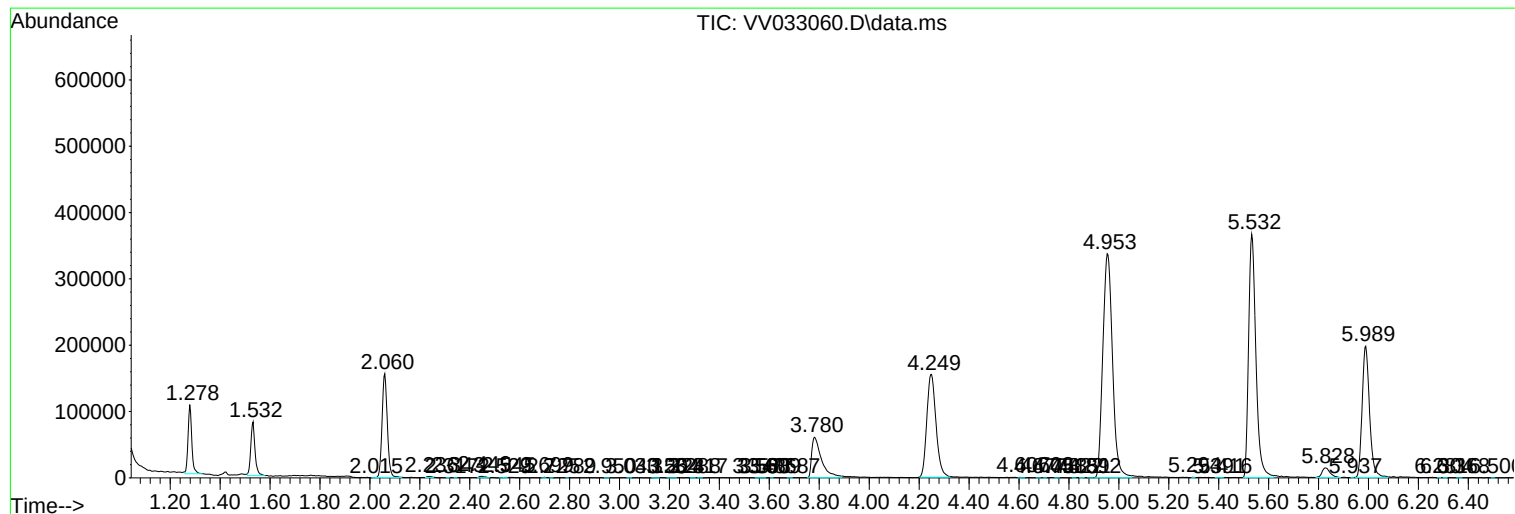

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033060.D
Acq On : 22 Nov 2023 15:29
Operator : SY/MD
Sample : VIBLK256
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK256

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033060.D
Acq On : 22 Nov 2023 15:29
Operator : SY/MD
Sample : VIBLK256
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK256

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------