


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112223\
Data File : VV033051.D
Acq On : 22 Nov 2023 08:52
Operator : SY/MD
Sample : BFB236
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB236

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM112023WMA.M
Title : VOC Analysis
Last Update : Wed Nov 22 03:48:12 2023

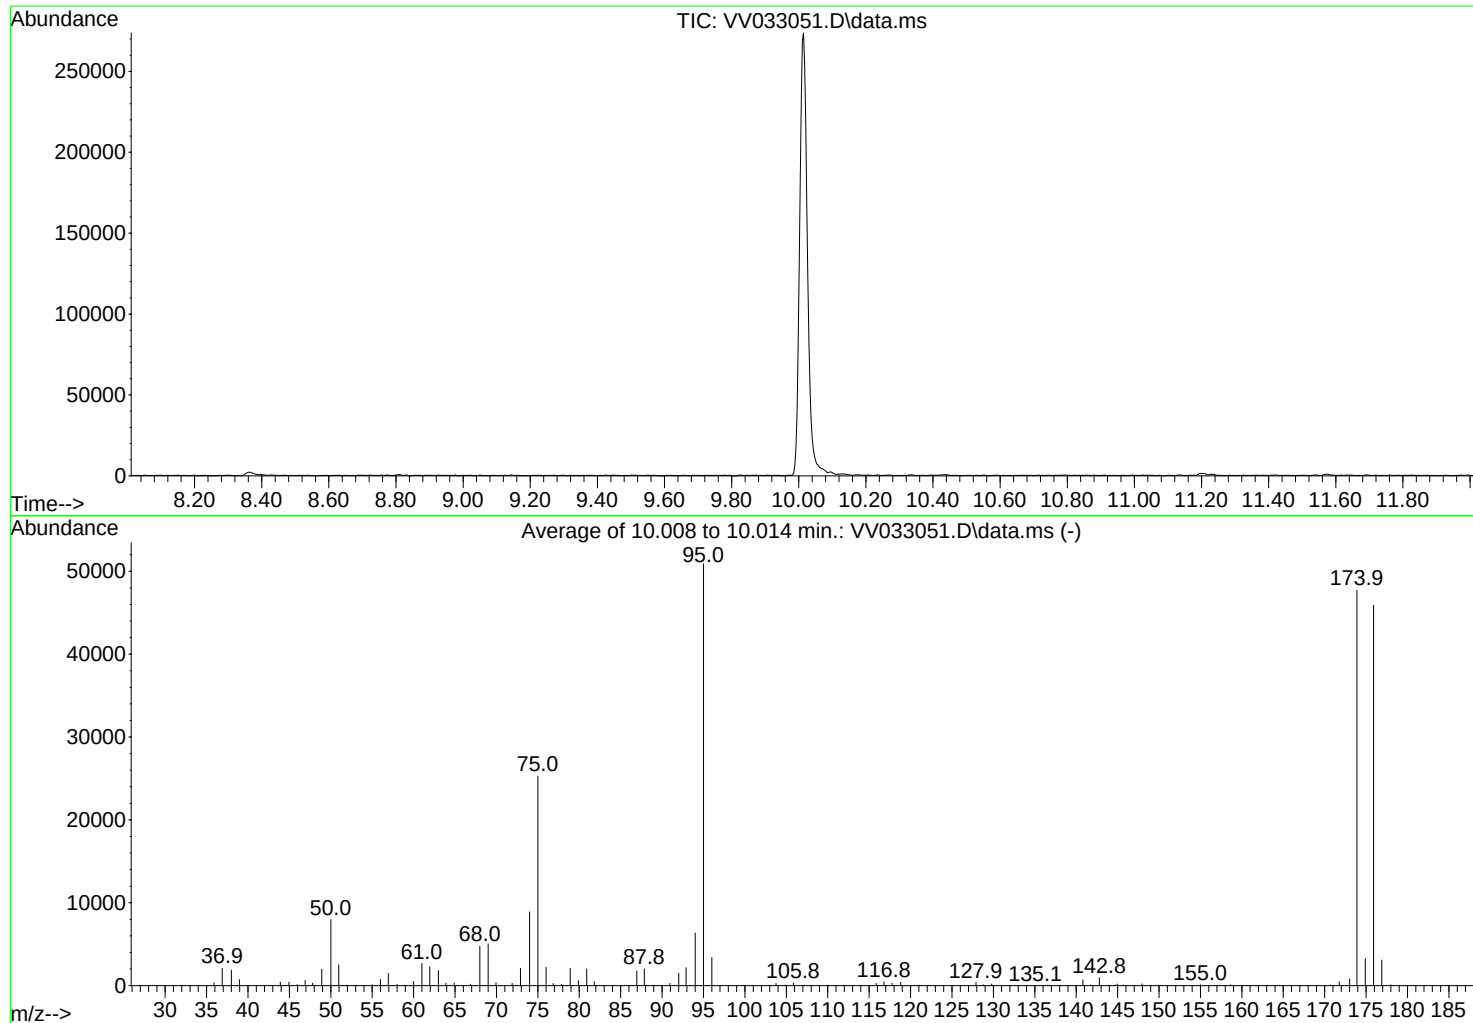

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	7963	PASS
75	95	30	80	49.7	25288	PASS
95	95	100	100	100.0	50899	PASS
96	95	5	9	6.7	3389	PASS
173	174	0.00	2	1.7	805	PASS
174	95	50	120	93.7	47709	PASS
175	174	5	9	6.8	3268	PASS
176	174	95	105	96.2	45904	PASS
177	176	5	10	6.7	3088	PASS

m/z	Abundance
39.70	132.0
39.90	133.0
43.60	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236

m/z	Abundance
35.90	371.0
36.90	1884.0
38.00	1774.0
39.00	798.0
39.80	166.0
43.90	332.0
45.00	389.0
45.90	144.0
46.90	641.0
47.80	301.0
48.90	1916.0
50.00	7692.0
51.00	2434.0
54.90	107.0
56.00	699.0
56.90	1362.0
58.00	146.0
60.00	506.0
61.00	2329.0
61.90	2130.0
63.00	1717.0
63.80	293.0
65.00	291.0
66.80	179.0
68.00	4553.0
69.00	4504.0
70.00	307.0
71.90	294.0
72.90	2002.0
74.00	8363.0
75.00	23344.0
76.00	2079.0
76.90	197.0
77.90	116.0
78.90	1875.0
79.90	603.0
80.90	1880.0
81.80	409.0
86.90	1576.0
87.80	1879.0
90.90	227.0
92.00	1346.0
92.90	1945.0
94.00	5695.0
95.00	47440.0
96.00	3090.0
103.80	284.0
105.90	312.0
115.80	273.0
116.80	404.0
117.80	290.0
118.80	371.0
127.90	266.0
129.40	118.0
129.70	133.0
140.80	628.0
141.70	105.0
142.80	910.0
145.00	268.0
148.00	213.0
149.90	103.0
155.00	102.0
160.70	110.0
170.70	158.0
171.70	407.0
173.00	734.0
173.90	42344.0
174.90	2943.0
175.90	40952.0
176.90	2818.0
178.00	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236

m/z	Abundance
35.90	354.0
36.90	2231.0
38.00	1945.0
39.00	756.0
39.90	166.0
43.90	413.0
45.00	465.0
46.00	164.0
46.90	634.0
47.80	318.0
48.90	2055.0
50.00	8218.0
50.90	2578.0
55.00	114.0
56.00	759.0
56.90	1558.0
58.00	158.0
60.00	535.0
61.00	2771.0
62.00	2303.0
63.00	1815.0
63.90	296.0
64.90	285.0
66.80	178.0
68.00	4974.0
69.00	5244.0
69.90	360.0
71.90	255.0
72.90	2154.0
74.00	9266.0
75.00	26248.0
76.00	2283.0
76.80	283.0
77.80	155.0
78.90	2150.0
79.90	634.0
80.90	2108.0
81.80	494.0
86.90	1802.0
87.90	2132.0
91.00	296.0
92.00	1538.0
92.90	2235.0
94.00	6562.0
95.00	52712.0
96.00	3466.0
103.70	264.0
104.90	104.0
105.80	318.0
115.80	297.0
116.80	484.0
117.80	331.0
118.80	392.0
127.90	398.0
128.80	130.0
129.80	176.0
140.80	743.0
141.80	124.0
142.80	1009.0
145.00	313.0
145.70	117.0
147.90	216.0
149.90	112.0
155.00	125.0
158.60	144.0
170.70	126.0
171.80	504.0
173.00	831.0
173.90	49152.0
174.90	3406.0
175.90	47144.0
176.90	3232.0
178.00	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236

m/z	Abundance
35.90	346.0
36.90	2200.0
38.00	1914.0
38.90	669.0
39.90	170.0
43.90	504.0
44.90	474.0
46.00	149.0
46.90	587.0
47.80	316.0
48.90	1927.0
50.00	7979.0
50.90	2551.0
51.90	150.0
55.10	142.0
56.00	727.0
57.00	1461.0
58.00	176.0
60.00	467.0
61.00	2904.0
61.90	2425.0
63.00	1912.0
64.00	301.0
64.80	339.0
66.90	161.0
68.00	4705.0
69.00	5352.0
69.90	386.0
71.90	257.0
72.90	2118.0
74.00	9069.0
75.00	26272.0
76.00	2246.0
76.80	303.0
77.80	174.0
78.90	2227.0
79.90	574.0
80.90	2046.0
81.80	535.0
87.00	1878.0
87.90	2063.0
91.00	299.0
92.00	1555.0
92.90	2297.0
94.00	6805.0
95.00	52544.0
96.00	3610.0
103.70	262.0
104.90	118.0
105.80	300.0
115.90	273.0
116.80	528.0
117.70	280.0
118.80	384.0
127.90	461.0
128.80	177.0
129.90	259.0
135.10	113.0
136.80	115.0
140.80	796.0
141.80	123.0
142.80	949.0
144.70	283.0
145.80	122.0
147.90	236.0
149.60	113.0
155.00	136.0
158.70	152.0
171.80	490.0
173.00	851.0
173.90	51632.0
174.90	3454.0
175.90	49616.0
176.90	3214.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236