

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112320\
 Data File : VV019431.D
 Acq On : 23 Nov 2020 19:37
 Operator : SY/MD
 Sample : L4794-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BG9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	83	rVB	268226	272923	16.96%	2.283%
2	1.576	144	151	163	rVB	210722	243598	15.14%	2.038%
3	2.119	311	320	346	rVB	448291	672233	41.78%	5.624%
4	2.521	440	445	446	rBV3	1588	1399	0.09%	0.012%
5	2.585	464	465	468	rBV2	414	263	0.02%	0.002%
6	2.624	475	477	480	rBV3	498	288	0.02%	0.002%
7	2.695	497	499	500	rBV	562	217	0.01%	0.002%
8	2.704	500	502	505	rVB3	719	348	0.02%	0.003%
9	3.100	621	625	627	rBV2	389	342	0.02%	0.003%
10	3.129	632	634	636	rBV	368	197	0.01%	0.002%
11	3.167	642	646	648	rBV	201	145	0.01%	0.001%
12	3.177	648	649	651	rBV	192	56	0.00%	0.000%
13	3.209	657	659	661	rVB	401	160	0.01%	0.001%
14	3.254	670	673	675	rBV2	305	136	0.01%	0.001%
15	3.270	676	678	683	rVB2	418	254	0.02%	0.002%
16	3.322	692	694	695	rBV	196	63	0.00%	0.001%
17	3.363	705	707	709	rBV	252	130	0.01%	0.001%
18	3.392	714	716	718	rBV	541	306	0.02%	0.003%
19	3.421	722	725	734	rVB3	617	720	0.04%	0.006%
20	3.460	734	737	738	rBV	495	189	0.01%	0.002%
21	3.482	742	744	746	rBV2	266	177	0.01%	0.001%
22	3.505	749	751	754	rBV3	254	210	0.01%	0.002%
23	3.537	759	761	766	rVB2	378	292	0.02%	0.002%
24	3.560	766	768	771	rBV	260	146	0.01%	0.001%
25	3.576	771	773	774	rBV	281	112	0.01%	0.001%
26	3.611	783	784	786	rVB	160	60	0.00%	0.001%
27	3.634	786	791	794	rBV	317	271	0.02%	0.002%
28	3.656	796	798	801	rVB	288	145	0.01%	0.001%
29	3.679	801	805	809	rBV3	380	375	0.02%	0.003%
30	3.736	821	823	825	rBV	77	36	0.00%	0.000%
31	3.756	825	829	833	rVB2	264	210	0.01%	0.002%
32	3.781	833	837	839	rBV2	287	225	0.01%	0.002%
33	3.798	840	842	845	rBV	275	124	0.01%	0.001%
34	3.817	845	848	850	rBV	332	197	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112320\
 Data File : VV019431.D
 Acq On : 23 Nov 2020 19:37
 Operator : SY/MD
 Sample : L4794-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BG9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

35	3.855	857	860	861	rBV	182	100	0.01%	0.001%
36	3.894	862	872	902	rBV	126497	337462	20.98%	2.823%
37	4.373	1003	1021	1049	rBV	259058	645968	40.15%	5.404%
38	4.852	1168	1170	1172	rBV2	267	129	0.01%	0.001%
39	4.900	1182	1185	1188	rBV	784	582	0.04%	0.005%
40	4.926	1192	1193	1195	rBV	256	103	0.01%	0.001%
41	4.981	1209	1210	1217	rVB3	548	394	0.02%	0.003%
42	5.068	1217	1237	1268	rBV2	628267	1608853	100.00%	13.459%
43	5.338	1317	1321	1326	rBV2	1024	1153	0.07%	0.010%
44	5.498	1369	1371	1372	rBV	474	179	0.01%	0.001%
45	5.553	1386	1388	1389	rBV	443	181	0.01%	0.002%
46	5.637	1401	1414	1445	rBV	419827	856248	53.22%	7.163%
47	5.926	1493	1504	1520	rBV	56887	113545	7.06%	0.950%
48	6.035	1535	1538	1540	rBV3	679	385	0.02%	0.003%
49	6.090	1541	1555	1584	rVV	363334	741778	46.11%	6.206%
50	6.469	1671	1673	1675	rVB	296	89	0.01%	0.001%
51	6.553	1698	1699	1701	rVB	267	85	0.01%	0.001%
52	6.582	1701	1708	1712	rBV3	969	969	0.06%	0.008%
53	6.604	1712	1715	1716	rBV	320	198	0.01%	0.002%
54	6.650	1727	1729	1731	rBV	107	47	0.00%	0.000%
55	6.675	1733	1737	1738	rBV2	618	391	0.02%	0.003%
56	6.833	1784	1786	1788	rBV2	356	168	0.01%	0.001%
57	6.904	1805	1808	1813	rVB2	455	443	0.03%	0.004%
58	6.965	1822	1827	1828	rBV	370	250	0.02%	0.002%
59	7.006	1828	1840	1864	rVV	187870	343916	21.38%	2.877%
60	7.334	1931	1942	1964	rBV	694742	1203856	74.83%	10.071%
61	7.640	2027	2037	2059	rBV	139981	245162	15.24%	2.051%
62	7.952	2132	2134	2140	rBV5	569	506	0.03%	0.004%
63	7.990	2143	2146	2147	rBV2	1208	651	0.04%	0.005%
64	8.067	2168	2170	2171	rBV	276	127	0.01%	0.001%
65	8.106	2171	2182	2215	rBV2	366375	767685	47.72%	6.422%
66	8.592	2331	2333	2337	rVB3	565	278	0.02%	0.002%
67	8.791	2392	2395	2396	rBV	378	206	0.01%	0.002%
68	8.871	2408	2420	2448	rBV	673148	1091043	67.81%	9.127%
69	9.161	2508	2510	2511	rBV	575	257	0.02%	0.002%
70	9.231	2529	2532	2534	rBV	539	345	0.02%	0.003%
71	9.296	2550	2552	2554	rBV3	371	152	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112320\
 Data File : VV019431.D
 Acq On : 23 Nov 2020 19:37
 Operator : SY/MD
 Sample : L4794-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BG9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

72	9.466	2604	2605	2606	rVB3	440	85	0.01%	0.001%
73	9.521	2618	2622	2626	rBV3	648	472	0.03%	0.004%
74	9.566	2634	2636	2638	rBV	609	383	0.02%	0.003%
75	10.061	2786	2790	2795	rBV4	653	771	0.05%	0.006%
76	10.122	2806	2809	2811	rBV2	582	351	0.02%	0.003%
77	10.167	2822	2823	2830	rVB	466	319	0.02%	0.003%
78	10.235	2832	2844	2865	rBV	389283	615554	38.26%	5.150%
79	10.447	2903	2910	2917	rVB5	793	1221	0.08%	0.010%
80	10.479	2918	2920	2922	rBV2	255	116	0.01%	0.001%
81	10.627	2963	2966	2968	rBV2	615	322	0.02%	0.003%
82	10.842	3031	3033	3036	rBV	542	247	0.02%	0.002%
83	10.890	3045	3048	3050	rBV2	439	258	0.02%	0.002%
84	10.923	3057	3058	3059	rBV2	205	66	0.00%	0.001%
85	11.090	3106	3110	3112	rBV2	443	381	0.02%	0.003%
86	11.270	3154	3166	3188	rBV	666846	1020501	63.43%	8.537%
87	11.556	3245	3255	3271	rBV3	12752	27001	1.68%	0.226%
88	11.646	3271	3283	3311	rVV	716525	1124657	69.90%	9.409%
89	12.489	3544	3545	3549	rBV2	501	368	0.02%	0.003%


Sum of corrected areas: 11953504

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV112320\
Data File : VV019431.D
Acq On : 23 Nov 2020 19:37
Operator : SY/MD
Sample : L4794-23
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0BG9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

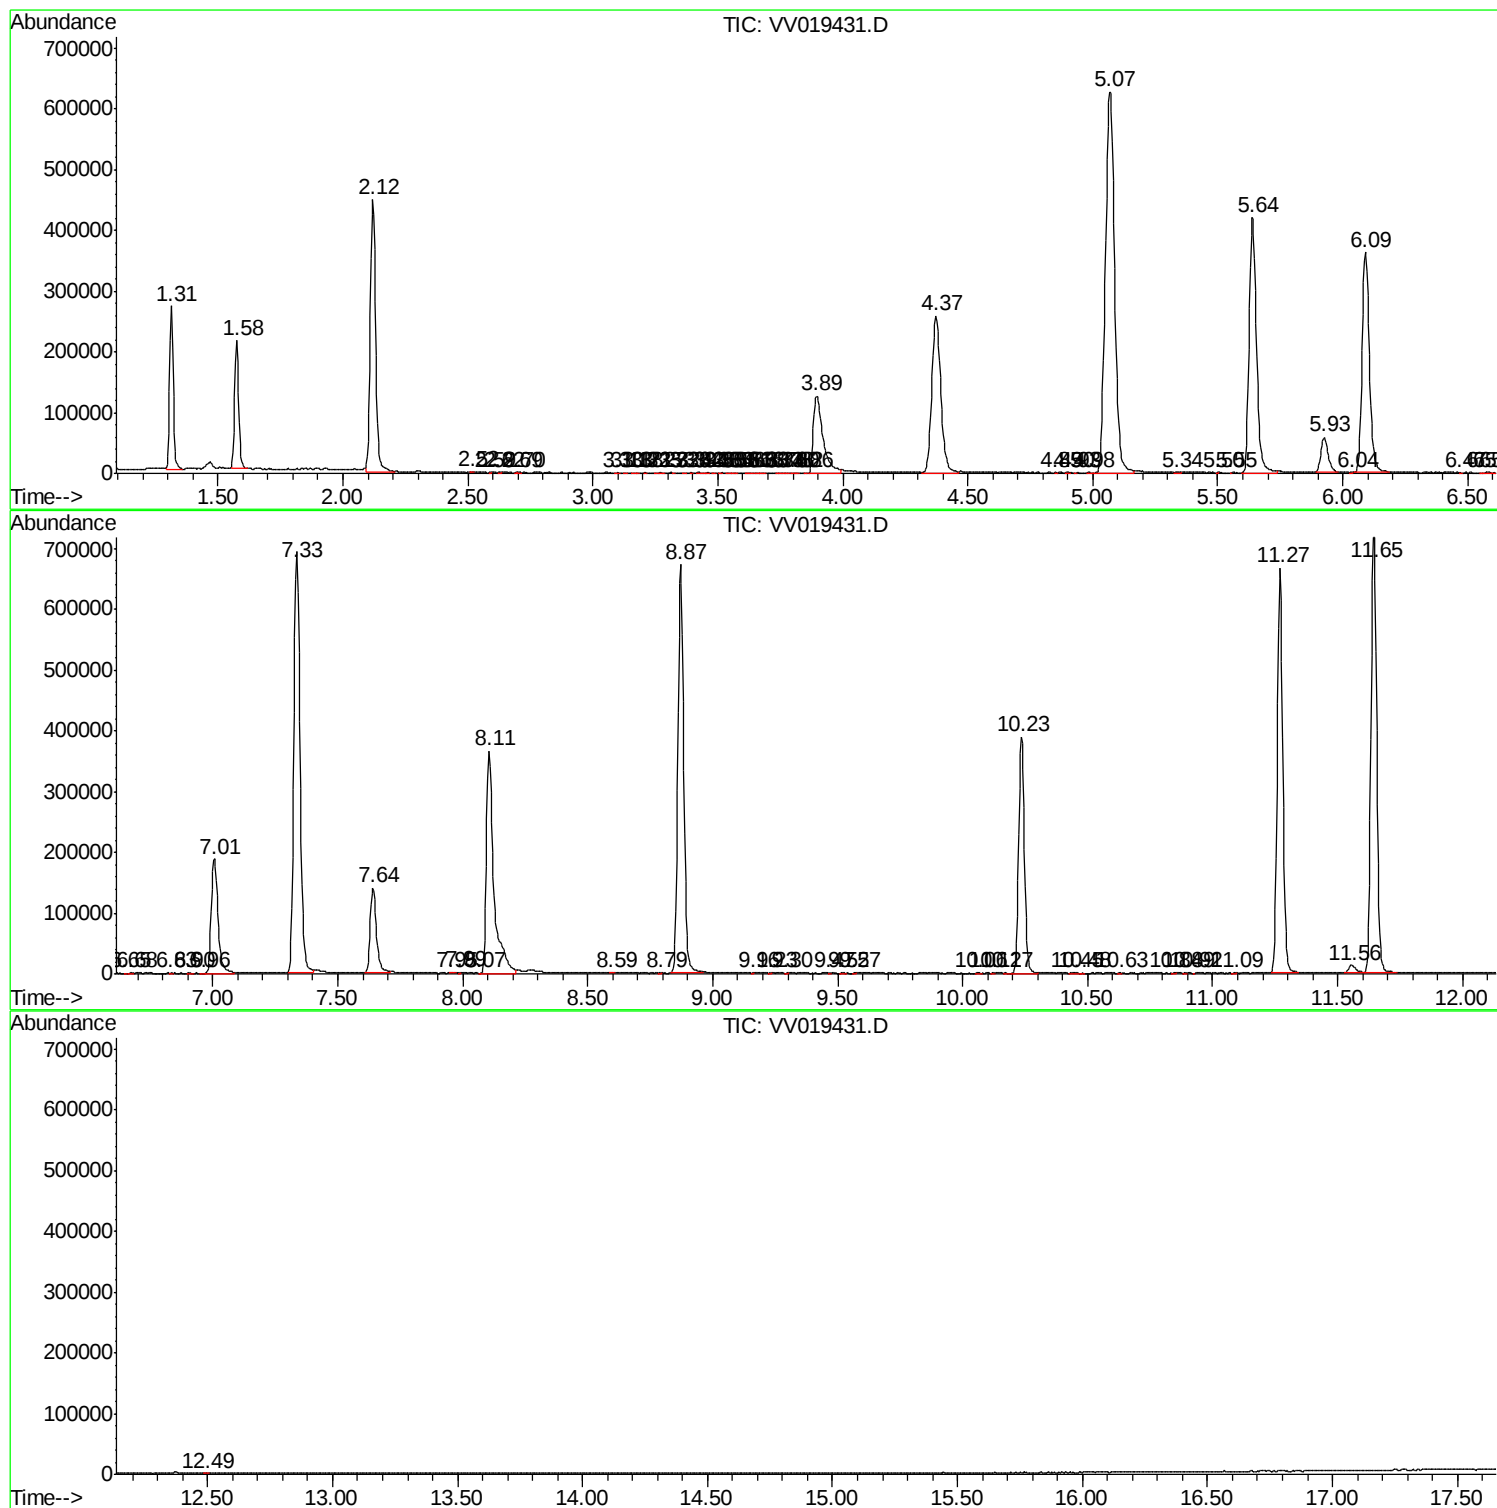

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV112320\
Data File : VV019431.D
Acq On : 23 Nov 2020 19:37
Operator : SY/MD
Sample : L4794-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BG9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112320\
Data File : VV019431.D
Acq On : 23 Nov 2020 19:37
Operator : SY/MD
Sample : L4794-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BG9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
