


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112320\
 Data File : VV019416.D
 Acq On : 23 Nov 2020 11:21
 Operator : SY/MD
 Sample : BFB96
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB96

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis
 Last Update : Mon Nov 23 12:45:37 2020

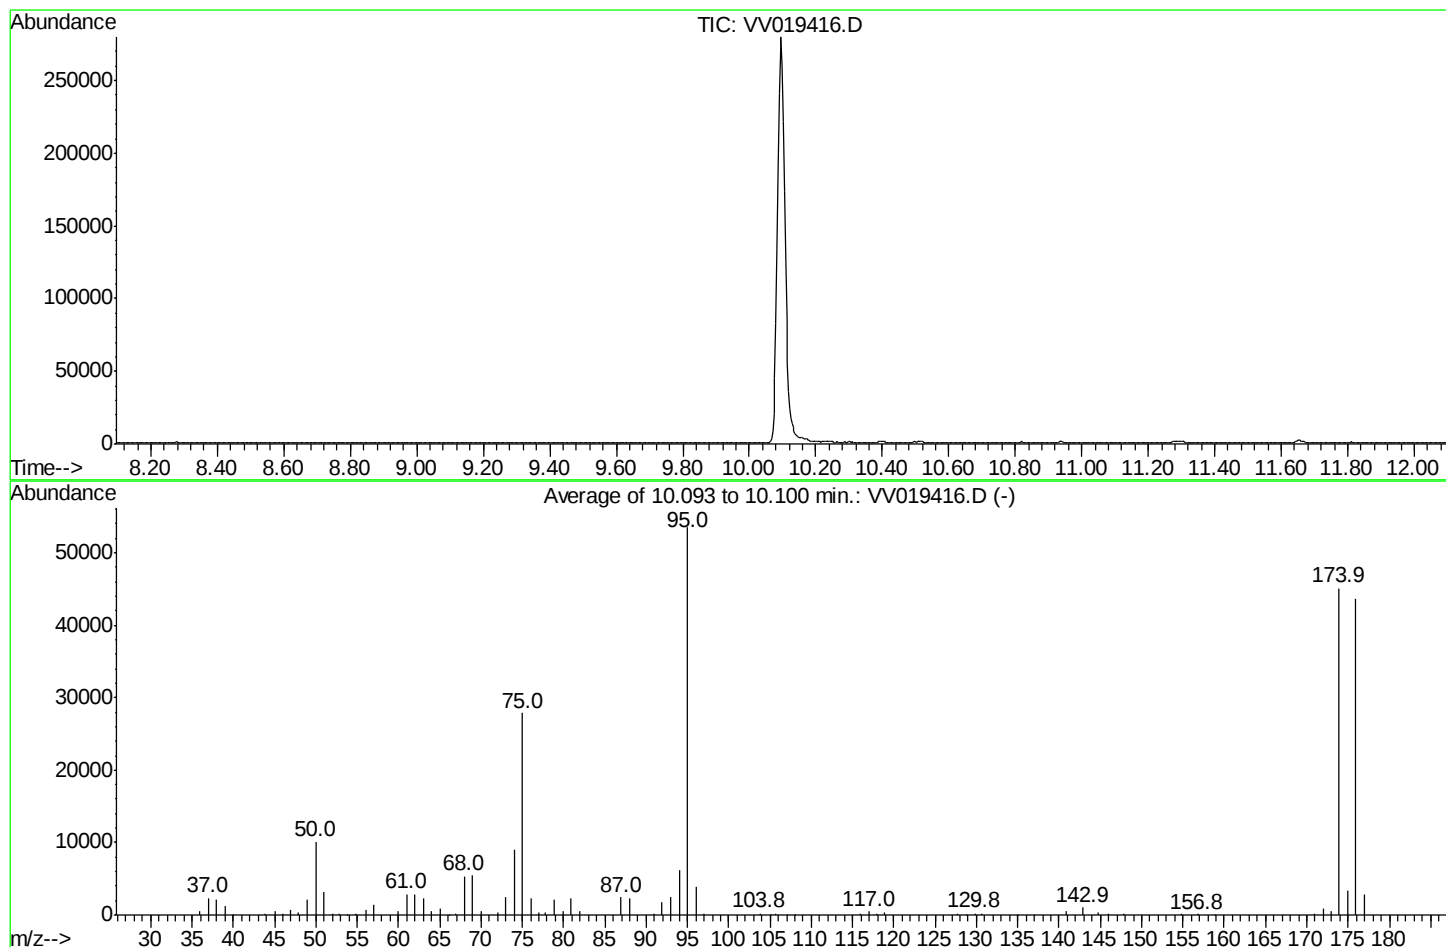

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	10077	PASS
75	95	30	80	52.1	27880	PASS
95	95	100	100	100.0	53520	PASS
96	95	5	9	7.1	3817	PASS
173	174	0.00	2	1.0	471	PASS
174	95	50	120	84.3	45122	PASS
175	174	5	9	7.3	3294	PASS
176	174	95	101	96.9	43709	PASS
177	176	5	9	6.4	2805	PASS

m/z	Abundance
35.90	625.0
37.00	2452.0
38.00	2269.0
39.00	1195.0
39.90	349.0
43.90	876.0
45.10	468.0
45.90	167.0
46.90	850.0
47.90	323.0
49.00	2131.0
50.00	10473.0
51.00	3346.0
52.00	195.0
52.80	123.0
54.80	270.0
56.00	701.0
57.00	1451.0
59.90	641.0
61.00	3107.0
62.00	2927.0
63.00	2428.0
64.00	538.0
65.00	815.0
67.00	161.0
68.00	5578.0
69.00	5541.0
69.90	423.0
72.00	330.0
73.00	2561.0
74.00	9001.0
75.00	28464.0
76.00	2326.0
76.90	346.0
77.80	296.0
78.90	2028.0
79.90	490.0
80.90	2262.0
81.90	477.0
87.00	2571.0
87.90	2079.0
90.90	219.0
92.00	1678.0
93.00	2372.0
94.00	6187.0
95.00	54712.0
96.00	3848.0
97.00	135.0
103.70	207.0
105.00	107.0
105.80	203.0
108.00	102.0
115.90	192.0
117.00	449.0
117.90	236.0
118.90	388.0
127.80	181.0
129.90	264.0
130.70	144.0
140.80	568.0
142.90	1042.0
144.70	338.0
145.90	104.0
147.80	147.0
154.70	102.0
156.80	117.0
158.80	113.0
171.10	252.0
172.00	887.0
173.90	44944.0
174.90	3380.0
175.90	42632.0
176.90	2925.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
35.90	611.0
37.00	2374.0
38.00	2222.0
39.00	1250.0
39.90	327.0
43.90	807.0
45.00	476.0
46.00	178.0
46.90	760.0
47.90	332.0
49.00	2203.0
50.00	10442.0
51.00	3234.0
52.00	193.0
52.80	121.0
53.80	109.0
54.90	272.0
56.00	651.0
57.00	1432.0
60.00	553.0
61.00	2999.0
62.00	2989.0
63.00	2391.0
64.00	584.0
65.00	821.0
67.00	162.0
68.00	5604.0
69.00	5705.0
70.00	478.0
72.00	328.0
73.00	2518.0
74.00	9227.0
75.00	28896.0
76.10	2486.0
77.00	374.0
77.80	327.0
78.90	2094.0
80.00	551.0
80.90	2244.0
81.90	494.0
87.00	2527.0
87.90	2238.0
90.90	282.0
91.90	1825.0
92.90	2515.0
94.00	6505.0
95.00	55216.0
96.00	3928.0
97.00	158.0
103.80	225.0
105.70	205.0
107.10	104.0
115.90	186.0
117.00	500.0
117.90	223.0
118.90	431.0
127.80	173.0
128.80	109.0
129.80	231.0
130.70	152.0
135.00	112.0
140.90	540.0
142.90	1081.0
144.70	379.0
145.90	151.0
147.90	139.0
154.80	112.0
156.80	125.0
171.00	269.0
172.00	975.0
172.90	722.0
173.90	46536.0
174.90	3357.0
175.90	45112.0
176.90	2836.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
35.90	484.0
37.00	2302.0
38.00	2017.0
39.00	1175.0
39.90	301.0
43.90	746.0
45.00	451.0
46.10	175.0
46.90	588.0
47.90	328.0
49.00	2132.0
50.00	9317.0
51.00	2882.0
52.10	185.0
52.80	105.0
53.80	115.0
54.90	259.0
56.00	676.0
57.00	1330.0
60.00	465.0
61.00	2650.0
62.00	2674.0
63.00	2197.0
64.00	572.0
65.00	807.0
66.10	111.0
66.90	162.0
68.00	4971.0
69.00	5344.0
70.00	443.0
72.00	306.0
73.00	2269.0
74.00	8576.0
75.00	26280.0
76.00	2261.0
77.00	379.0
77.80	284.0
78.90	2006.0
79.90	524.0
80.90	2165.0
81.90	485.0
86.90	2258.0
88.00	2396.0
90.90	280.0
91.90	1782.0
92.90	2333.0
94.00	6056.0
95.00	50632.0
96.00	3677.0
96.90	158.0
103.90	212.0
105.80	219.0
115.80	170.0
117.00	505.0
117.90	203.0
118.90	435.0
127.70	175.0
128.80	119.0
129.80	212.0
130.70	132.0
135.00	140.0
137.00	103.0
140.90	477.0
142.90	983.0
144.70	368.0
145.90	158.0
148.00	150.0
154.90	120.0
156.80	112.0
170.90	247.0
172.00	960.0
172.90	691.0
173.90	43888.0
174.90	3146.0
175.90	43384.0
176.90	2655.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

Scan 2789 (10.058 min): VV019416.D
BFB96

m/z	Abundance
39.90	239.0
44.00	624.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96