

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112321\
 Data File : VW023690.D
 Acq On : 23 Nov 2021 22:52
 Operator : SY/MD
 Sample : M4723-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 24 05:03:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 04:42:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	153903	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	151481	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	83840	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	50567	4.002	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.000%
7) Chloroethane-d5	1.568	69	41528	4.182	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.600%
11) 1,1-Dichloroethene-d2	2.108	63	69447	3.119	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.400%
20) 2-Butanone-d5	3.902	46	64001	42.139	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.280%
24) Chloroform-d	4.349	84	97994	4.454	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
26) 1,2-Dichloroethane-d4	5.037	65	47297	4.602	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
32) Benzene-d6	5.053	84	195092	4.728	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%
36) 1,2-Dichloropropane-d6	6.072	67	53065	4.587	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.800%
41) Toluene-d8	7.317	98	183526	4.760	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.200%
43) trans-1,3-Dichloroprop...	7.622	79	21074	4.519	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.400%
46) 2-Hexanone-d5	8.088	63	79384	51.239	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.480%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40435	4.857	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	73285	4.944	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.800%
Target Compounds						
					Qvalue	
3) Chloromethane	1.243	50	739	0.058	ug/L	96
8) Chloroethane	1.471	64	26221	3.104	ug/L #	54
12) 1,1-Dichloroethene	2.108	96	673	0.065	ug/L #	1
13) Acetone	2.130	43	19768	14.464	ug/L	68
14) Carbon disulfide	2.294	76	2504	0.072	ug/L	99
15) Methyl Acetate	2.432	43	38956	12.558	ug/L #	50
17) Methyl tert-butyl Ether	2.770	73	13962	0.661	ug/L #	1
19) 1,1-Dichloroethane	3.272	63	4286	0.217	ug/L #	1
21) 2-Butanone	3.764	43	124436	71.936	ug/L #	54
22) cis-1,2-Dichloroethene	3.915	96	989	0.088	ug/L	77
25) Chloroform	4.407	83	33597	1.527	ug/L #	33
27) 1,2-Dichloroethane	5.104	62	141036	12.059	ug/L #	79
30) Cyclohexane	4.680	56	1470230	88.999	ug/L	97
33) Benzene	5.104	78	14152303	327.704	ug/L	100
34) Trichloroethene	5.940	95	5068	0.438	ug/L #	30
35) Methylcyclohexane	6.133	83	962865	53.387	ug/L	98
37) 1,2-Dichloropropane	6.130	63	11176	1.089	ug/L #	95
38) Bromodichloromethane	6.564	83	10693	0.767	ug/L #	32
39) cis-1,3-Dichloropropene	6.992	75	3209	0.220	ug/L #	42

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112321\
 Data File : VV023690.D
 Acq On : 23 Nov 2021 22:52
 Operator : SY/MD
 Sample : M4723-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 24 05:03:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 04:42:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


42) Toluene	7.387	91	1051183	22.445	ug/L	98
45) 1,1,2-Trichloroethane	7.789	97	42919	6.038	ug/L #	20
48) 2-Hexanone	8.165	43	3983	1.100	ug/L #	1
52) Ethylbenzene	9.011	91	5019715	102.535	ug/L	99
53) m,p-xylene	9.140	106	609837	31.299	ug/L	99
54) o-xylene	9.541	106	109560	5.913	ug/L	98
55) Styrene	9.541	104	7794	0.250	ug/L #	1
57) 1,1,2,2-Tetrachloroethane	10.242	83	2958	0.374	ug/L #	56
60) Isopropylbenzene	9.931	105	611566	12.217	ug/L	100
61) 1,2,3-Trichloropropane	10.352	75	7283	1.225	ug/L #	1
62) 1,3,5-Trimethylbenzene	10.538	105	202025	4.850	ug/L	99
63) 1,2,4-Trimethylbenzene	10.914	105	108379	2.631	ug/L	99
67) 1,2-Dichlorobenzene	11.644	146	2763	0.118	ug/L #	75
68) 1,2-Dibromo-3-chloropr...	12.410	75	6999	5.928	ug/L #	1
71) Naphthalene	13.487	128	29337	1.406	ug/L #	24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
Data File : VV023690.D
Acq On : 23 Nov 2021 22:52
Operator : SY/MD
Sample : M4723-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 24 05:03:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 04:42:45 2021
Response via : Initial Calibration




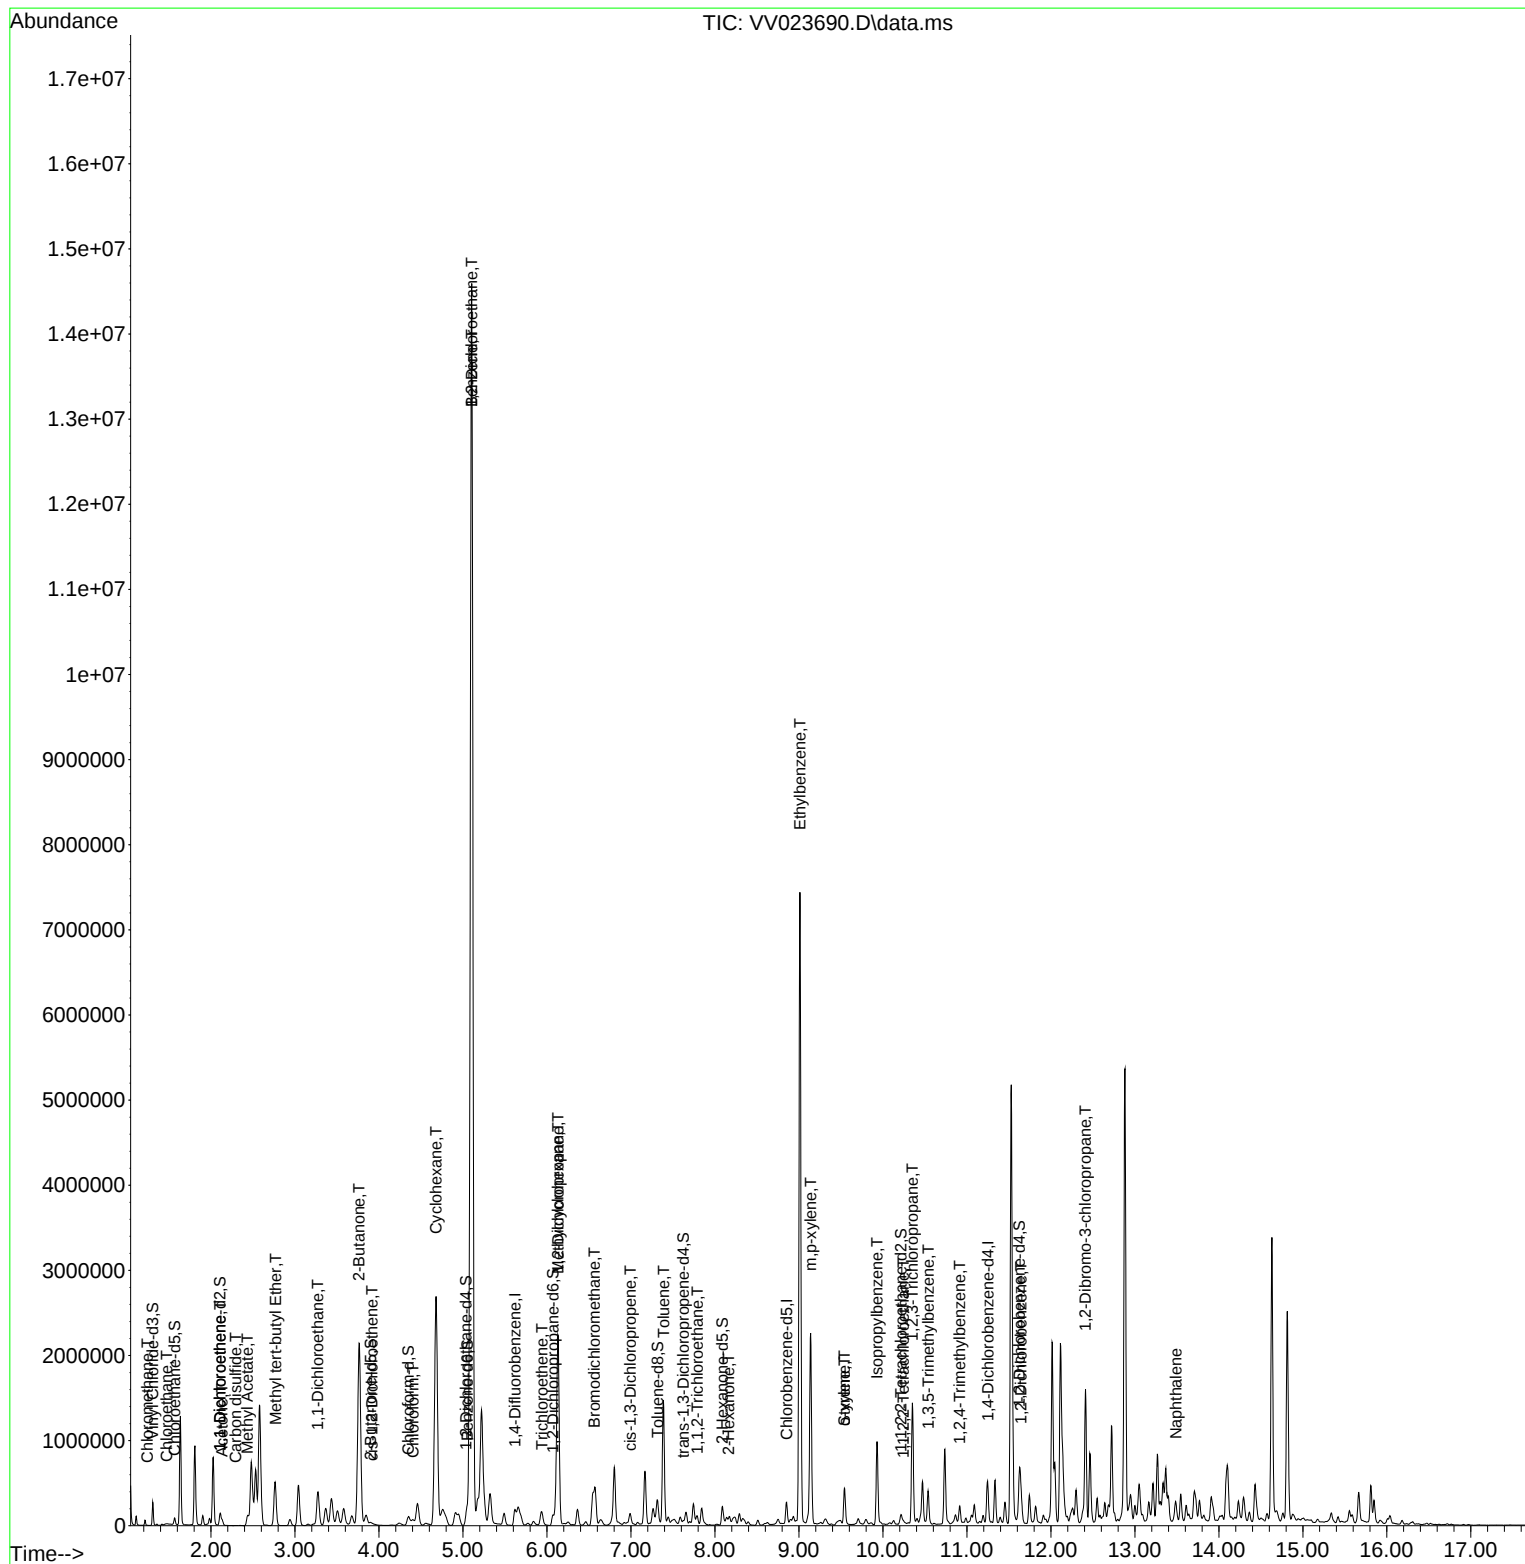


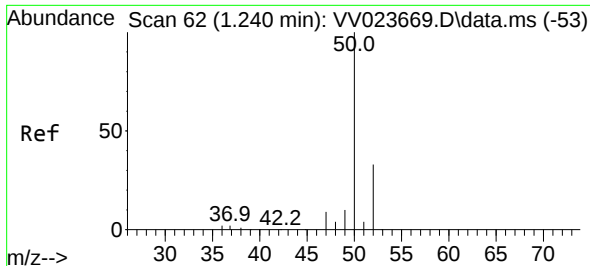

#3
Chloromethane
Concen: 0.058 ug/L
RT: 1.243 min Scan# 61
Delta R.T. 0.003 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 50 Resp: 739
Ion Ratio Lower Upper
50 100
52 29.3 22.0 41.0

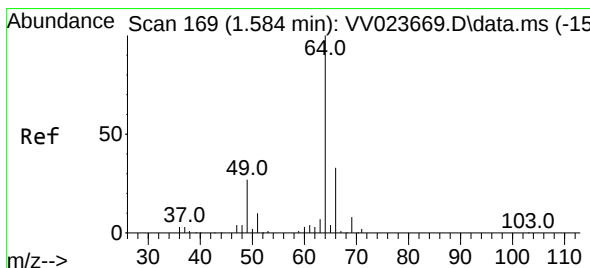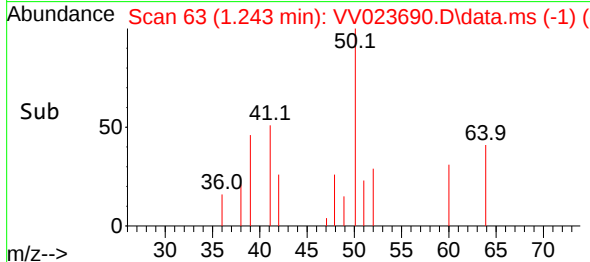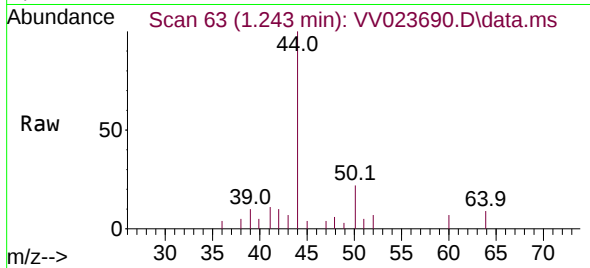

#8
Chloroethane
Concen: 3.104 ug/L
RT: 1.471 min Scan# 134
Delta R.T. -0.113 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52


Tgt Ion: 64 Resp: 26221
Ion Ratio Lower Upper
64 100
66 5.3 21.4 39.8#

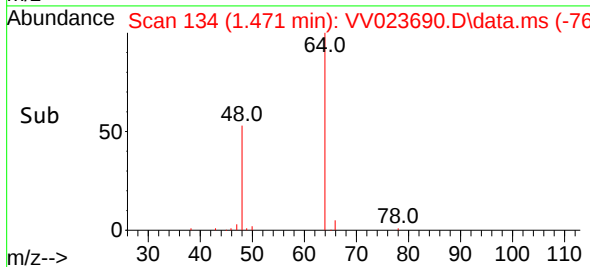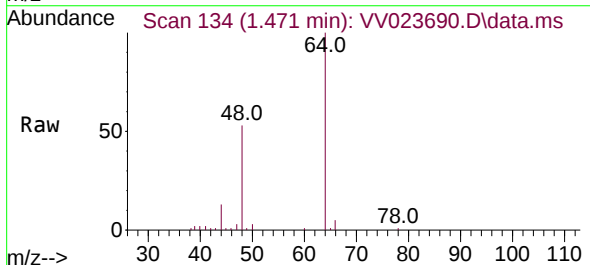






#12
1,1-Dichloroethene
Concen: 0.065 ug/L
RT: 2.108 min Scan# 311
Delta R.T. -0.010 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52

Instrument :
MSVOA_V
ClientSampleId :



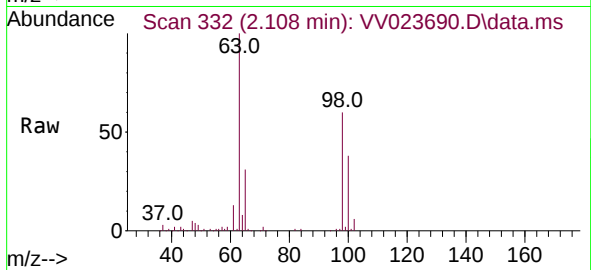



Tgt Ion: 96 Resp: 673
Ion Ratio Lower Upper
96 100
61 1421.2 116.1 215.5#
63 10889.4 79.4 147.4#

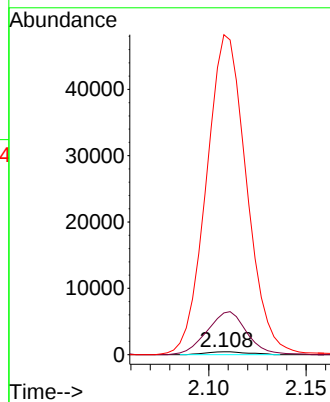

#13
Acetone
Concen: 14.464 ug/L
RT: 2.130 min Scan# 339
Delta R.T. -0.058 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52


Tgt Ion: 43 Resp: 19768
Ion Ratio Lower Upper
43 100
58 6.0 0.0 41.4

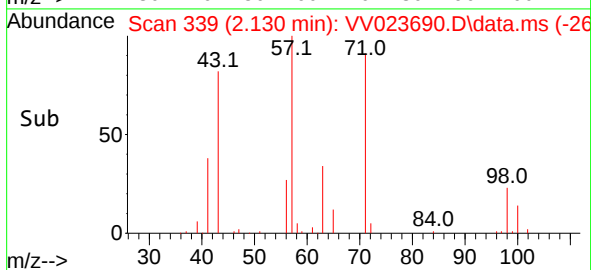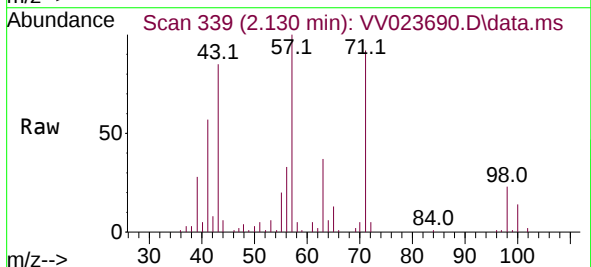






#14
Carbon disulfide
Concen: 0.072 ug/L
RT: 2.294 min Scan# 390
Delta R.T. -0.000 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52

Instrument :
MSVOA_V
ClientSampleId :







Tgt Ion: 76 Resp: 2504
Ion Ratio Lower Upper
76 100
78 9.6 7.5 11.3

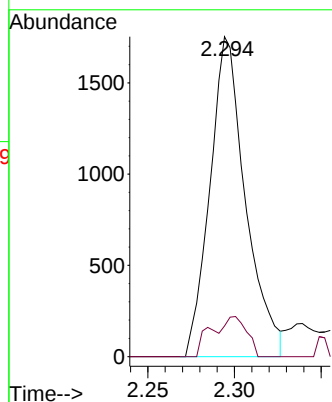

#15
Methyl Acetate
Concen: 12.558 ug/L
RT: 2.432 min Scan# 433
Delta R.T. -0.010 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52


Tgt Ion: 43 Resp: 38956
Ion Ratio Lower Upper
43 100
74 0.1 20.2 30.2#








#17
Methyl tert-butyl Ether
Concen: 0.661 ug/L
RT: 2.770 min Scan# 51
Delta R.T. 0.003 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52


Instrument :
MSVOA_V
ClientSampleId :

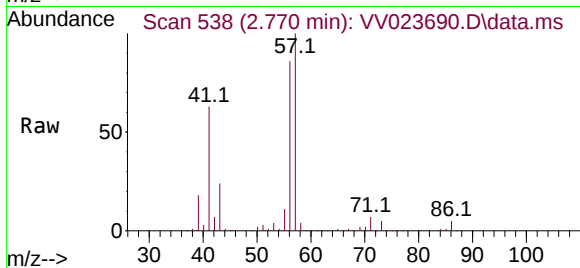



Tgt Ion: 73 Resp: 13962
Ion Ratio Lower Upper
73 100
43 484.5 15.5 23.3#
57 2079.7 17.1 25.7#

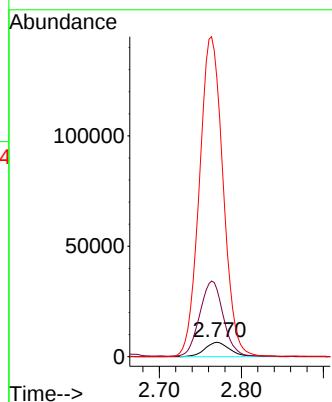


#19
1,1-Dichloroethane
Concen: 0.217 ug/L
RT: 3.272 min Scan# 694
Delta R.T. 0.083 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52

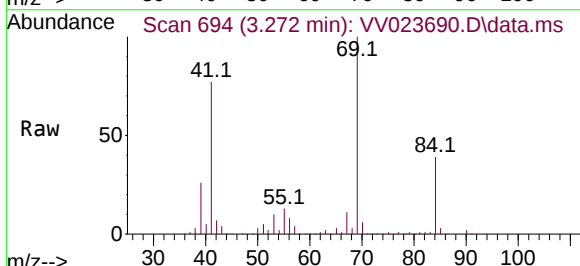

Tgt Ion: 63 Resp: 4286
Ion Ratio Lower Upper
63 100
65 156.6 22.3 41.3#
83 62.1 10.7 19.9#




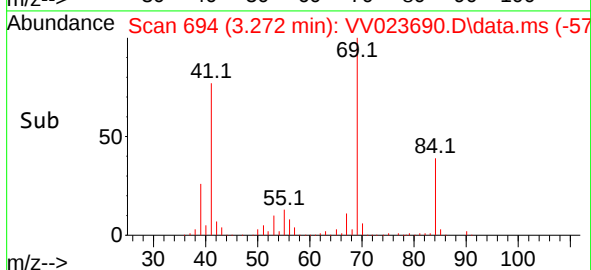




#21
2-Butanone
Concen: 71.936 ug/L
RT: 3.764 min Scan# 84
Delta R.T. -0.225 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 43 Resp: 124436
Ion Ratio Lower Upper
43 100
72 0.0 11.1 33.1#



#22
cis-1,2-Dichloroethene
Concen: 0.088 ug/L
RT: 3.915 min Scan# 894
Delta R.T. 0.003 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52

Tgt Ion: 96 Resp: 989
Ion Ratio Lower Upper
96 100
61 93.6 83.4 154.8
68 0.0 0.0 0.0


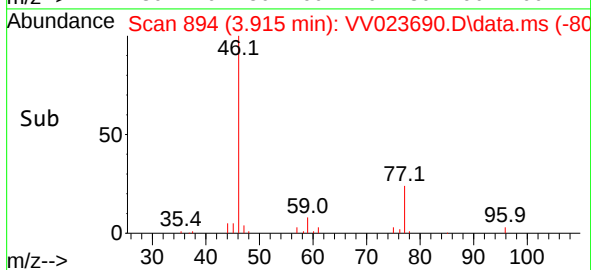




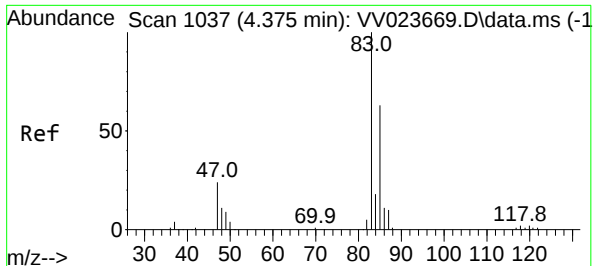

#25
Chloroform
Concen: 1.527 ug/L
RT: 4.407 min Scan# 1047
Delta R.T. 0.032 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 83 Resp: 33597
Ion Ratio Lower Upper
83 100
85 11.8 45.2 84.0#

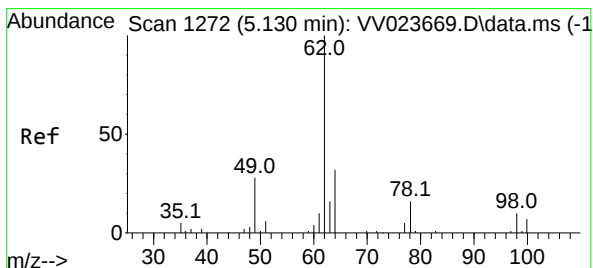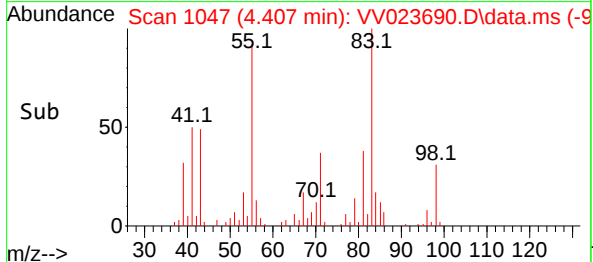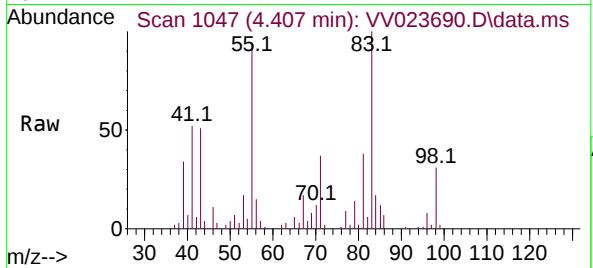

#27
1,2-Dichloroethane
Concen: 12.059 ug/L
RT: 5.104 min Scan# 1264
Delta R.T. -0.026 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52


Tgt Ion: 62 Resp: 141036
Ion Ratio Lower Upper
62 100
98 2.2 8.1 12.1#

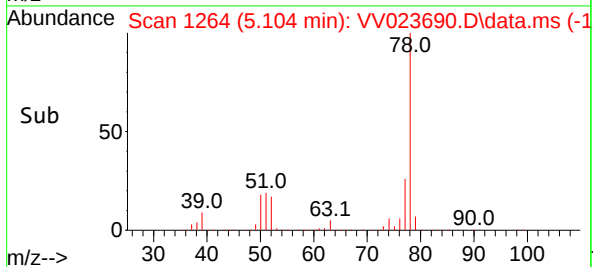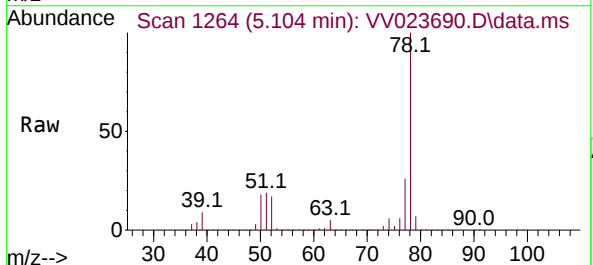



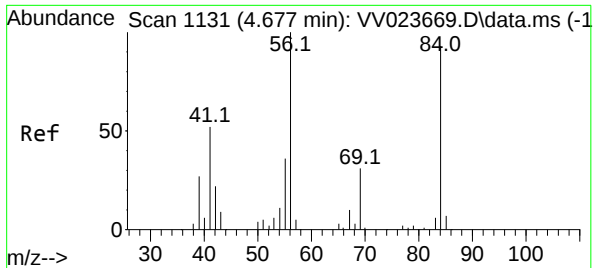


#30
Cyclohexane
Concen: 88.999 ug/L
RT: 4.680 min Scan# 1131
Delta R.T. 0.003 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52

Instrument :
MSVOA_V
ClientSampleId :



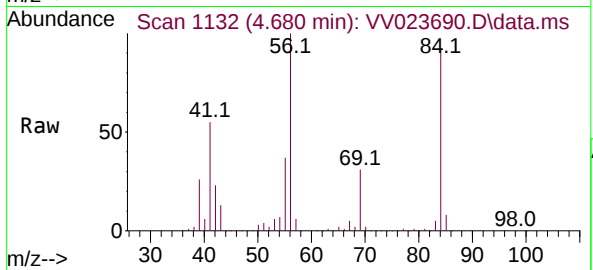



Tgt Ion: 56 Resp: 1470230
Ion Ratio Lower Upper
56 100
69 34.4 24.8 37.2
84 92.7 75.9 113.9

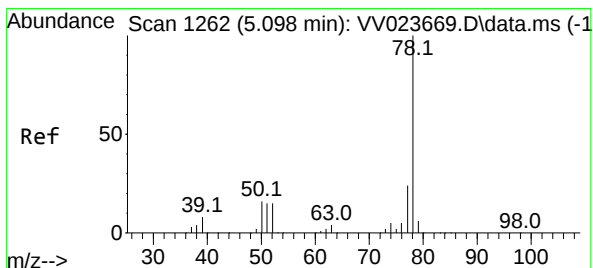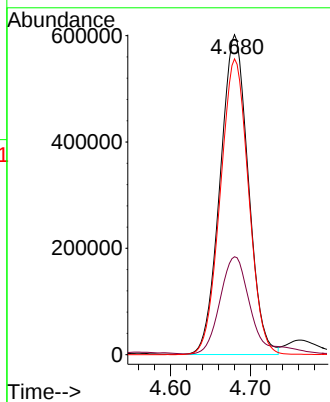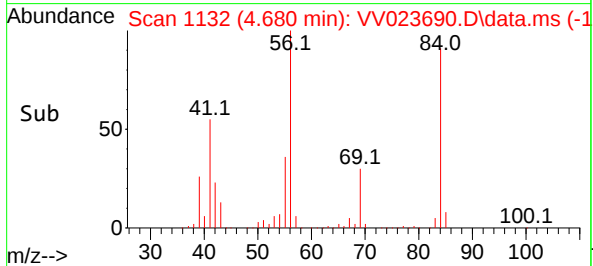

#33
Benzene
Concen: 327.704 ug/L
RT: 5.104 min Scan# 1264
Delta R.T. 0.006 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52

Tgt Ion: 78 Resp:14152303



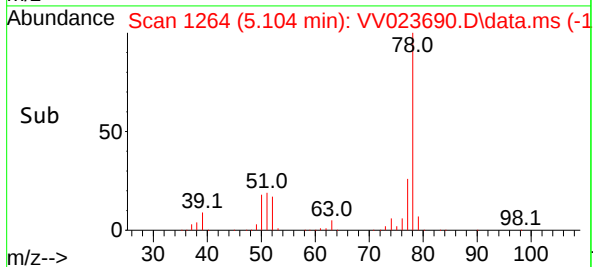
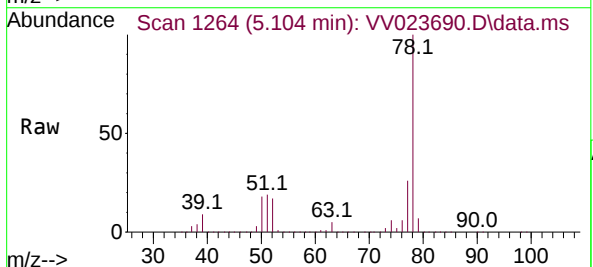




#34
Trichloroethene
Concen: 0.438 ug/L
RT: 5.940 min Scan# 1516
Delta R.T. 0.026 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 95 Resp: 5068
Ion Ratio Lower Upper
95 100
97 48.4 45.2 84.0
132 21.4 76.1 141.3#
130 17.3 75.4 140.0#

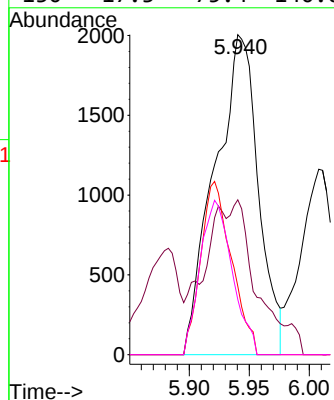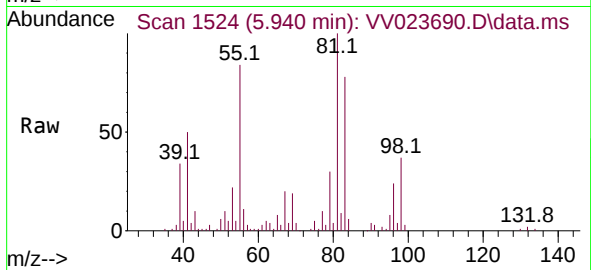

#35
Methylcyclohexane
Concen: 53.387 ug/L
RT: 6.133 min Scan# 1584
Delta R.T. 0.003 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52

Tgt Ion: 83 Resp: 962865
Ion Ratio Lower Upper
83 100
55 76.7 60.2 90.2
98 50.3 41.0 61.4

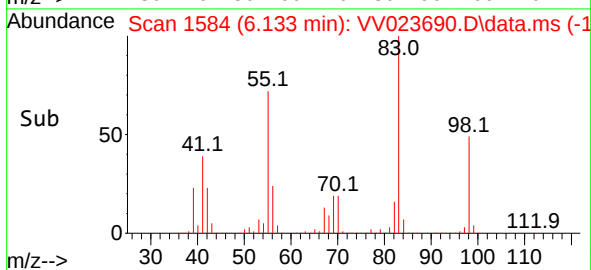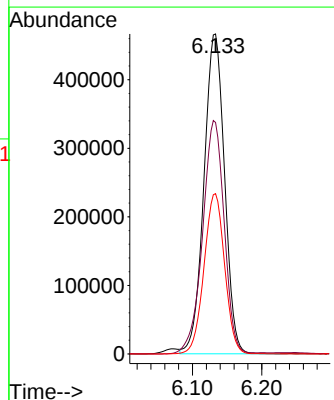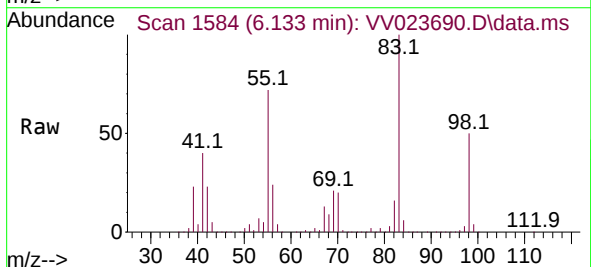

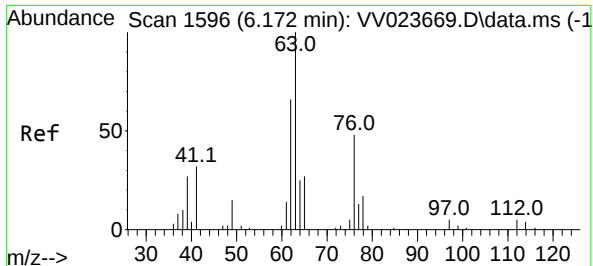

#37

1,2-Dichloropropane

Concen: 1.089 ug/L

RT: 6.130 min Scan# 11

Delta R.T. -0.042 min

Lab File: VV023690.D

Acq: 23 Nov 2021 22:52

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 63 Resp: 11176

Ion Ratio Lower Upper

63 100

112 7.2 4.3 6.5#

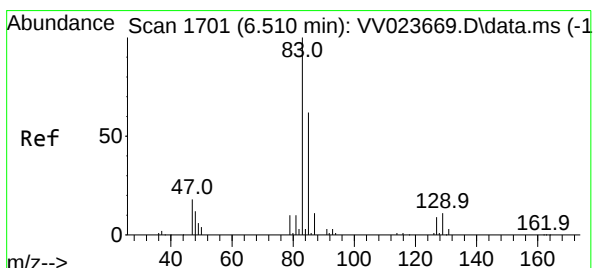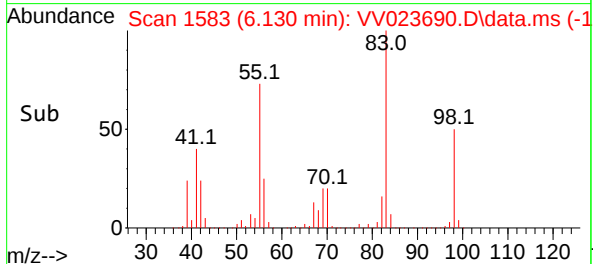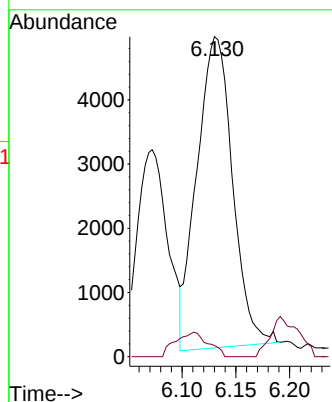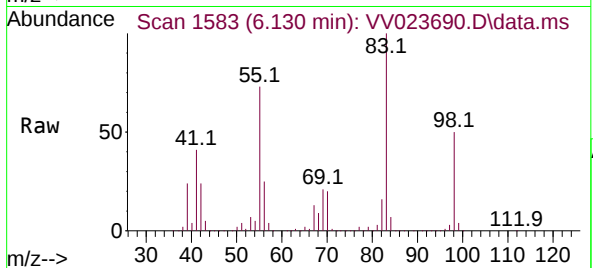

#38

Bromodichloromethane

Concen: 0.767 ug/L

RT: 6.564 min Scan# 1718

Delta R.T. 0.055 min

Lab File: VV023690.D

Acq: 23 Nov 2021 22:52




Tgt Ion: 83 Resp: 10693


Ion Ratio Lower Upper

83 100

85 5.0 44.0 81.8#

127 0.0 8.6 12.8#

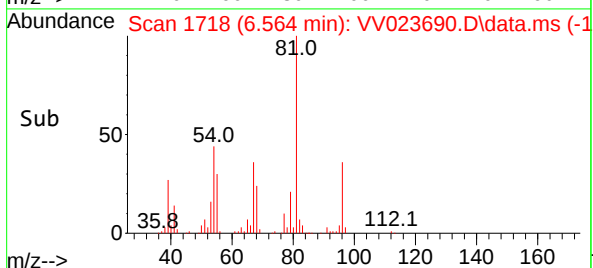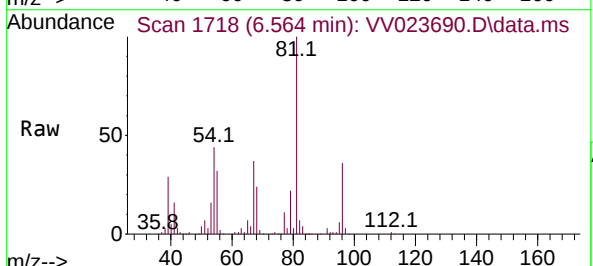

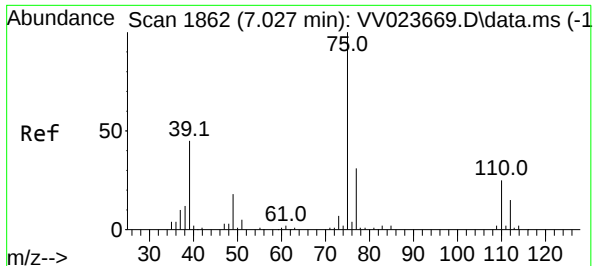

#39

cis-1,3-Dichloropropene

Concen: 0.220 ug/L

RT: 6.992 min Scan# 1851

Delta R.T. -0.035 min

Lab File: VV023690.D

Acq: 23 Nov 2021 22:52

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 75 Resp: 3209

Ion Ratio Lower Upper

75 100

77 63.8 22.0 41.0#

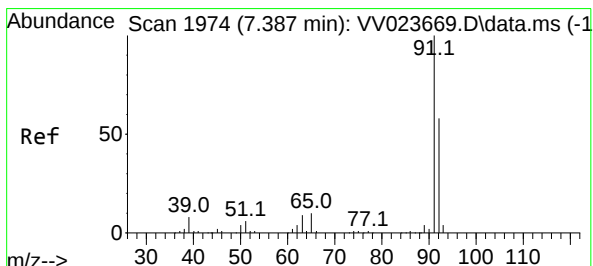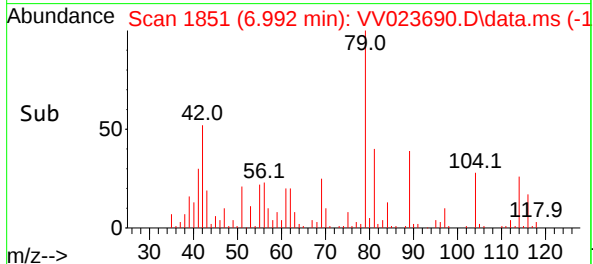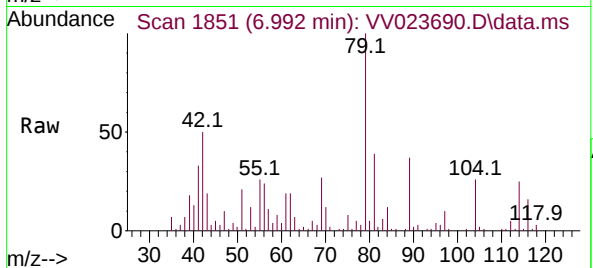

#42

Toluene

Concen: 22.445 ug/L

RT: 7.387 min Scan# 1974

Delta R.T. -0.000 min

Lab File: VV023690.D




Acq: 23 Nov 2021 22:52


Tgt Ion: 91 Resp: 1051183

Ion Ratio Lower Upper

91 100

92 57.9 41.5 77.1

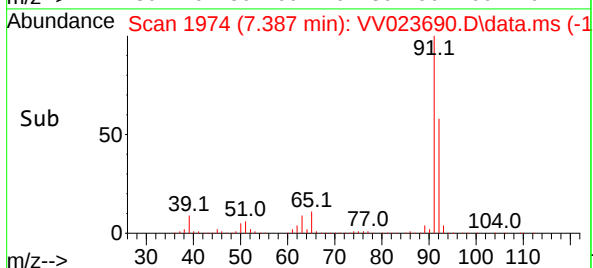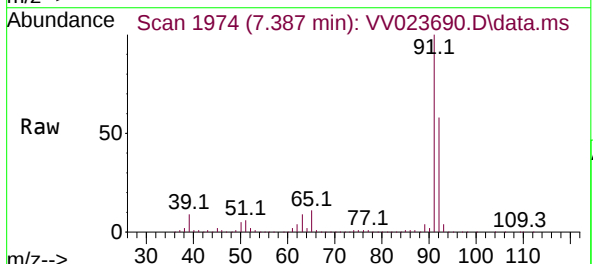



#45

1,1,2-Trichloroethane

Concen: 6.038 ug/L

RT: 7.789 min Scan# 2099

Delta R.T. -0.052 min

Lab File: VV023690.D

Acq: 23 Nov 2021 22:52

Instrument :

MSVOA_V

ClientSampleId :

Tgt Ion: 97 Resp: 42919





Ion Ratio Lower Upper

97 100

99 0.0 43.1 80.1#

83 8.2 57.9 107.5#

85 0.9 38.0 70.6#

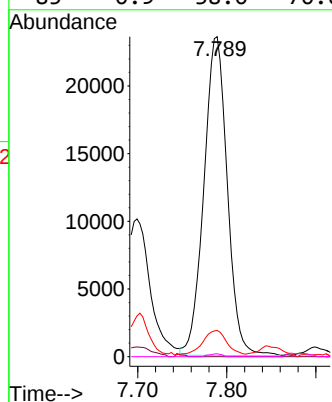

#48

2-Hexanone

Concen: 1.100 ug/L

RT: 8.165 min Scan# 2216

Delta R.T. 0.026 min

Lab File: VV023690.D

Acq: 23 Nov 2021 22:52

Tgt Ion: 43 Resp: 3983




Ion Ratio Lower Upper


43 100

58 26.2 44.5 66.7#

57 443.3 15.1 22.7#

100 0.5 10.7 16.1#


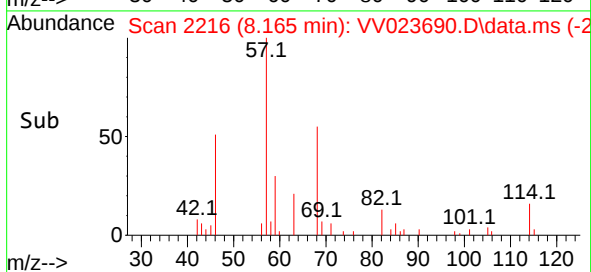






#52
Ethylbenzene
Concen: 102.535 ug/L
RT: 9.011 min Scan# 2479
Delta R.T. -0.000 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 91 Resp: 5019715
Ion Ratio Lower Upper
91 100
106 32.0 22.0 41.0



#53
m,p-xylene
Concen: 31.299 ug/L
RT: 9.140 min Scan# 2519
Delta R.T. 0.003 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52

Tgt Ion: 106 Resp: 609837
Ion Ratio Lower Upper
106 100
91 200.3 139.5 259.1




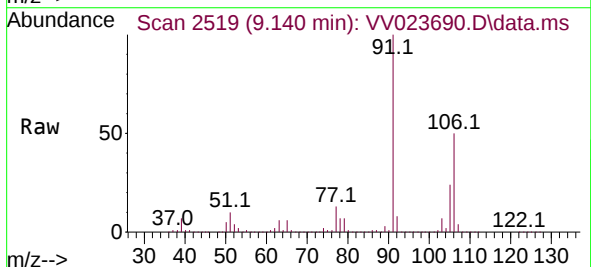




#54
o-xylene
Concen: 5.913 ug/L
RT: 9.541 min Scan# 2644
Delta R.T. -0.000 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion:106 Resp: 109560
Ion Ratio Lower Upper
106 100
91 214.7 147.9 274.7



#55
Styrene
Concen: 0.250 ug/L
RT: 9.541 min Scan# 2644
Delta R.T. -0.019 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52

Tgt Ion:104 Resp: 7794
Ion Ratio Lower Upper
104 100
78 280.2 31.0 57.6#

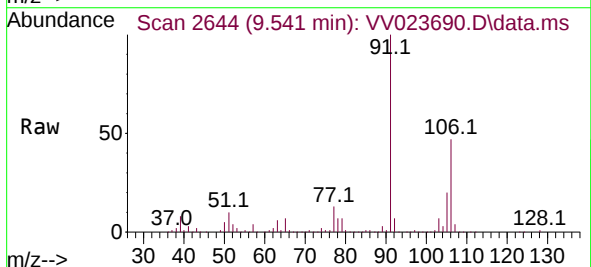



#57

1,1,2,2-Tetrachloroethane

Concen: 0.374 ug/L

RT: 10.242 min Scan# 2862

Delta R.T. -0.000 min

Lab File: VV023690.D

Acq: 23 Nov 2021 22:52

Instrument :

MSVOA_V

ClientSampleId :





Tgt Ion: 83 Resp: 2958

Ion Ratio Lower Upper

83 100

85 24.7 44.6 82.8#

131 6.5 8.3 12.5#

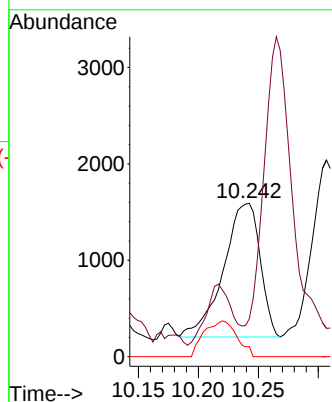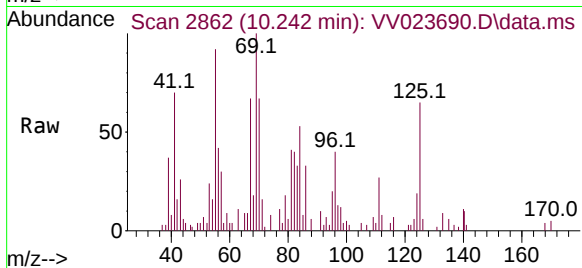

#60

Isopropylbenzene

Concen: 12.217 ug/L

RT: 9.931 min Scan# 2765

Delta R.T. -0.000 min

Lab File: VV023690.D

Acq: 23 Nov 2021 22:52




Tgt Ion: 105 Resp: 611566


Ion Ratio Lower Upper

105 100

120 26.9 21.4 32.0

77 15.2 12.2 18.4


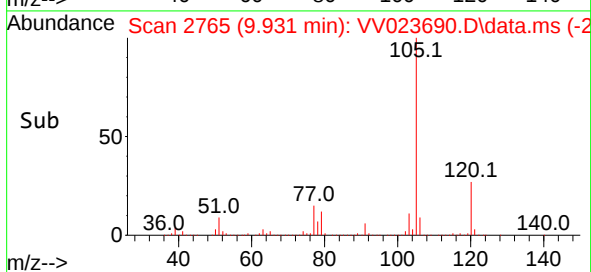
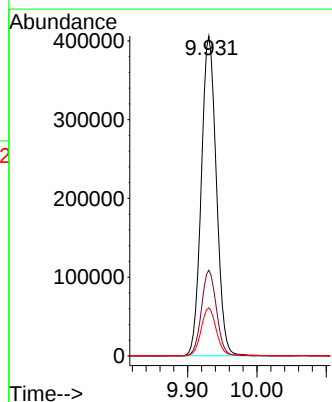
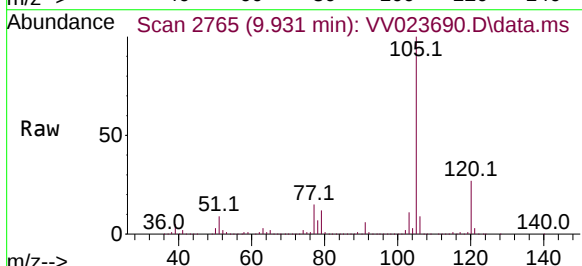




#61
1,2,3-Trichloropropane
Concen: 1.225 ug/L
RT: 10.352 min Scan# 2871
Delta R.T. 0.080 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 75 Resp: 7283
Ion Ratio Lower Upper
75 100
77 569.2 26.4 39.6#
110 13.3 34.2 51.2#



#62
1,3,5-Trimethylbenzene
Concen: 4.850 ug/L
RT: 10.538 min Scan# 2954
Delta R.T. -0.000 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52

Tgt Ion: 105 Resp: 202025
Ion Ratio Lower Upper
105 100
120 50.5 40.1 60.1

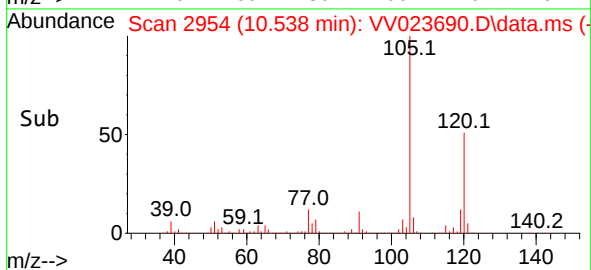

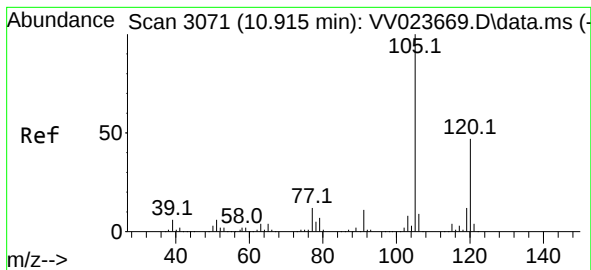

#63

1,2,4-Trimethylbenzene

Concen: 2.631 ug/L

RT: 10.914 min Scan# 3071

Delta R.T. -0.000 min

Lab File: VV023690.D

Acq: 23 Nov 2021 22:52

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion:105 Resp: 108379

Ion Ratio Lower Upper

105 100

120 46.3 36.7 55.1

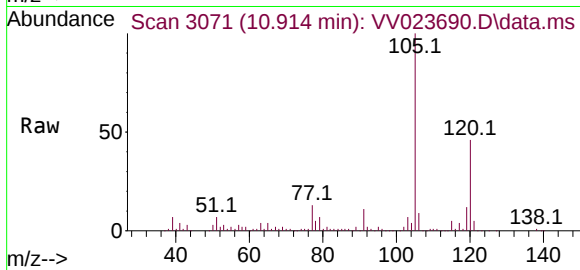

#67

1,2-Dichlorobenzene

Concen: 0.118 ug/L

RT: 11.644 min Scan# 3298

Delta R.T. -0.000 min

Lab File: VV023690.D

Acq: 23 Nov 2021 22:52




Tgt Ion:146 Resp: 2763


Ion Ratio Lower Upper

146 100

111 78.4 31.9 47.9#

148 63.8 50.5 75.7



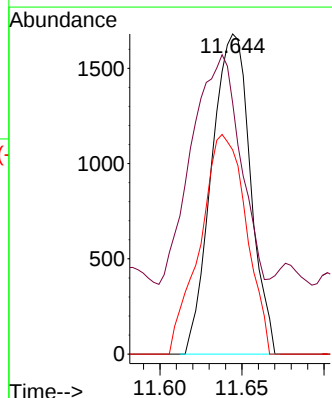
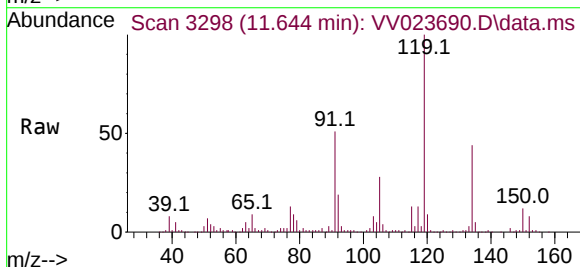




#68
1,2-Dibromo-3-chloropropane
Concen: 5.928 ug/L
RT: 12.410 min Scan# 3536
Delta R.T. -0.016 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 6999
Ion Ratio Lower Upper
75 100
155 0.0 71.7 107.5#
157 0.0 103.3 154.9#

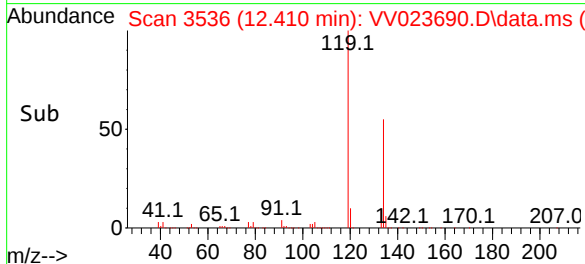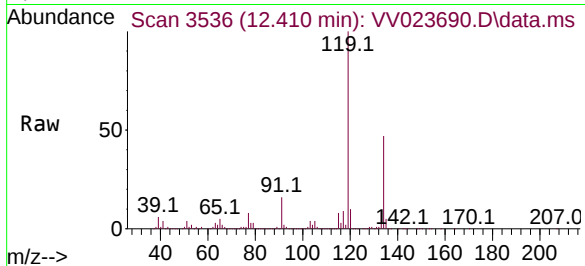

#71
Naphthalene
Concen: 1.406 ug/L
RT: 13.487 min Scan# 3871
Delta R.T. -0.016 min
Lab File: VV023690.D
Acq: 23 Nov 2021 22:52

Tgt Ion: 128 Resp: 29337
Ion Ratio Lower Upper
128 100
129 59.1 9.0 13.4#
127 25.8 10.2 15.4#

