


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
Data File : VV023672.D
Acq On : 23 Nov 2021 15:44
Operator : SY/MD
Sample : M4723-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G06

Manual IntegrationsAPPROVED

Quant Time: Nov 24 04:59:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 04:42:45 2021
Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021
Supervised By :Mahesh Dadoda 11/26/2021

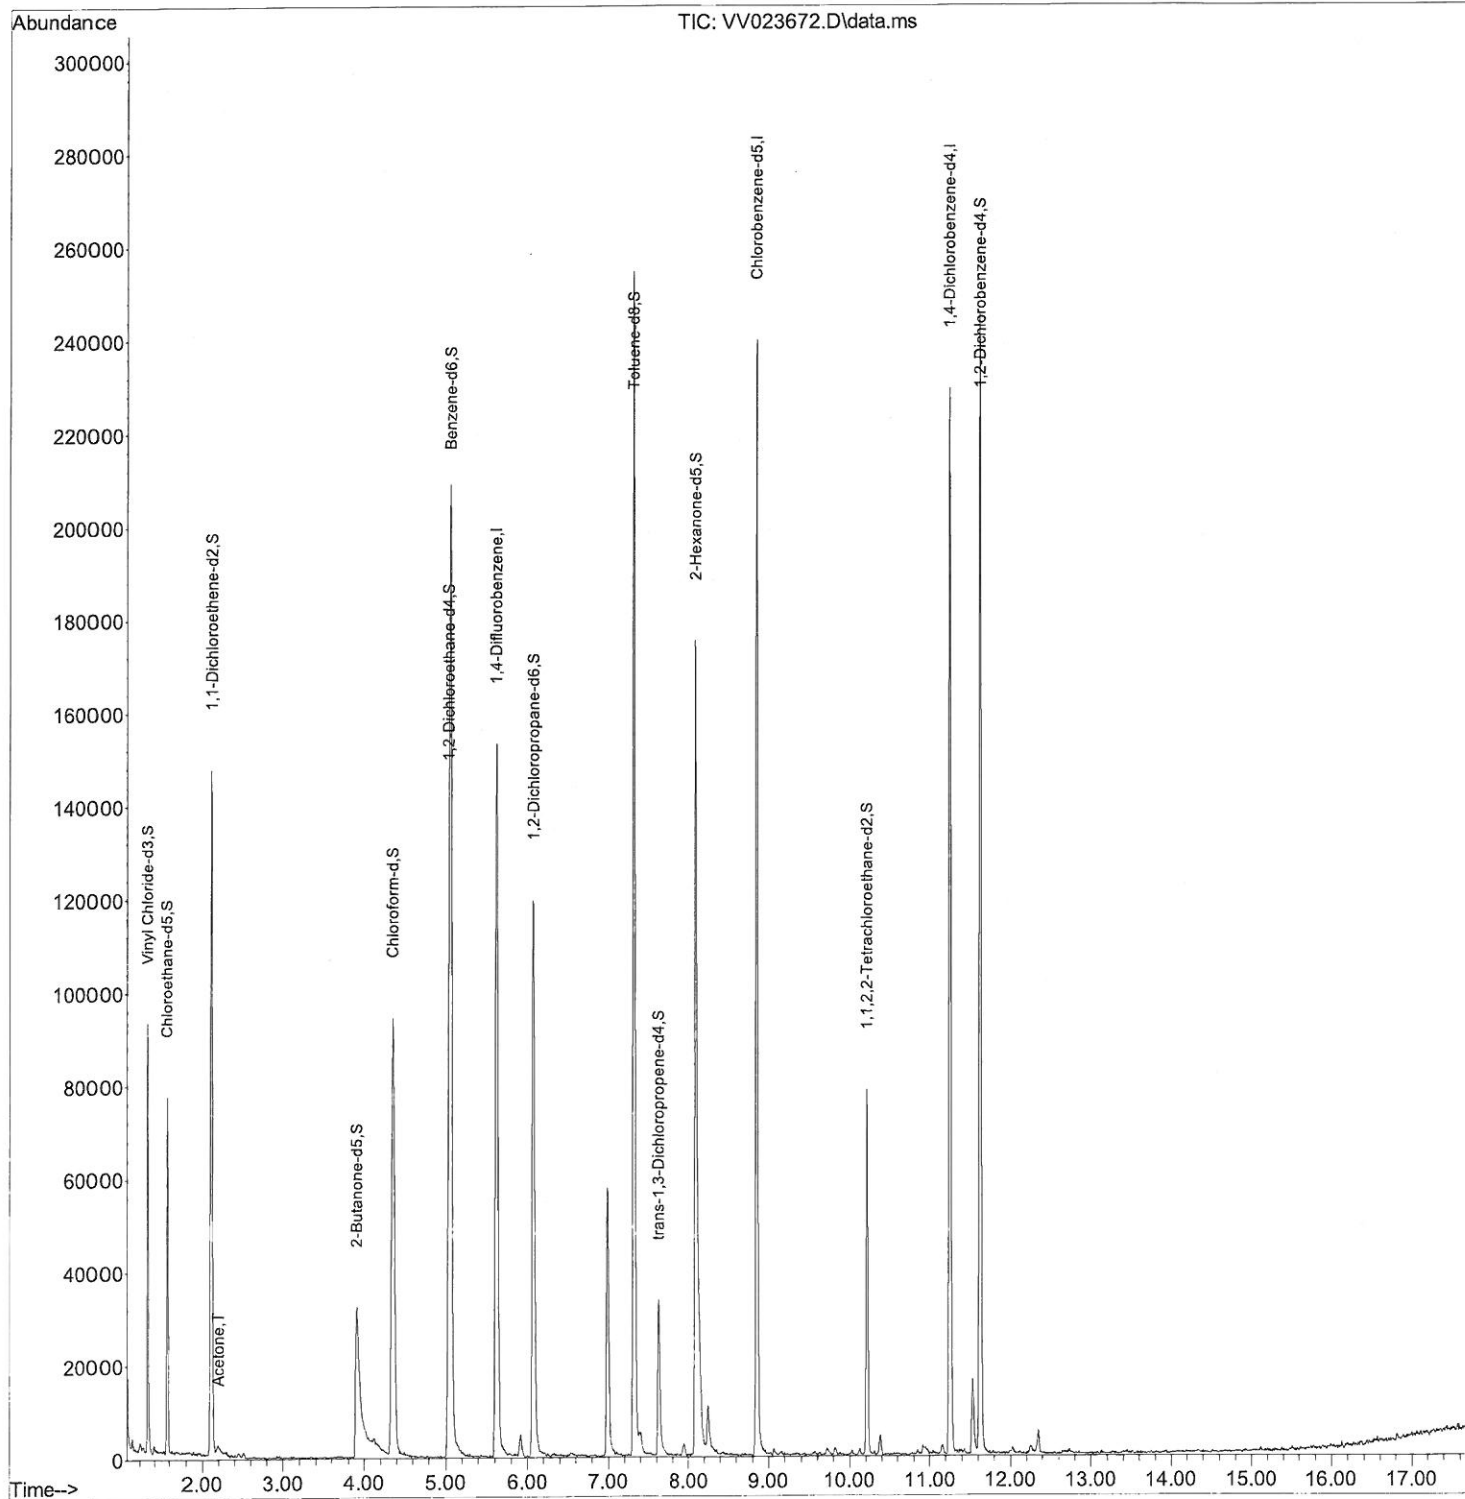

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
Data File : VV023672.D
Acq On : 23 Nov 2021 15:44
Operator : SY/MD
Sample : M4723-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G06

Manual IntegrationsAPPROVED

Quant Time: Nov 24 04:59:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 04:42:45 2021
Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021
Supervised By :Mahesh Dadoda 11/26/2021

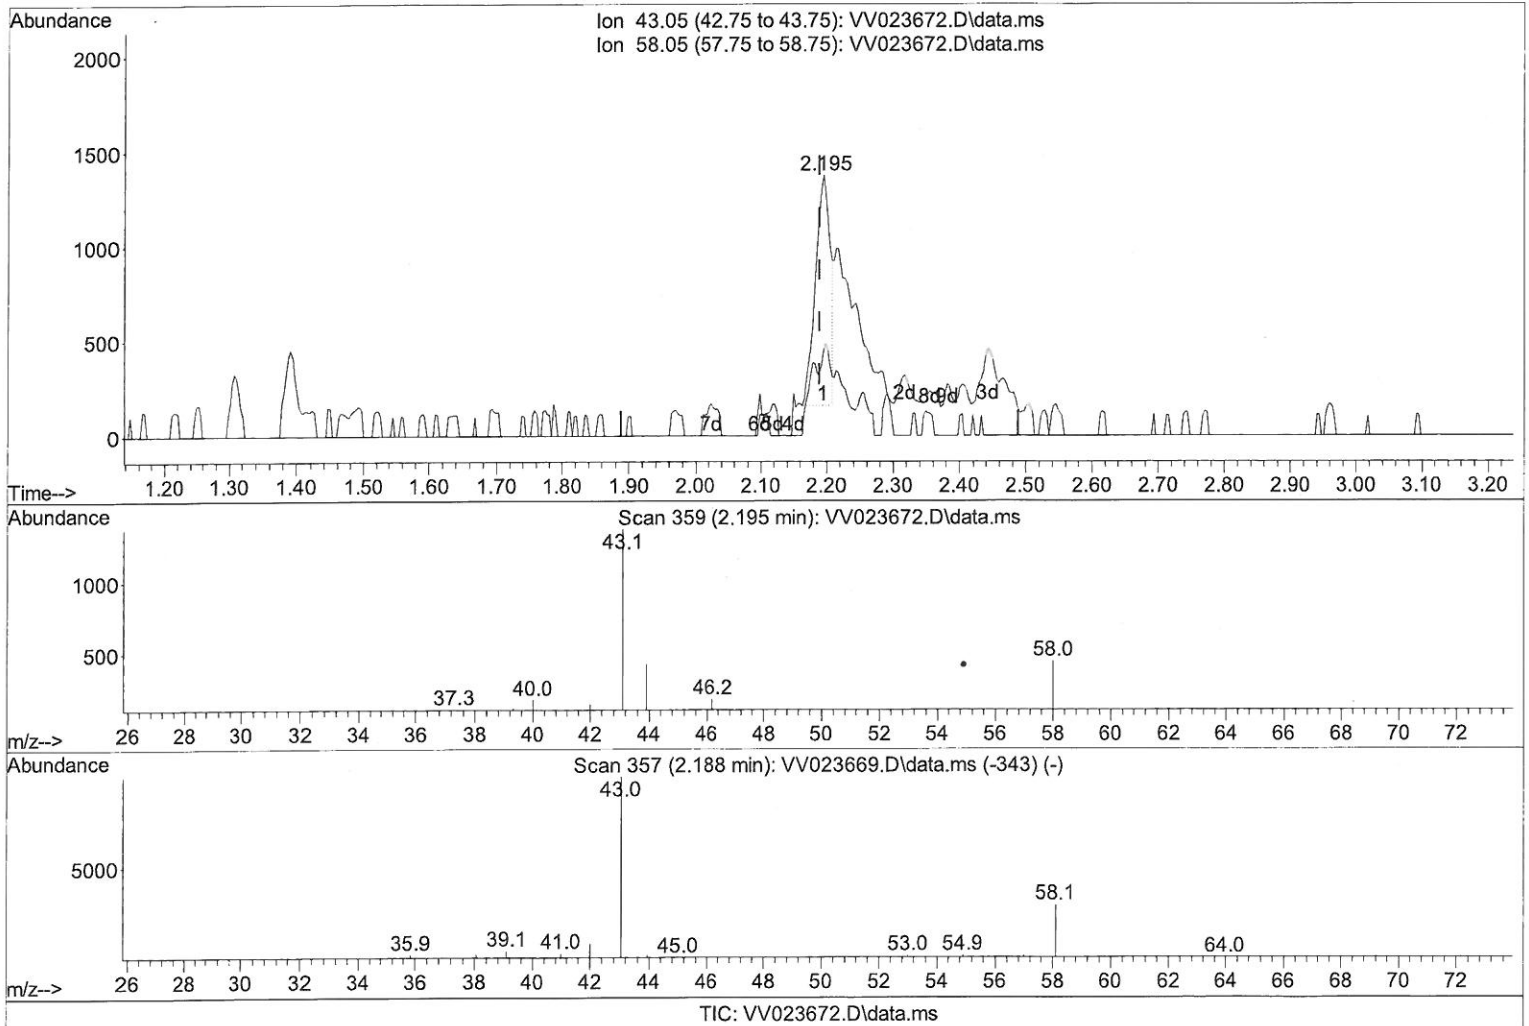

(13) Acetone (T)

2.195min (+ 0.006) 1.55 ug/L

response 1871

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	11.22
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
 Data File : VV023672.D
 Acq On : 23 Nov 2021 15:44
 Operator : SY/MD
 Sample : M4723-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G06

Manual IntegrationsAPPROVED

Quant Time: Nov 24 04:59:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 04:42:45 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021
 Supervised By :Mahesh Dadoda 11/26/2021

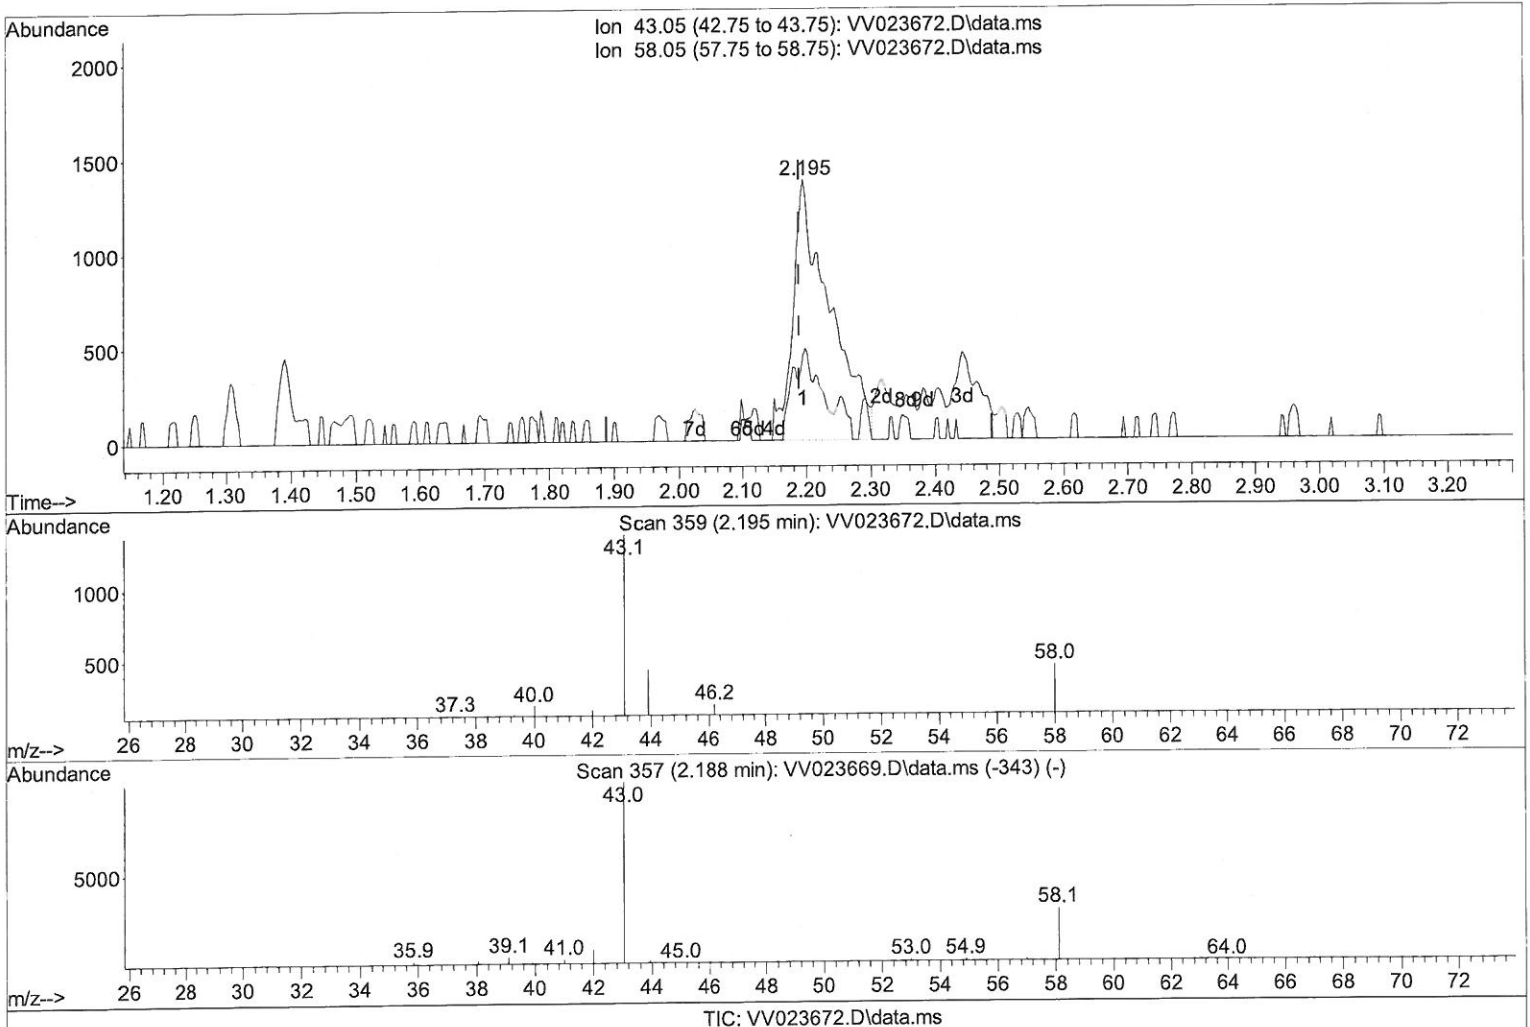

(13) Acetone (T)

2.195min (+ 0.006) 4.39 ug/L m *MD*
12/01/21

response 5302

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	3.96
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112321\
 Data File : VW023672.D
 Acq On : 23 Nov 2021 15:44
 Operator : SY/MD
 Sample : M4723-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G06

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 11/24/2021
 Supervised By : Mahesh Dadoda 11/26/2021

Quant Time: Nov 24 04:59:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 04:42:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	136050	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	136154	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63893	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	55418	4.962	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	99.200%		
7) Chloroethane-d5	1.568	69	44399	5.057	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	101.200%		
11) 1,1-Dichloroethene-d2	2.108	63	76711	3.897	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	78.000%		
20) 2-Butanone-d5	3.905	46	76774	57.181	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	114.360%		
24) Chloroform-d	4.349	84	98600	5.070	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	101.400%		
26) 1,2-Dichloroethane-d4	5.034	65	47529	5.231	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	104.600%		
32) Benzene-d6	5.053	84	193018	5.204	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	104.000%		
36) 1,2-Dichloropropane-d6	6.069	67	55886	5.375	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	107.400%		
41) Toluene-d8	7.317	98	169152	4.881	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	97.600%		
43) trans-1,3-Dichloroprop...	7.625	79	20319	4.848	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	97.000%		
46) 2-Hexanone-d5	8.092	63	65548	47.071	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	94.140%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	35709	4.772	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	95.400%		
66) 1,2-Dichlorobenzene-d4	11.625	152	65632	5.810	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	116.200%		
Target Compounds						
13) Acetone	2.195	43	5302m	4.389	ug/L	Qvalue

> $\frac{mD}{12/01/24}$

(#) = qualifier out of range (m) = manual integration (+) = signals summed