


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112321\  
Data File : VV023674.D  
Acq On : 23 Nov 2021 16:31  
Operator : SY/MD  
Sample : M4723-06  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0G14

Manual IntegrationsAPPROVED

Quant Time: Nov 24 04:59:50 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Wed Nov 24 04:42:45 2021  
Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021  
Supervised By :Mahesh Dadoda 11/26/2021

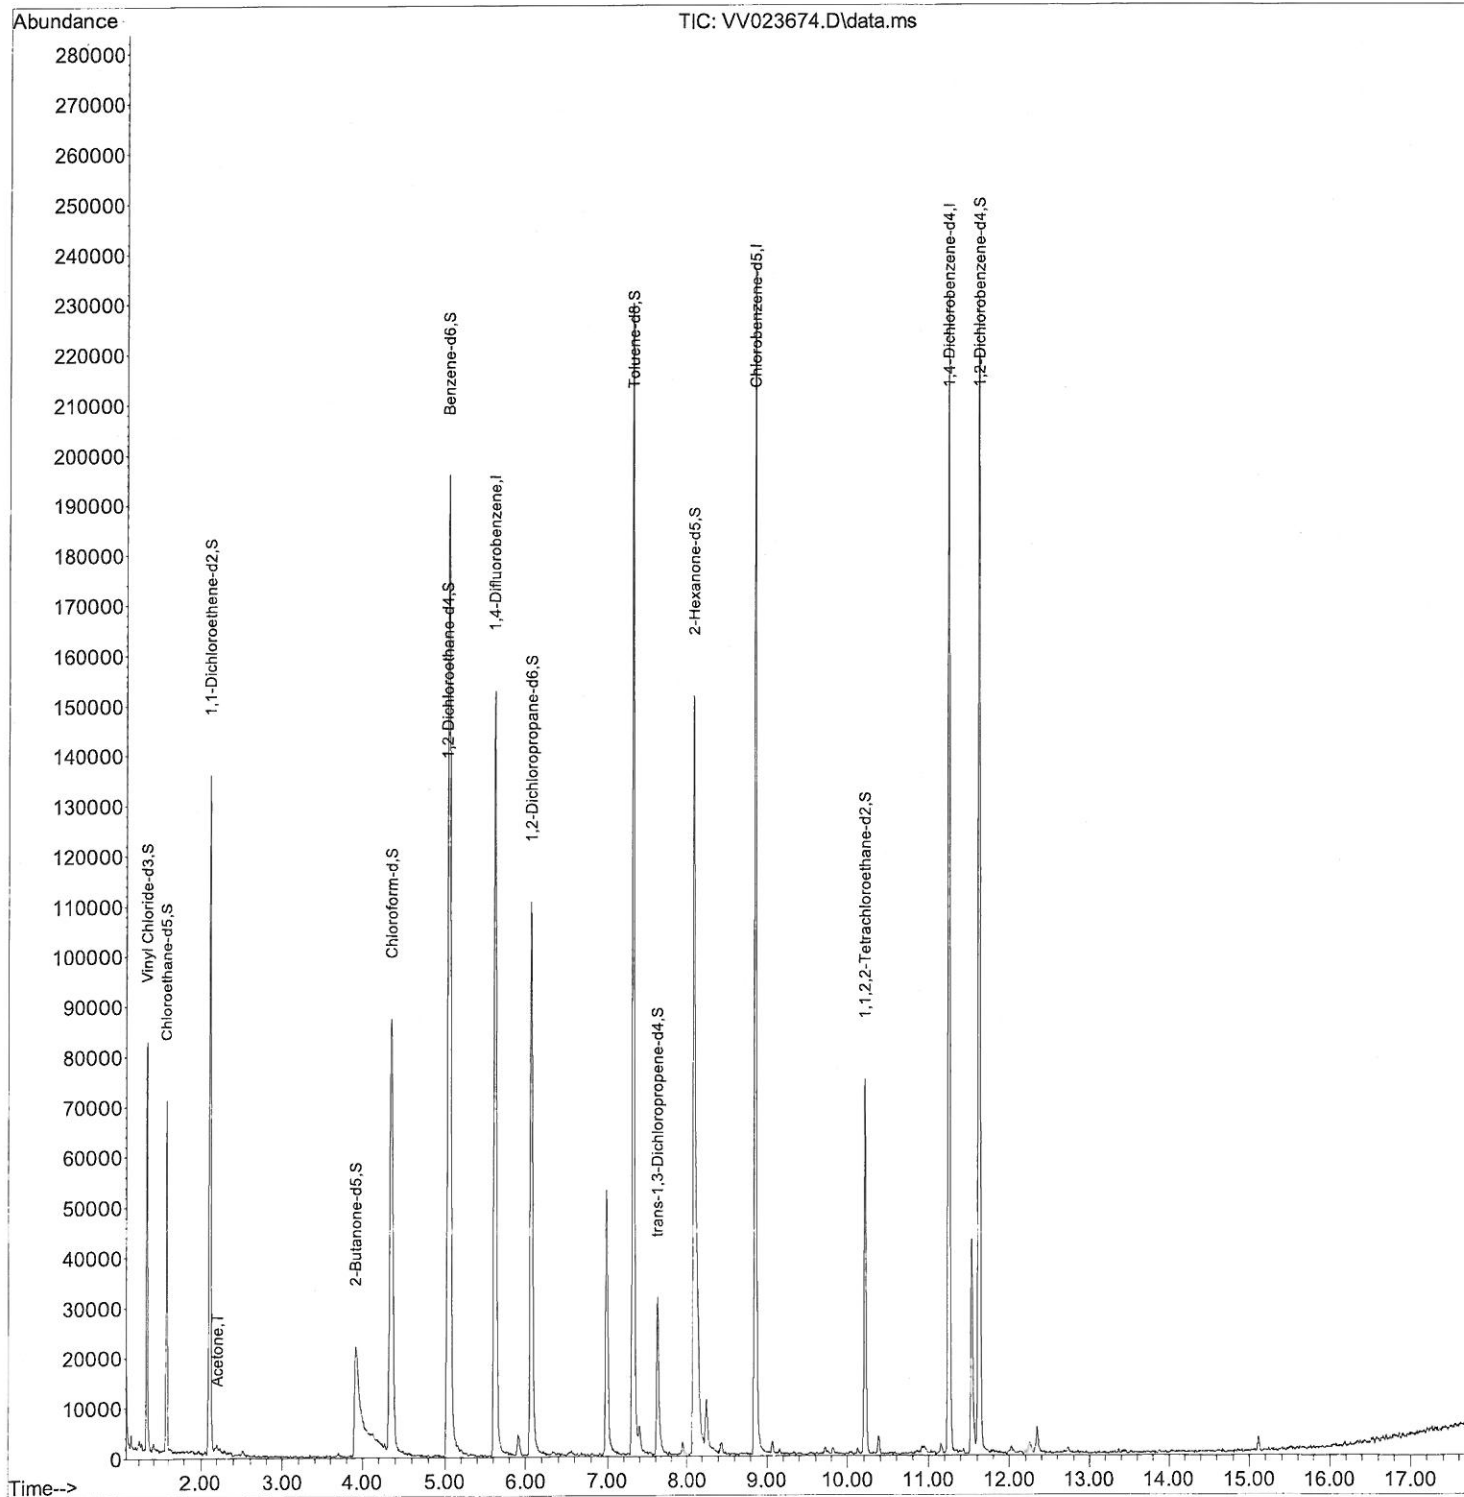

# Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112321\  
 Data File : VV023674.D  
 Acq On : 23 Nov 2021 16:31  
 Operator : SY/MD  
 Sample : M4723-06  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0G14

Manual IntegrationsAPPROVED

Quant Time: Nov 24 04:59:50 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Wed Nov 24 04:42:45 2021  
 Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021  
 Supervised By :Mahesh Dadoda 11/26/2021

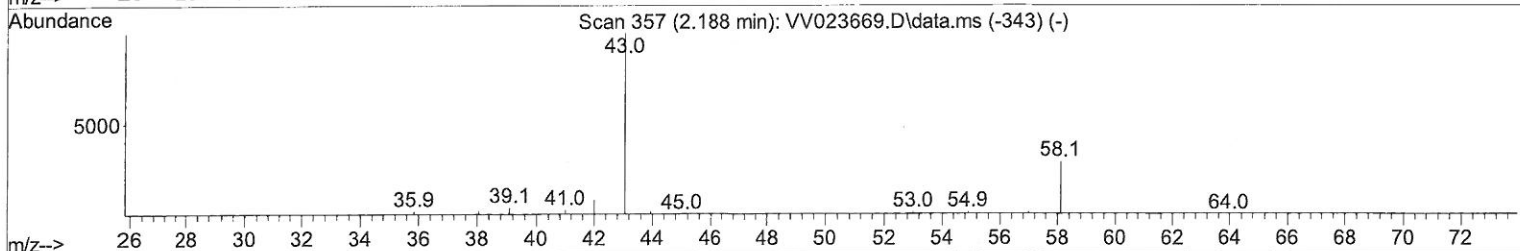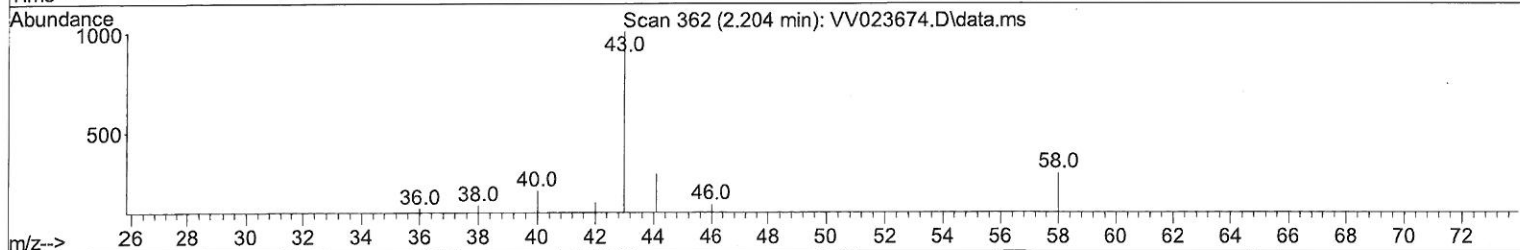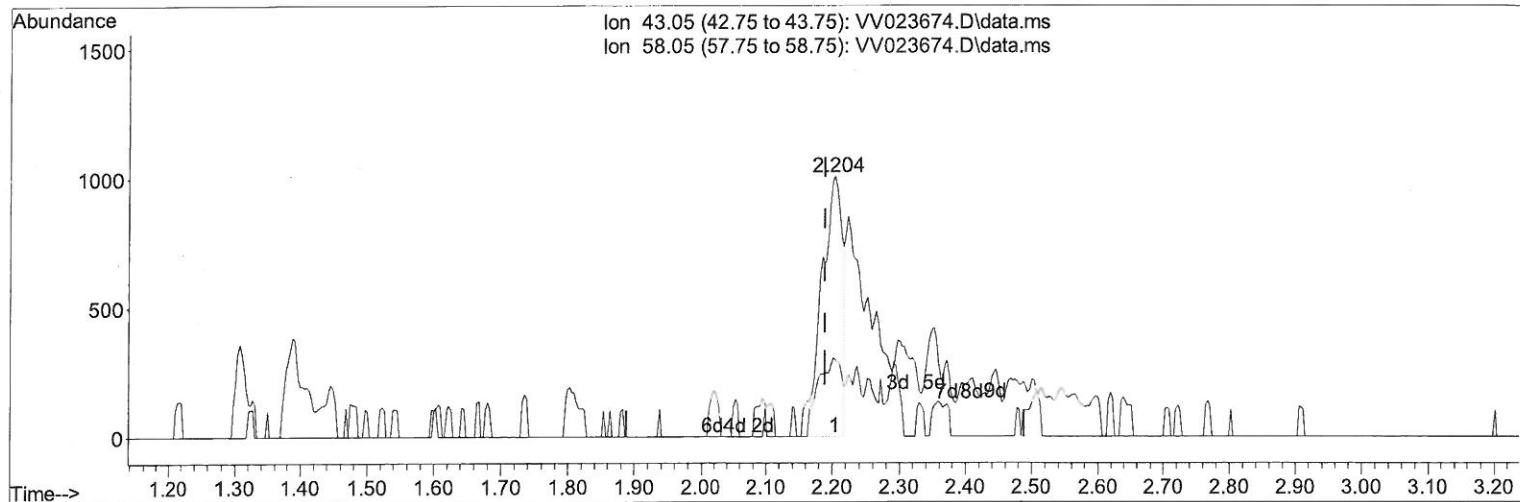

TIC: VV023674.D\data.ms

(13) Acetone (T)

2.204min (+ 0.016) 1.81 ug/L

response 2196

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	34.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112321\  
Data File : VV023674.D  
Acq On : 23 Nov 2021 16:31  
Operator : SY/MD  
Sample : M4723-06  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0G14

Manual IntegrationsAPPROVED

Quant Time: Nov 24 04:59:50 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Wed Nov 24 04:42:45 2021  
Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021  
Supervised By :Mahesh Dadoda 11/26/2021

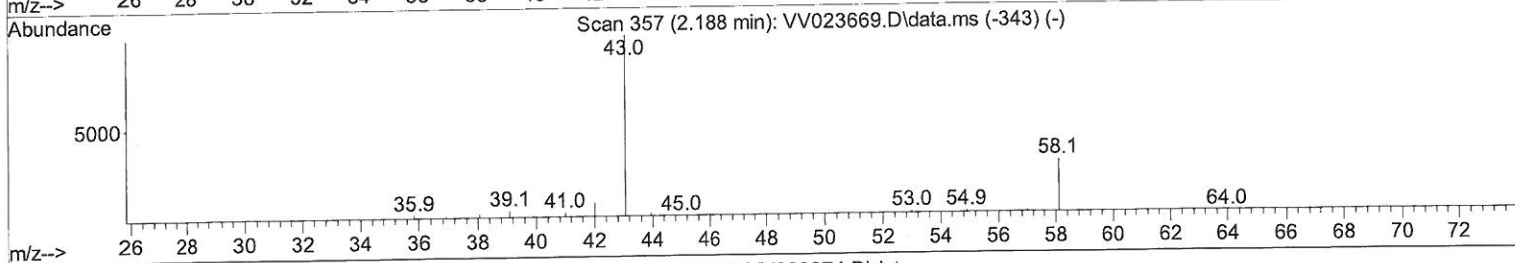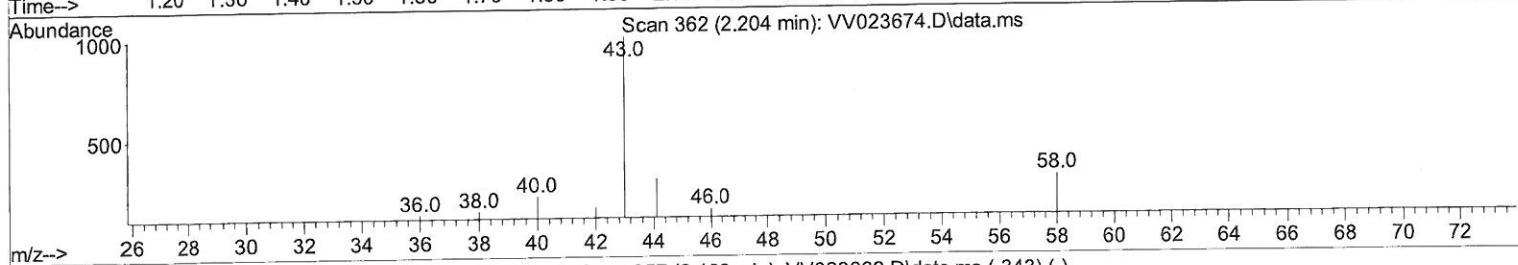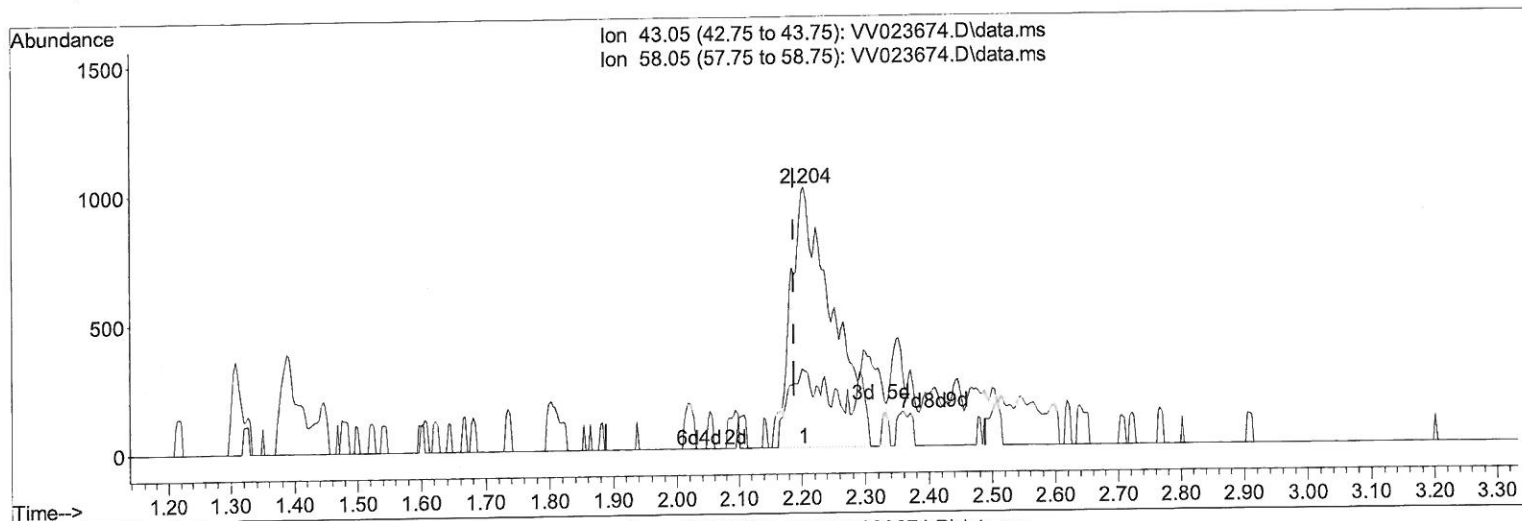

TIC: VV023674.D\data.ms

(13) Acetone (T)

2.204min (+ 0.016) 4.26 ug/L m

response 5176

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	14.53
0.00	0.00	0.00
0.00	0.00	0.00

7 MD  
12/01/21


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112321\  
Data File : VV023674.D  
Acq On : 23 Nov 2021 16:31  
Operator : SY/MD  
Sample : M4723-06  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0G14

Manual IntegrationsAPPROVED

Quant Time: Nov 24 04:59:50 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Wed Nov 24 04:42:45 2021  
Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021  
Supervised By :Mahesh Dadoda 11/26/2021

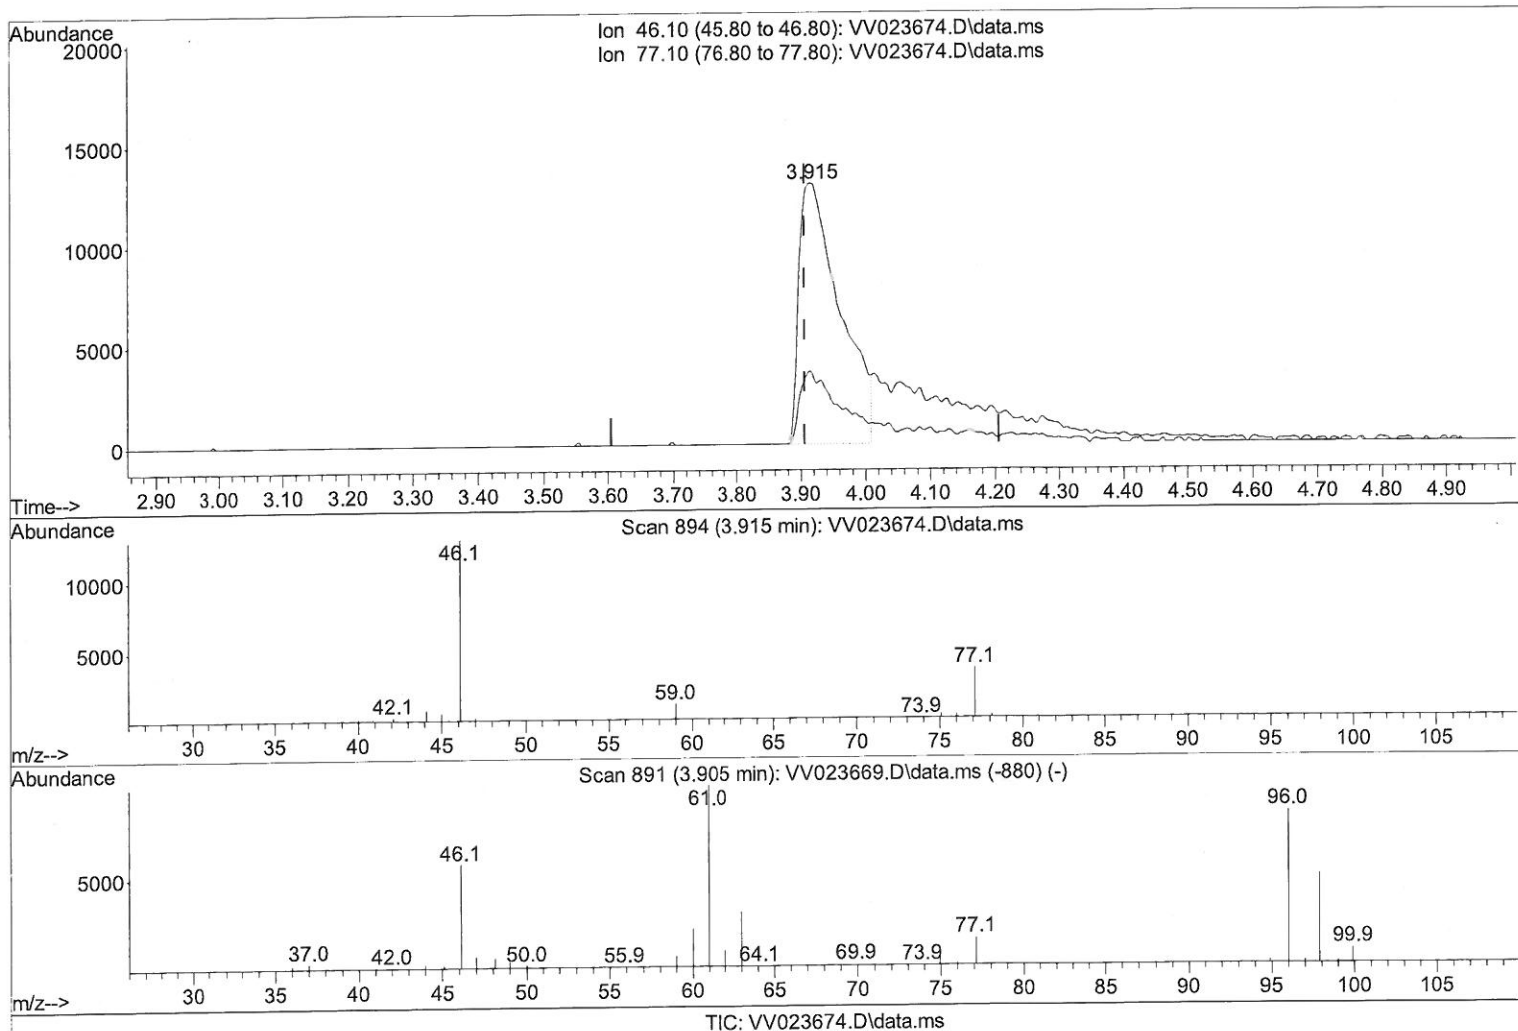

(20) 2-Butanone-d5 (S)

3.915min (+ 0.010) 42.18 ug/L

response 56893

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	10.85
0.00	0.00	0.00
0.00	0.00	0.00



# Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112321\  
 Data File : VV023674.D  
 Acq On : 23 Nov 2021 16:31  
 Operator : SY/MD  
 Sample : M4723-06  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0G14

Manual IntegrationsAPPROVED

Quant Time: Nov 24 04:59:50 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Wed Nov 24 04:42:45 2021  
 Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021  
 Supervised By :Mahesh Dadoda 11/26/2021

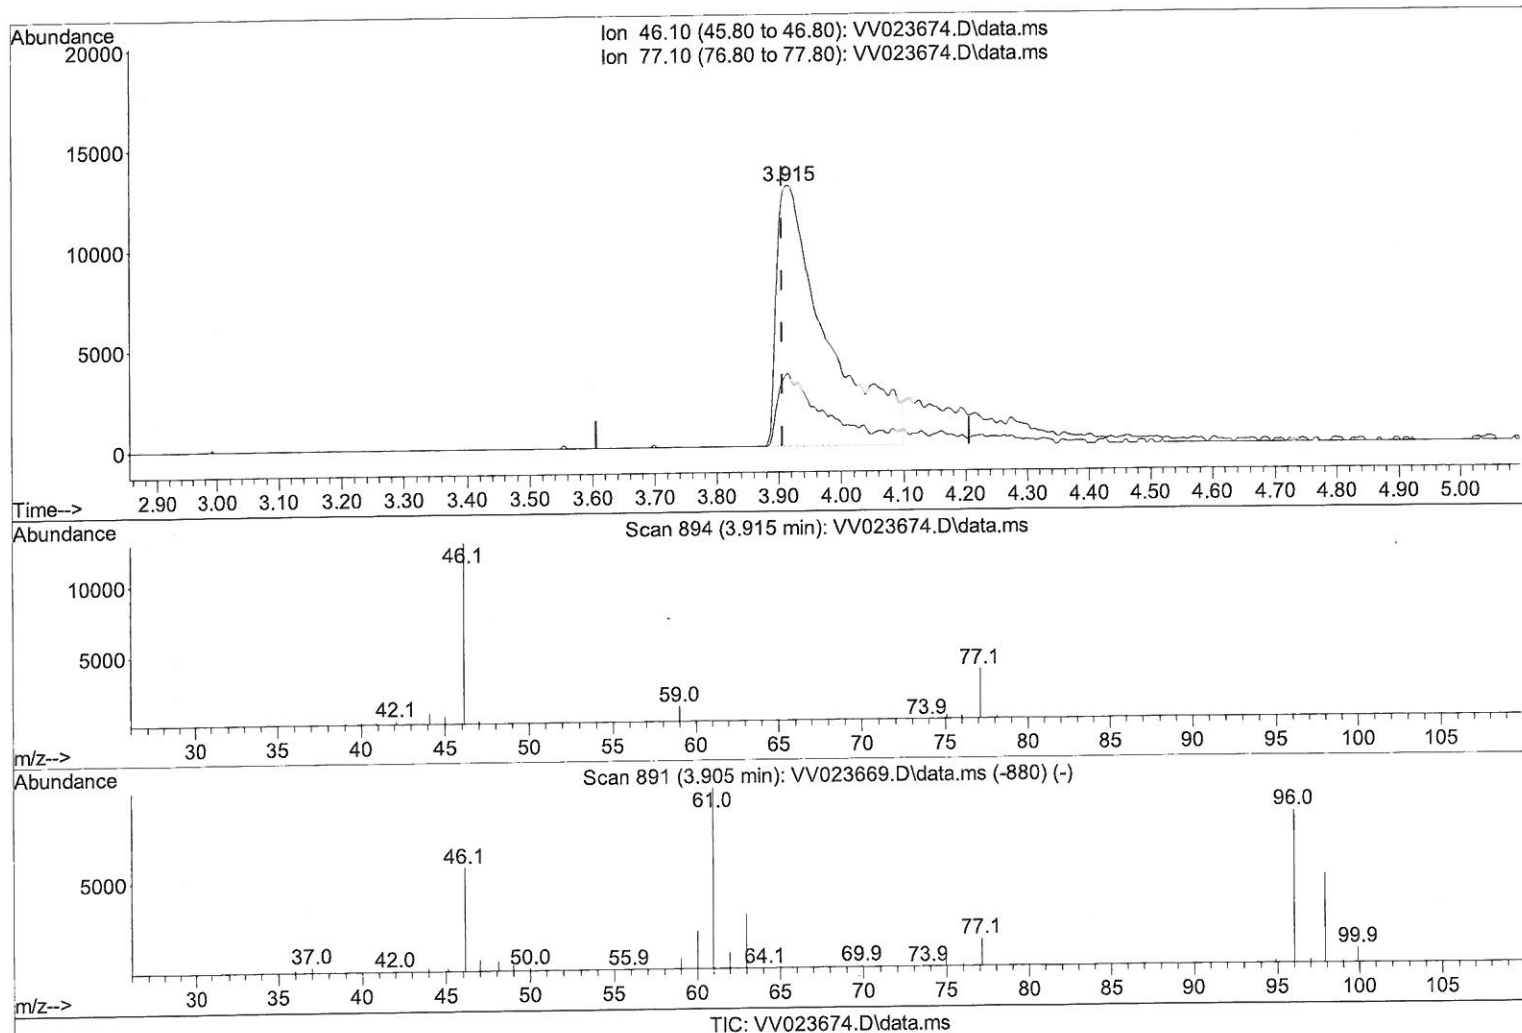

(20) 2-Butanone-d5 (S)

3.915min (+ 0.010) 53.31 ug/L m

response 71897

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	8.59
0.00	0.00	0.00
0.00	0.00	0.00

*Handwritten:* 7 MD  
12/01/24

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112321\  
 Data File : VV023674.D  
 Acq On : 23 Nov 2021 16:31  
 Operator : SY/MD  
 Sample : M4723-06  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0G14

## Manual Integrations APPROVED

Reviewed By : John Carlone 11/24/2021  
 Supervised By : Mahesh Dadoda 11/26/2021

Quant Time: Nov 24 04:59:50 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Wed Nov 24 04:42:45 2021  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	136672	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	136208	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63744	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	50876	4.535	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.600%	
7) Chloroethane-d5	1.568	69	41538	4.710	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.200%	
11) 1,1-Dichloroethene-d2	2.108	63	71101	3.596	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.000%	
20) 2-Butanone-d5	3.915	46	71897m	53.305	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	106.620%	
24) Chloroform-d	4.352	84	92027	4.710	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.200%	
26) 1,2-Dichloroethane-d4	5.034	65	44223	4.845	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.000%	
32) Benzene-d6	5.050	84	180908	4.876	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.600%	
36) 1,2-Dichloropropane-d6	6.069	67	51261	4.928	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.600%	
41) Toluene-d8	7.317	98	155178	4.476	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.600%	
43) trans-1,3-Dichloroprop...	7.625	79	18638	4.445	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.000%	
46) 2-Hexanone-d5	8.091	63	63721	45.741	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	91.480%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34060	4.550	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	61798	5.484	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	109.600%	
Target Compounds						
13) Acetone	2.204	43	5176m	4.265	ug/L	Qvalue

SMD  
12/01/21

SMD  
12/01/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed