

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112321\  
Data File : VV023675.D  
Acq On : 23 Nov 2021 16:55  
Operator : SY/MD  
Sample : M4723-07  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 15 Sample Multiplier: 1


Instrument :  
MSVOA\_V  
ClientSampleId :  
C0G15

Manual IntegrationsAPPROVED

Quant Time: Nov 24 05:00:03 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Wed Nov 24 04:42:45 2021  
Response via : Initial Calibration

Reviewed By :John  
Carlone

11/24/2021  
Supervised By :Mahesh  
Dadoda

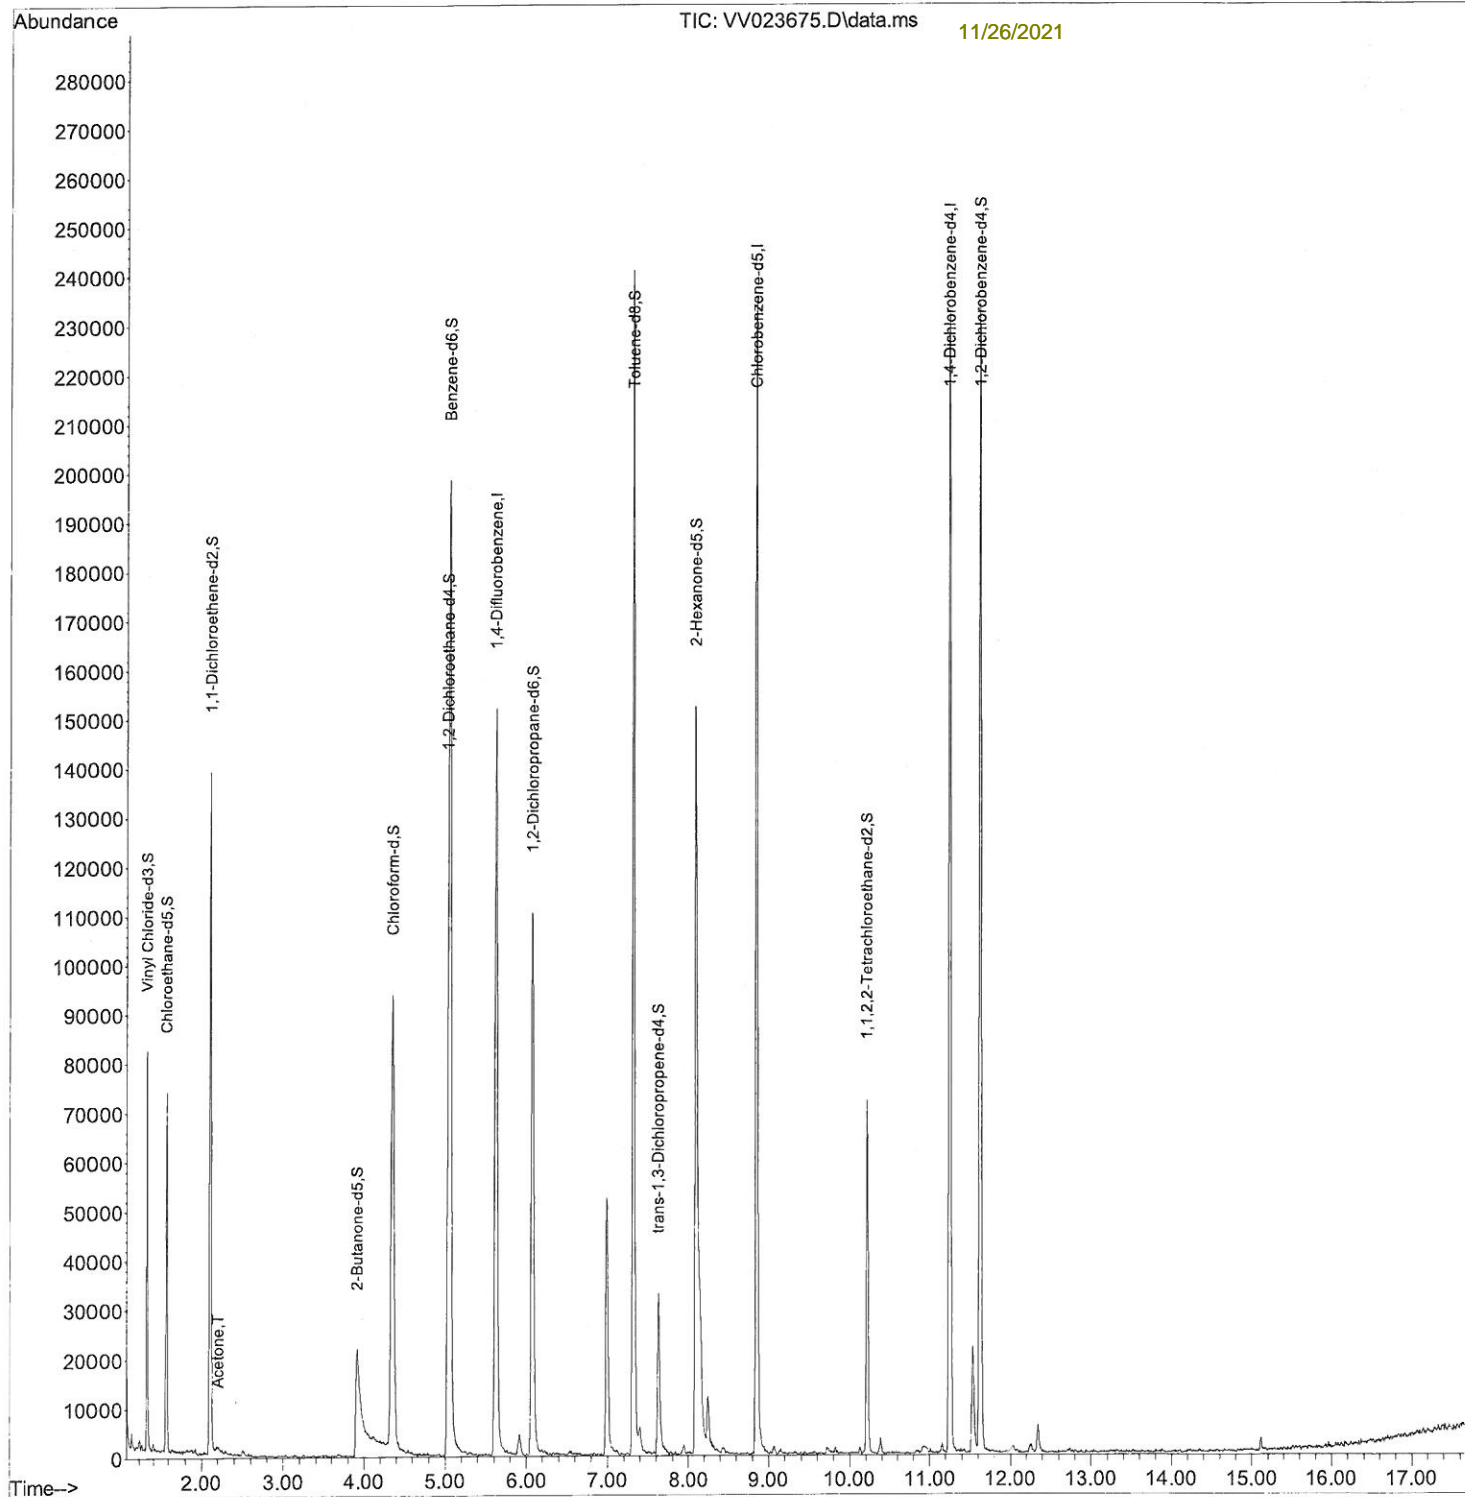

# Quantitation Report (Qedit)

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112321\  
 Data File : VV023675.D  
 Acq On : 23 Nov 2021 16:55  
 Operator : SY/MD  
 Sample : M4723-07  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 15 Sample Multiplier: 1




Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0G15

Manual IntegrationsAPPROVED

Quant Time: Nov 24 05:00:03 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Wed Nov 24 04:42:45 2021  
 Response via : Initial Calibration

Reviewed By :John  
 Carlone

11/24/2021  
 Supervised By :Mahesh  
 Dadoda

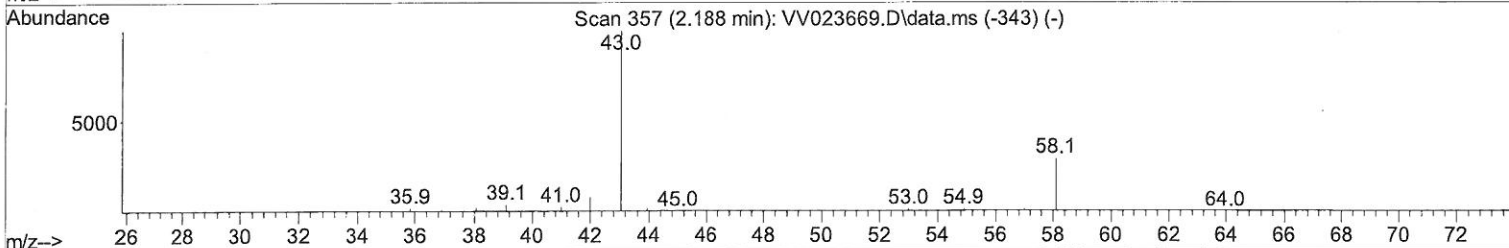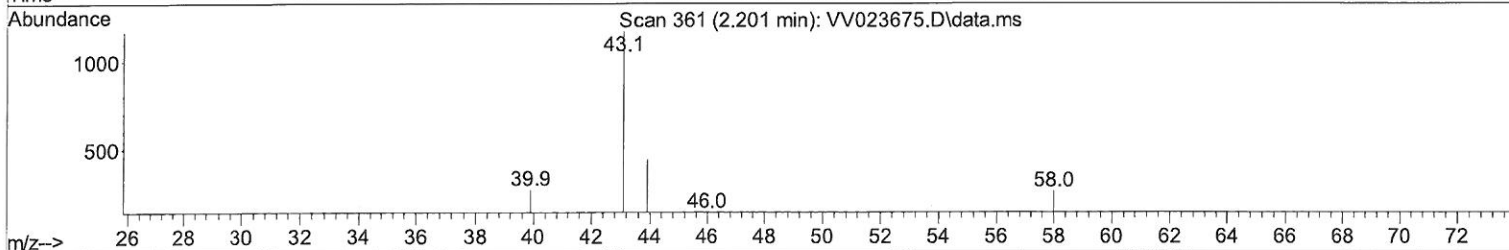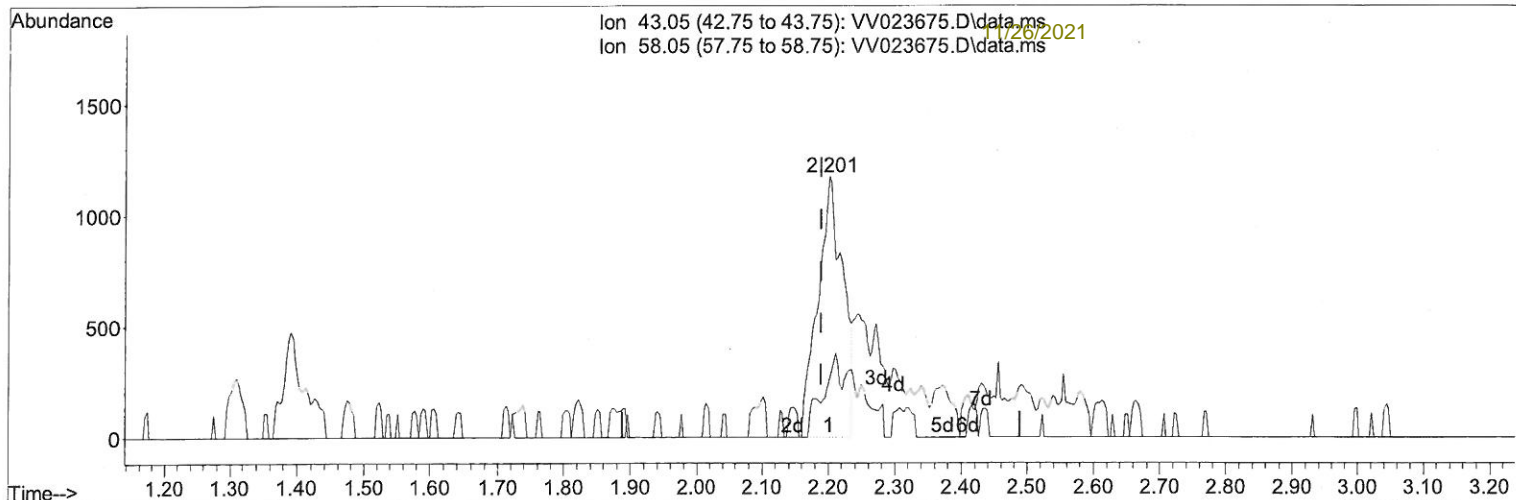

TIC: VV023675.D\data.ms

(13) Acetone (T)

2.201min (+ 0.013) 2.54 ug/L

response 3039

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	13.95
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112321\  
Data File : VV023675.D  
Acq On : 23 Nov 2021 16:55  
Operator : SY/MD  
Sample : M4723-07  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 15 Sample Multiplier: 1




Instrument :  
MSVOA\_V  
Client Sample Id :  
C0G15

Manual Integrations APPROVED

Quant Time: Nov 24 05:00:03 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Wed Nov 24 04:42:45 2021  
Response via : Initial Calibration

Reviewed By : John  
Carlone

11/24/2021  
Supervised By : Mahesh  
Dadoda

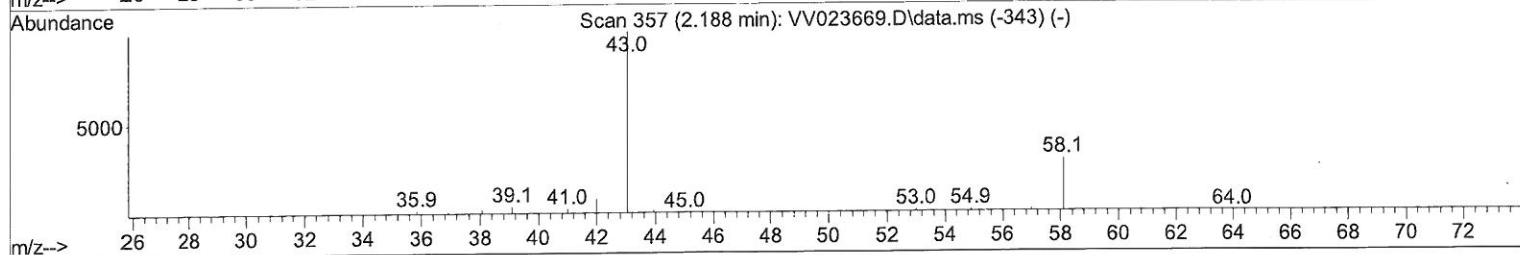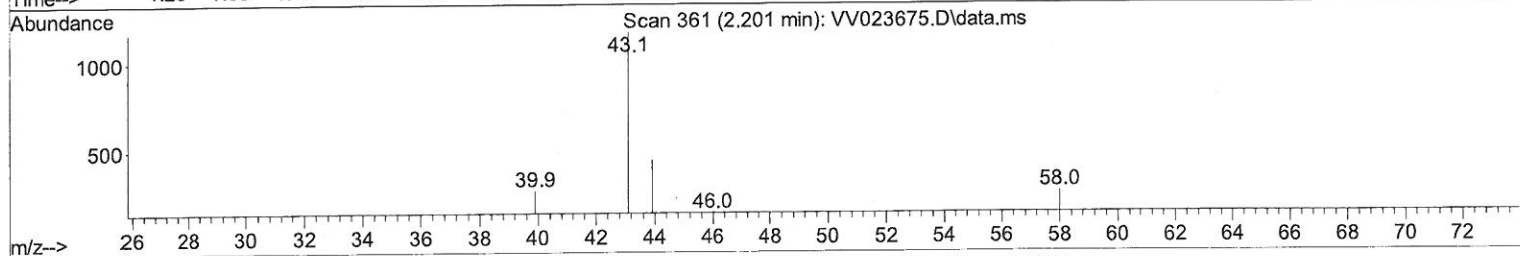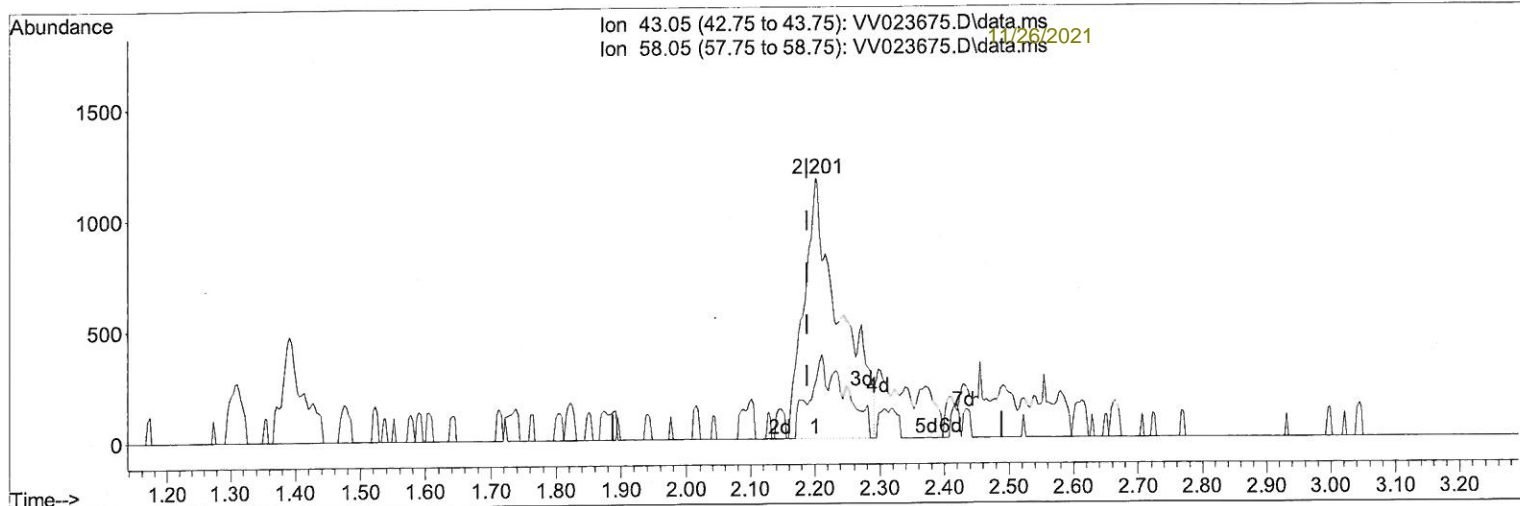

TIC: VV023675.D\data.ms

(13) Acetone (T)

2.201min (+ 0.013) 3.78 ug/L m

response 4529

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	9.36
0.00	0.00	0.00
0.00	0.00	0.00

7 MD  
12/01/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW112321\  
 Data File : VW023675.D  
 Acq On : 23 Nov 2021 16:55  
 Operator : SY/MD  
 Sample : M4723-07  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0G15

## Manual IntegrationsAPPROVED

Quant Time: Nov 24 05:00:03 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Wed Nov 24 04:42:45 2021  
 Response via : Initial Calibration

Reviewed By : John  
 Carlone

11/24/2021  
 Supervised By : Mahesh  
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	134841	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	135532	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63887	5.000	ug/L	0.00

## System Monitoring Compounds

4) Vinyl Chloride-d3	1.307	65	51616	4.663	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.200%	
7) Chloroethane-d5	1.568	69	42078	4.836	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.800%	
11) 1,1-Dichloroethene-d2	2.108	63	71123	3.646	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	73.000%	
20) 2-Butanone-d5	3.912	46	59087	44.403	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	88.800%	
24) Chloroform-d	4.352	84	94193	4.887	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.800%	
26) 1,2-Dichloroethane-d4	5.034	65	43822	4.866	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.400%	
32) Benzene-d6	5.050	84	180806	4.897	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.000%	
36) 1,2-Dichloropropane-d6	6.069	67	51773	5.002	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.000%	
41) Toluene-d8	7.317	98	156731	4.543	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.800%	
43) trans-1,3-Dichloroprop...	7.625	79	20412	4.892	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	97.800%	
46) 2-Hexanone-d5	8.092	63	65046	46.925	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	93.860%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34194	4.591	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	61718	5.464	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	109.200%	

## Target Compounds

Compound	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	2.201	43	4529m	3.782	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed