

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112321\
 Data File : VW023671.D
 Acq On : 23 Nov 2021 15:20
 Operator : SY/MD
 Sample : M4723-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G01

Manual Integrations
 APPROVED

Reviewed By : John Carlone 11/24/2021
 Supervised By : Mahesh Dadoda 11/26/2021

Quant Time: Nov 24 04:59:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 04:42:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	136095	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	136121	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63856	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	53525	4.791	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	95.800%		
7) Chloroethane-d5	1.568	69	43695	4.976	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	99.600%		
11) 1,1-Dichloroethene-d2	2.108	63	76392	3.880	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	77.600%		
20) 2-Butanone-d5	3.905	46	62748m	46.719	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	93.440%		
24) Chloroform-d	4.349	84	94907	4.878	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.600%		
26) 1,2-Dichloroethane-d4	5.034	65	45064	4.958	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	99.200%		
32) Benzene-d6	5.053	84	185922	5.014	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	100.200%		
36) 1,2-Dichloropropane-d6	6.069	67	53183	5.116	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	102.400%		
41) Toluene-d8	7.317	98	167960	4.848	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	97.000%		
43) trans-1,3-Dichloroprop...	7.625	79	19350	4.618	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	92.400%		
46) 2-Hexanone-d5	8.092	63	63515	45.622	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	91.240%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34269	4.581	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	91.600%		
66) 1,2-Dichlorobenzene-d4	11.625	152	62927	5.574	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	111.400%		
Target Compounds					Qvalue	
13) Acetone	2.211	43	4057m	3.357	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
Data File : VV023671.D
Acq On : 23 Nov 2021 15:20
Operator : SY/MD
Sample : M4723-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0G01

Manual Integrations
APPROVED

Reviewed By : John Carlone 11/24/2021
Supervised By : Mahesh Dadoda 11/26/2021


Quant Time: Nov 24 04:59:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 04:42:45 2021
Response via : Initial Calibration

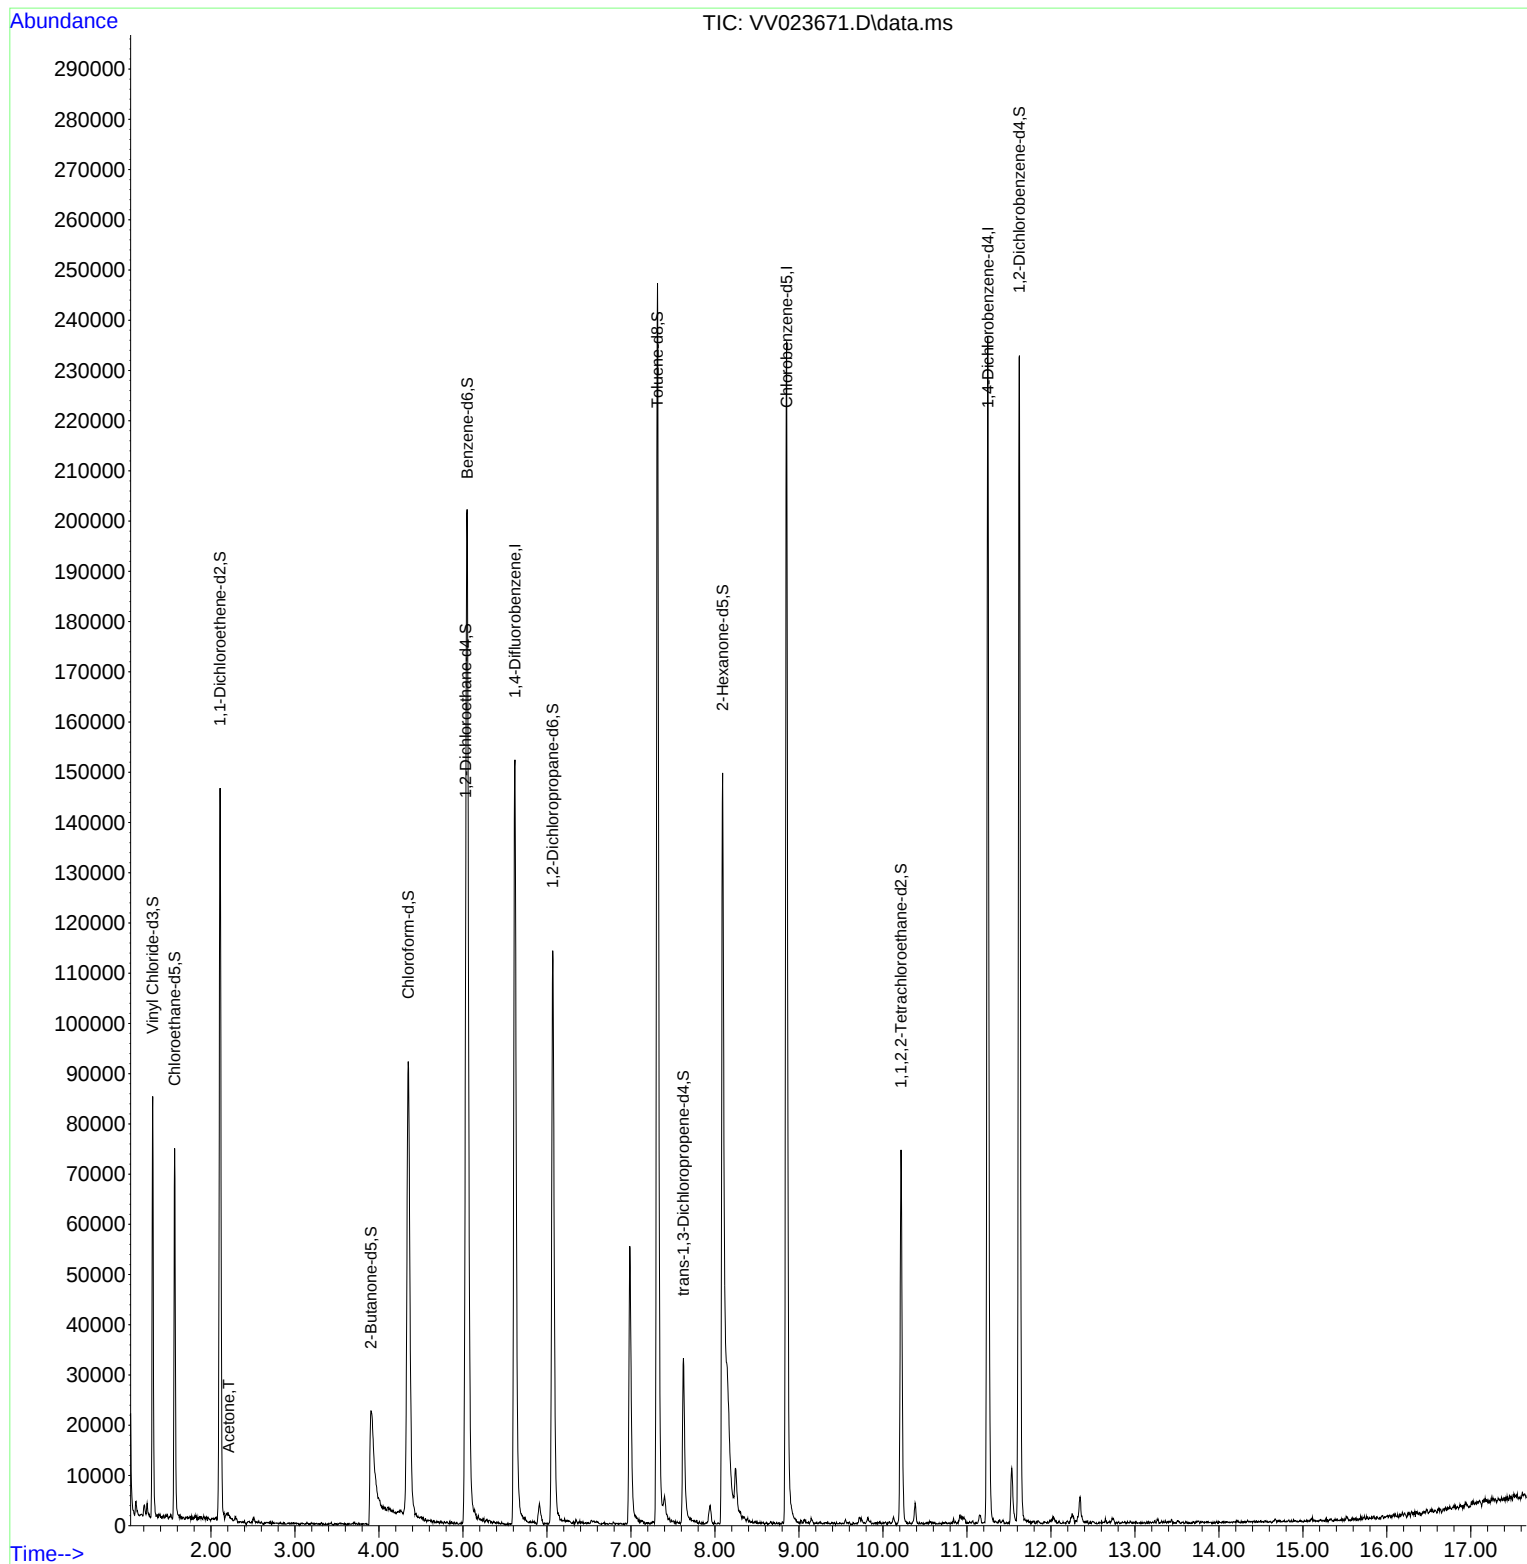

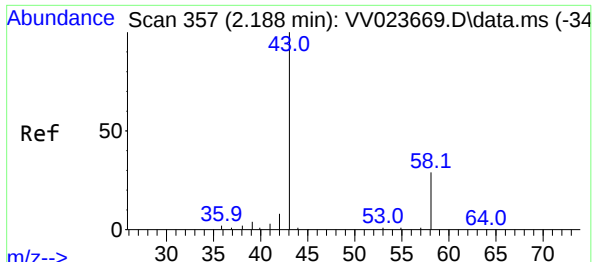

#13
Acetone
Concen: 3.357 ug/L m
RT: 2.211 min Scan# 30
Delta R.T. 0.023 min
Lab File: VV023671.D
Acq: 23 Nov 2021 15:20

Instrument :
MSVOA_V
ClientSampleId :
C0G01

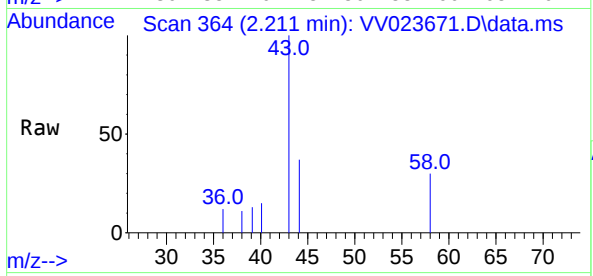

Tgt Ion: 43 Resp: 405
Ion Ratio Lower Upper
43 100
58 25.1 0.0 41.4

Manual Integrations
APPROVED

Reviewed By :John Carlone 11/24/2021
Supervised By :Mahesh Dadoda 11/26/2021

