

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112321\
 Data File : VW023673.D
 Acq On : 23 Nov 2021 16:08
 Operator : SY/MD
 Sample : M4723-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G07

Manual Integrations
 APPROVED

Reviewed By : John Carlone 11/24/2021
 Supervised By : Mahesh Dadoda 11/26/2021

Quant Time: Nov 24 04:59:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 04:42:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	144595	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	142558	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	67671	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	53796	4.532	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.600%
7) Chloroethane-d5	1.568	69	42756	4.582	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.600%
11) 1,1-Dichloroethene-d2	2.108	63	71692	3.427	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.600%
20) 2-Butanone-d5	3.905	46	65186	45.682	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.360%
24) Chloroform-d	4.352	84	93327	4.515	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%
26) 1,2-Dichloroethane-d4	5.034	65	45541	4.716	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
32) Benzene-d6	5.050	84	179261	4.616	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
36) 1,2-Dichloropropane-d6	6.072	67	52215	4.796	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	7.317	98	160947	4.436	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.800%
43) trans-1,3-Dichloroprop...	7.622	79	19596	4.465	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.400%
46) 2-Hexanone-d5	8.092	63	64621	44.321	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.640%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34534	4.408	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	61429	5.134	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.600%
Target Compounds					Qvalue	
13) Acetone	2.192	43	5528m	4.305	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
Data File : VV023673.D
Acq On : 23 Nov 2021 16:08
Operator : SY/MD
Sample : M4723-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0G07

Quant Time: Nov 24 04:59:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 04:42:45 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :John Carlone 11/24/2021
Supervised By :Mahesh Dadoda 11/26/2021

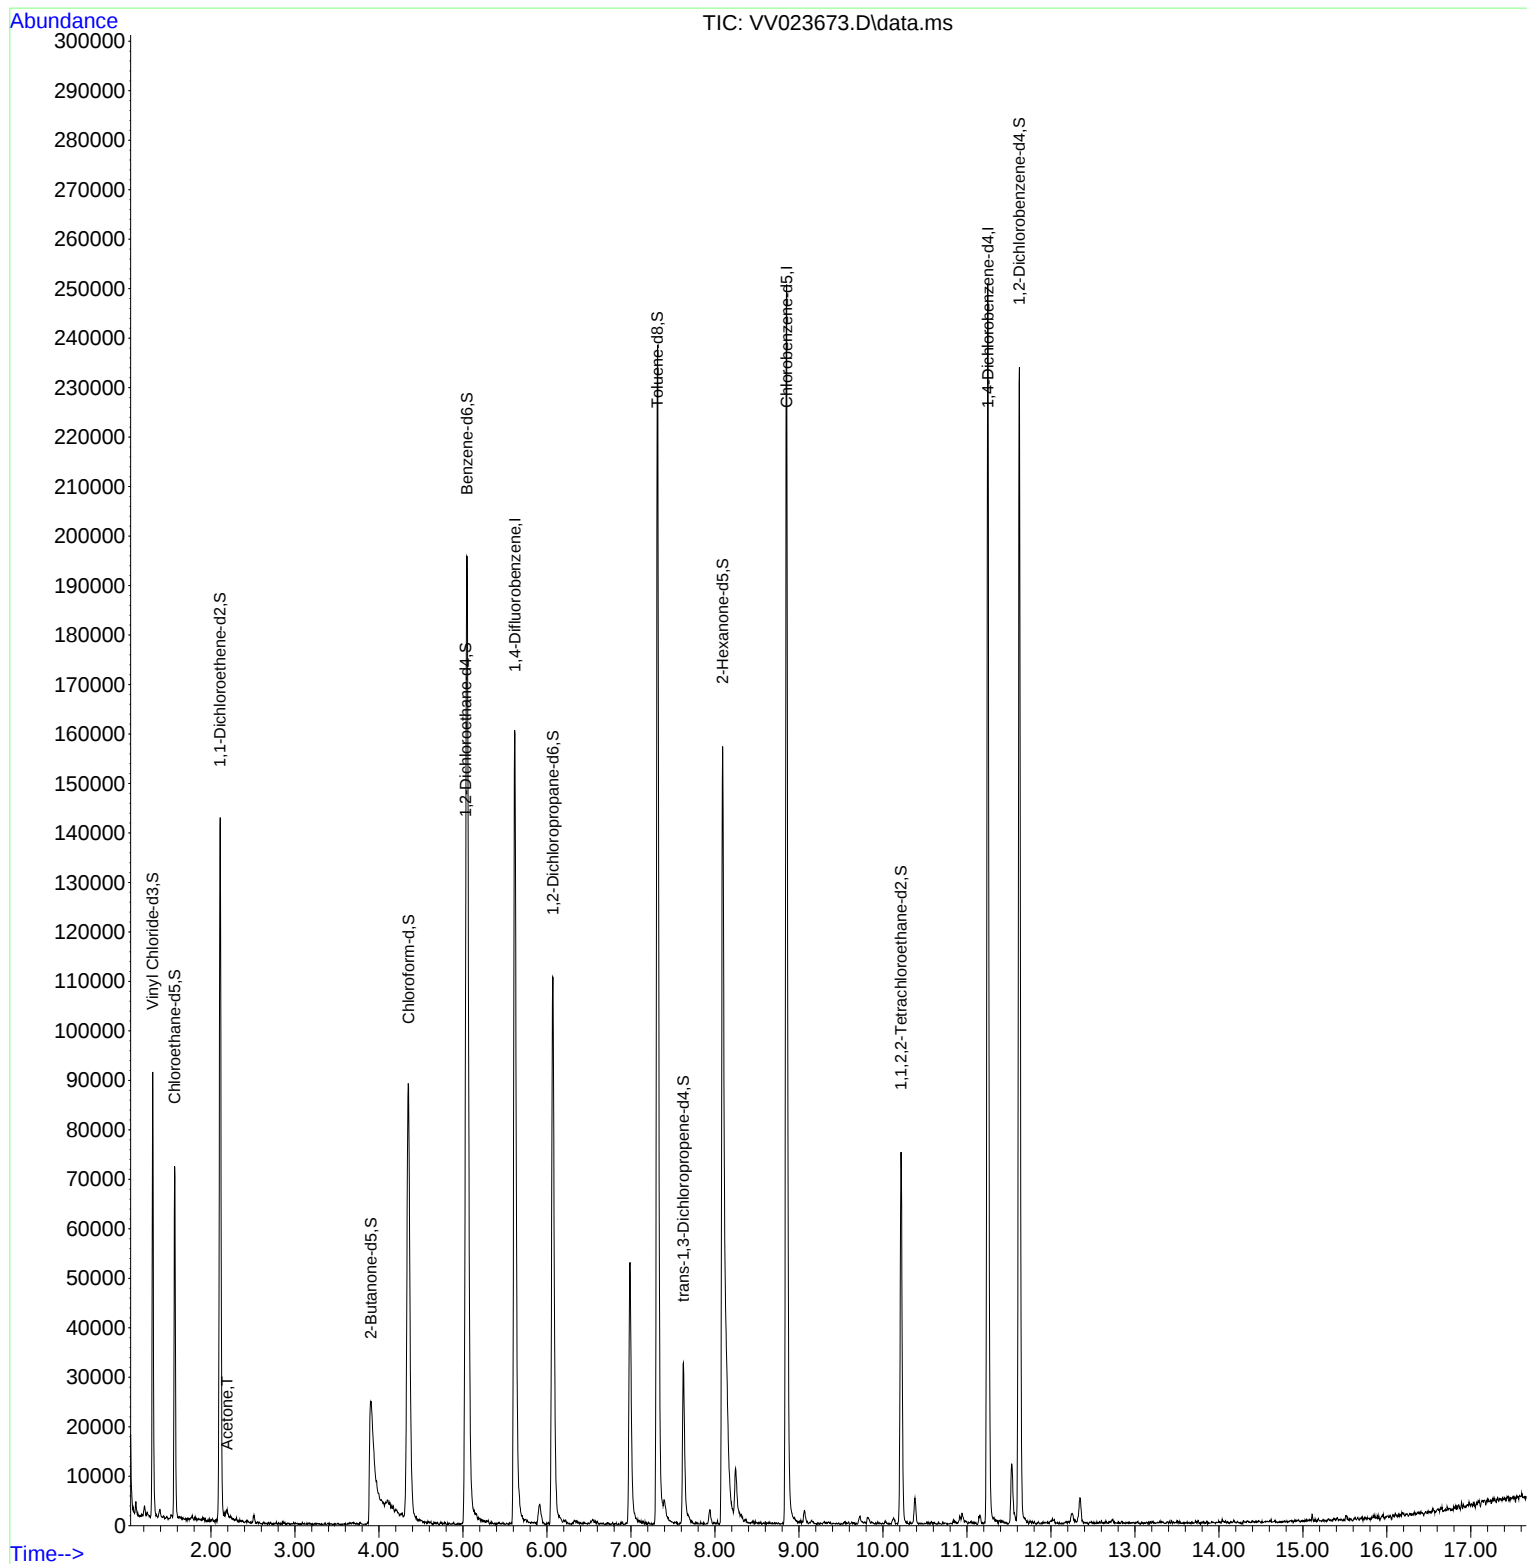

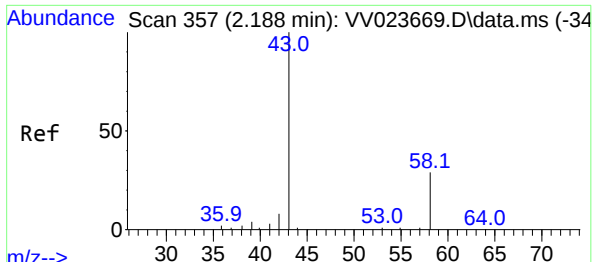

#13
Acetone
Concen: 4.305 ug/L m
RT: 2.192 min Scan# 3
Delta R.T. 0.003 min
Lab File: VV023673.D
Acq: 23 Nov 2021 16:08

Instrument :
MSVOA_V
ClientSampleId :
C0G07

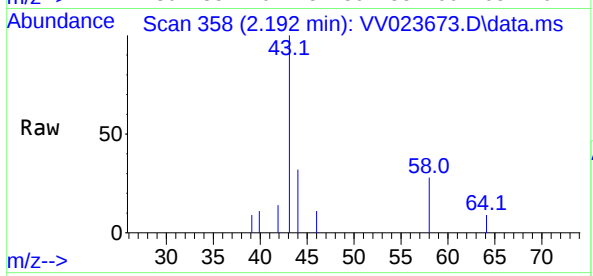

Tgt Ion: 43 Resp: 5528
Ion Ratio Lower Upper
43 100
58 14.9 0.0 41.4

Manual Integrations
APPROVED

Reviewed By :John Carlone 11/24/2021
Supervised By :Mahesh Dadoda 11/26/2021

