

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW112321\  
 Data File : VW023675.D  
 Acq On : 23 Nov 2021 16:55  
 Operator : SY/MD  
 Sample : M4723-07  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0G15

Manual Integrations  
 APPROVED

Reviewed By : John Carlone 11/24/2021  
 Supervised By : Mahesh Dadoda 11/26/2021

Quant Time: Nov 24 05:00:03 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Wed Nov 24 04:42:45 2021  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon           | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|--------|----------------|----------|--------|----------|----------|
| -----                         |        |                |          |        |          |          |
| Internal Standards            |        |                |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 5.619  | 114            | 134841   | 5.000  | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 8.854  | 117            | 135532   | 5.000  | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249 | 152            | 63887    | 5.000  | ug/L     | 0.00     |
|                               |        |                |          |        |          |          |
| System Monitoring Compounds   |        |                |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.307  | 65             | 51616    | 4.663  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 40 - 130 | Recovery | =      | 93.200%  |          |
| 7) Chloroethane-d5            | 1.568  | 69             | 42078    | 4.836  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 130 | Recovery | =      | 96.800%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.108  | 63             | 71123    | 3.646  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 125 | Recovery | =      | 73.000%  |          |
| 20) 2-Butanone-d5             | 3.912  | 46             | 59087    | 44.403 | ug/L     | 0.00     |
| Spiked Amount                 | 50.000 | Range 40 - 130 | Recovery | =      | 88.800%  |          |
| 24) Chloroform-d              | 4.352  | 84             | 94193    | 4.887  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 97.800%  |          |
| 26) 1,2-Dichloroethane-d4     | 5.034  | 65             | 43822    | 4.866  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 97.400%  |          |
| 32) Benzene-d6                | 5.050  | 84             | 180806   | 4.897  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 98.000%  |          |
| 36) 1,2-Dichloropropane-d6    | 6.069  | 67             | 51773    | 5.002  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 140 | Recovery | =      | 100.000% |          |
| 41) Toluene-d8                | 7.317  | 98             | 156731   | 4.543  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 90.800%  |          |
| 43) trans-1,3-Dichloroprop... | 7.625  | 79             | 20412    | 4.892  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 55 - 130 | Recovery | =      | 97.800%  |          |
| 46) 2-Hexanone-d5             | 8.092  | 63             | 65046    | 46.925 | ug/L     | 0.00     |
| Spiked Amount                 | 50.000 | Range 45 - 130 | Recovery | =      | 93.860%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217 | 84             | 34194    | 4.591  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 120 | Recovery | =      | 91.800%  |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.625 | 152            | 61718    | 5.464  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 80 - 120 | Recovery | =      | 109.200% |          |
|                               |        |                |          |        |          |          |
| Target Compounds              |        |                |          |        | Qvalue   |          |
| 13) Acetone                   | 2.201  | 43             | 4529m    | 3.782  | ug/L     |          |
| -----                         |        |                |          |        |          |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV112321\  
Data File : VV023675.D  
Acq On : 23 Nov 2021 16:55  
Operator : SY/MD  
Sample : M4723-07  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 15 Sample Multiplier: 1


Instrument :  
MSVOA\_V  
ClientSampleId :  
C0G15

Manual Integrations  
APPROVED

Reviewed By : John Carlone 11/24/2021  
Supervised By : Mahesh Dadoda 11/26/2021

Quant Time: Nov 24 05:00:03 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR112321WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Wed Nov 24 04:42:45 2021  
Response via : Initial Calibration

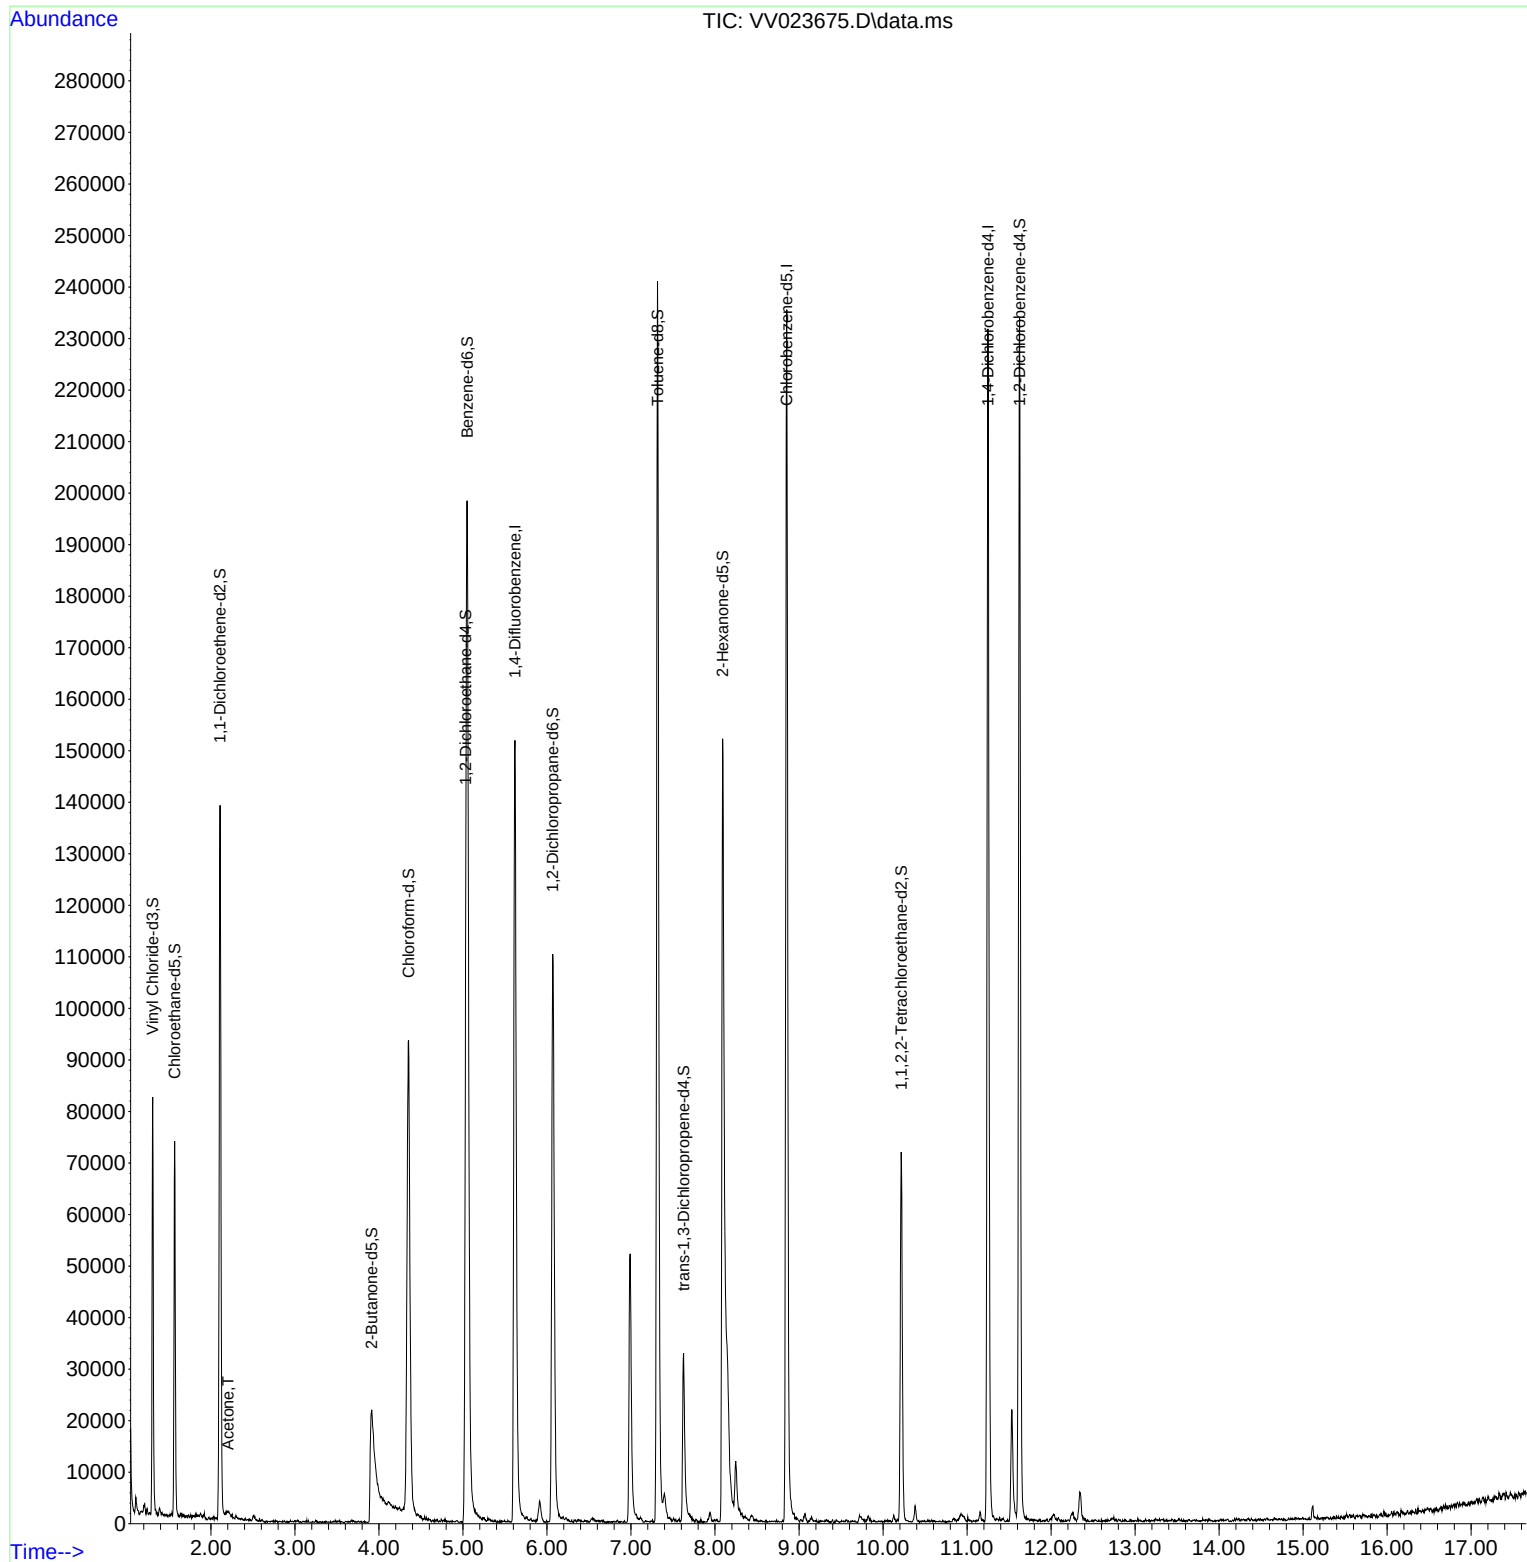

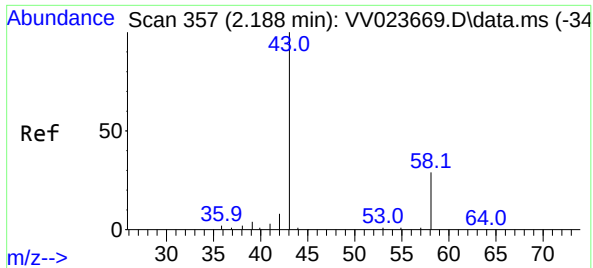

#13  
Acetone  
Concen: 3.782 ug/L m  
RT: 2.201 min Scan# 30  
Delta R.T. 0.013 min  
Lab File: VV023675.D  
Acq: 23 Nov 2021 16:55

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0G15

Tgt Ion: 43 Resp: 4529  
Ion Ratio Lower Upper  
43 100  
58 9.4 0.0 41.4

Manual Integrations  
APPROVED

Reviewed By :John Carlone 11/24/2021  
Supervised By :Mahesh Dadoda 11/26/2021

