

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112321\
 Data File : VW023678.D
 Acq On : 23 Nov 2021 18:07
 Operator : SY/MD
 Sample : M4723-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G23

Quant Time: Nov 24 05:00:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 04:42:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	133648	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	132101	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59846	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	51453	4.690	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.800%	
7) Chloroethane-d5	1.568	69	43220	5.012	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	100.200%	
11) 1,1-Dichloroethene-d2	2.108	63	72036	3.726	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	74.600%	
20) 2-Butanone-d5	3.892	46	91816	69.614	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	139.220%#	
24) Chloroform-d	4.349	84	94107	4.926	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.600%	
26) 1,2-Dichloroethane-d4	5.034	65	47393	5.310	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.200%	
32) Benzene-d6	5.053	84	184097	5.116	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.400%	
36) 1,2-Dichloropropane-d6	6.069	67	52824	5.236	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.800%	
41) Toluene-d8	7.317	98	158514	4.714	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.200%	
43) trans-1,3-Dichloroprop...	7.625	79	19744	4.855	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	97.200%	
46) 2-Hexanone-d5	8.088	63	67041	49.620	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	99.240%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	35333	4.867	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	60907	5.756	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	115.200%	
Target Compounds						
13) Acetone	2.188	43	1722	1.451	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
Data File : VV023678.D
Acq On : 23 Nov 2021 18:07
Operator : SY/MD
Sample : M4723-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G23

Quant Time: Nov 24 05:00:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 04:42:45 2021
Response via : Initial Calibration

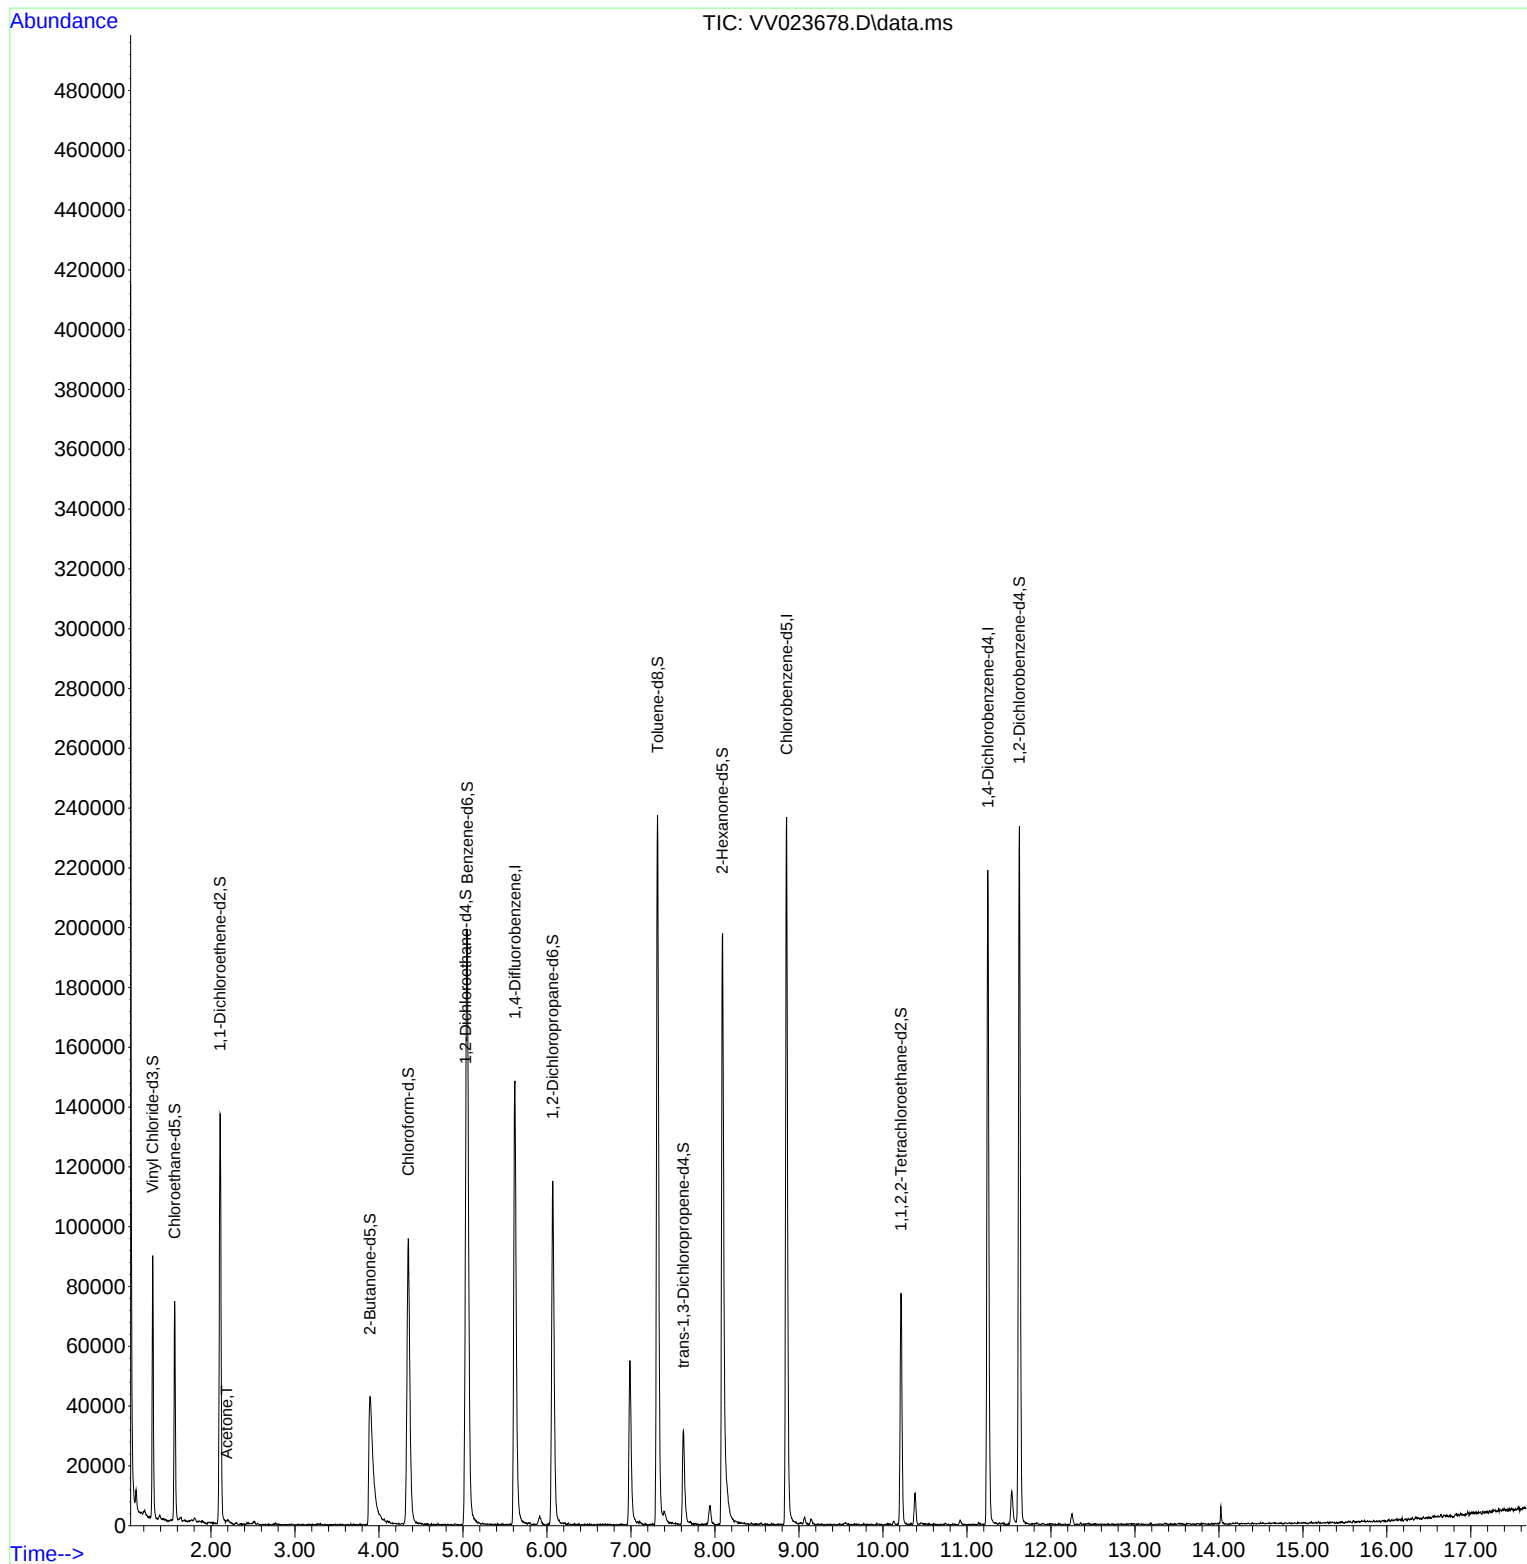

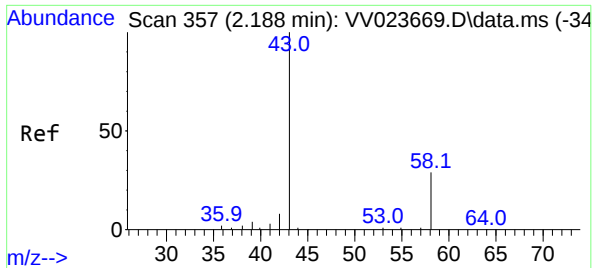

#13
Acetone
Concen: 1.451 ug/L
RT: 2.188 min Scan# 31
Delta R.T. 0.000 min
Lab File: VV023678.D
Acq: 23 Nov 2021 18:07

Instrument :
MSVOA_V
ClientSampleId :
C0G23

Tgt Ion: 43 Resp: 1722
Ion Ratio Lower Upper
43 100
58 15.9 0.0 41.4

