

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
 Data File : VV023672.D
 Acq On : 23 Nov 2021 15:44
 Operator : SY/MD
 Sample : M4723-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G06

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	98	rVB	92095	93779	17.83%	2.230%
2	1.568	154	164	175	rBV	76597	86101	16.37%	2.047%
3	2.108	321	332	348	rBV	146763	213994	40.68%	5.088%
4	3.905	881	891	933	rBV	32259	132632	25.21%	3.154%
5	4.349	1013	1029	1052	rBV	93590	234419	44.56%	5.574%
6	5.050	1227	1247	1270	rBV2	208772	526023	100.00%	12.507%
7	5.619	1412	1424	1446	rBV	153193	314849	59.85%	7.486%
8	5.915	1506	1516	1529	rBV8	4583	8802	1.67%	0.209%
9	6.069	1550	1564	1590	rBV	119240	246156	46.80%	5.853%
10	6.989	1836	1850	1873	rBV	57499	109706	20.86%	2.608%
11	7.317	1940	1952	1970	rBV	254369	445307	84.66%	10.588%
12	7.622	2039	2047	2070	rBV2	33435	64185	12.20%	1.526%
13	8.092	2183	2193	2231	rBV2	174537	402322	76.48%	9.566%
14	8.249	2234	2242	2248	rBV5	8356	12707	2.42%	0.302%
15	8.854	2414	2430	2454	rBV	239559	397377	75.54%	9.448%
16	10.217	2843	2854	2868	rVB	77847	122855	23.36%	2.921%
17	10.384	2891	2906	2917	rVB3	4237	7007	1.33%	0.167%
18	11.249	3162	3175	3195	rBV	228916	364057	69.21%	8.656%
19	11.532	3254	3263	3279	rBV2	16048	29015	5.52%	0.690%
20	11.625	3281	3292	3310	rVB	243911	385749	73.33%	9.172%
21	12.345	3504	3516	3526	rVB8	4769	8729	1.66%	0.208%




Sum of corrected areas: 4205771

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
Data File : VV023672.D
Acq On : 23 Nov 2021 15:44
Operator : SY/MD
Sample : M4723-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

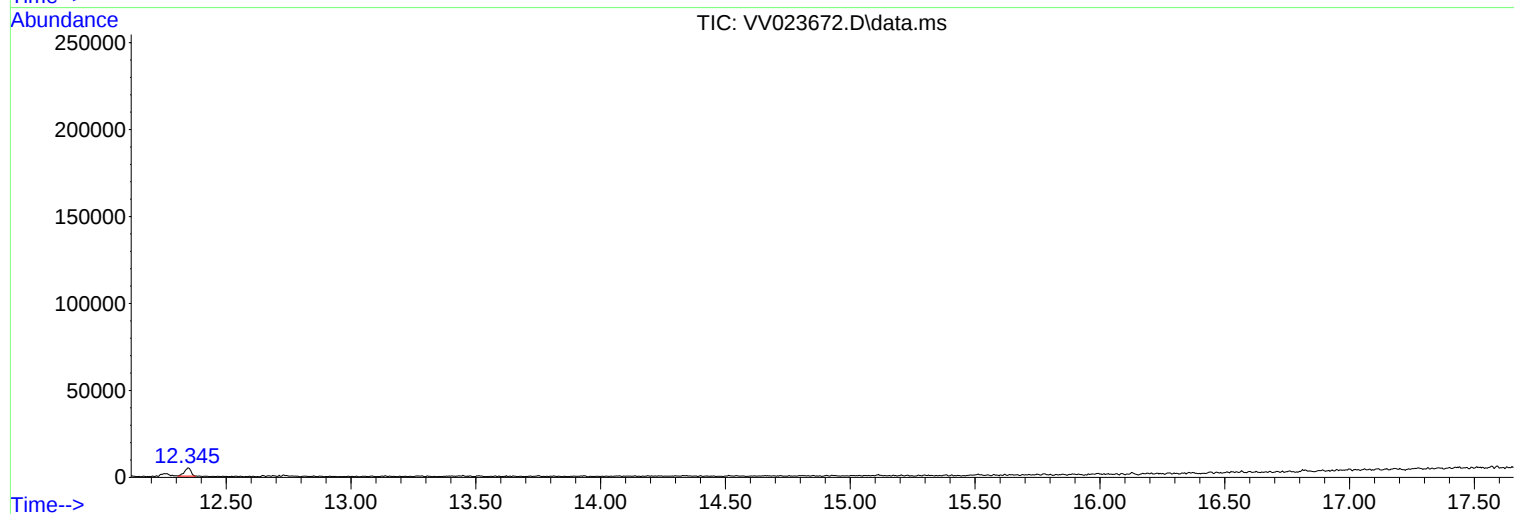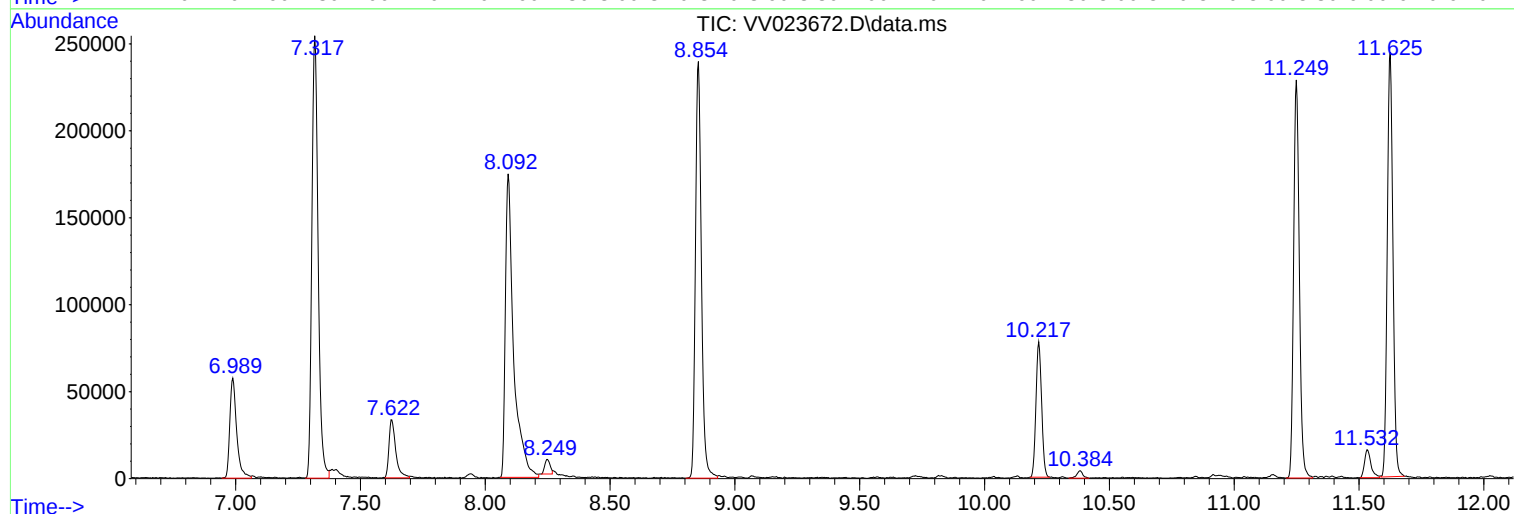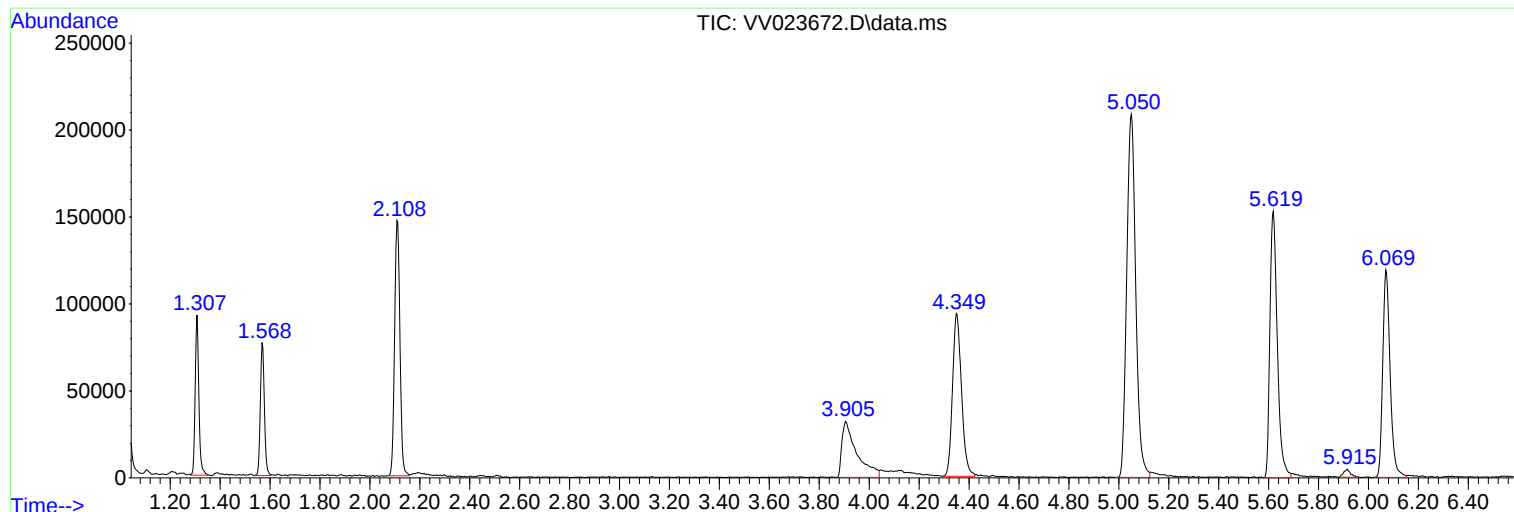

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
Data File : VV023672.D
Acq On : 23 Nov 2021 15:44
Operator : SY/MD
Sample : M4723-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112321\
Data File : VV023672.D
Acq On : 23 Nov 2021 15:44
Operator : SY/MD
Sample : M4723-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
